




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025968.D
 Acq On : 26 May 2022 19:10
 Operator : SY/MD
 Sample : N3039-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 27 01:31:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
 Supervised By :Mahesh Dadoda 05/27/2022

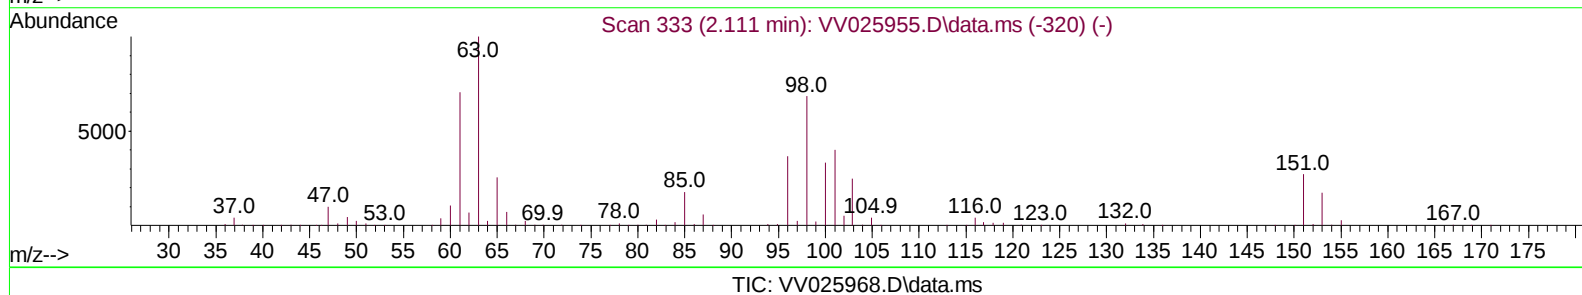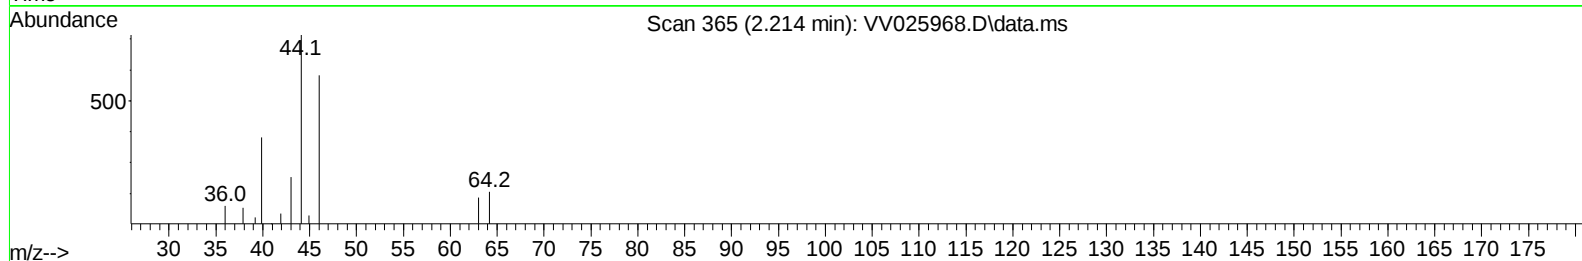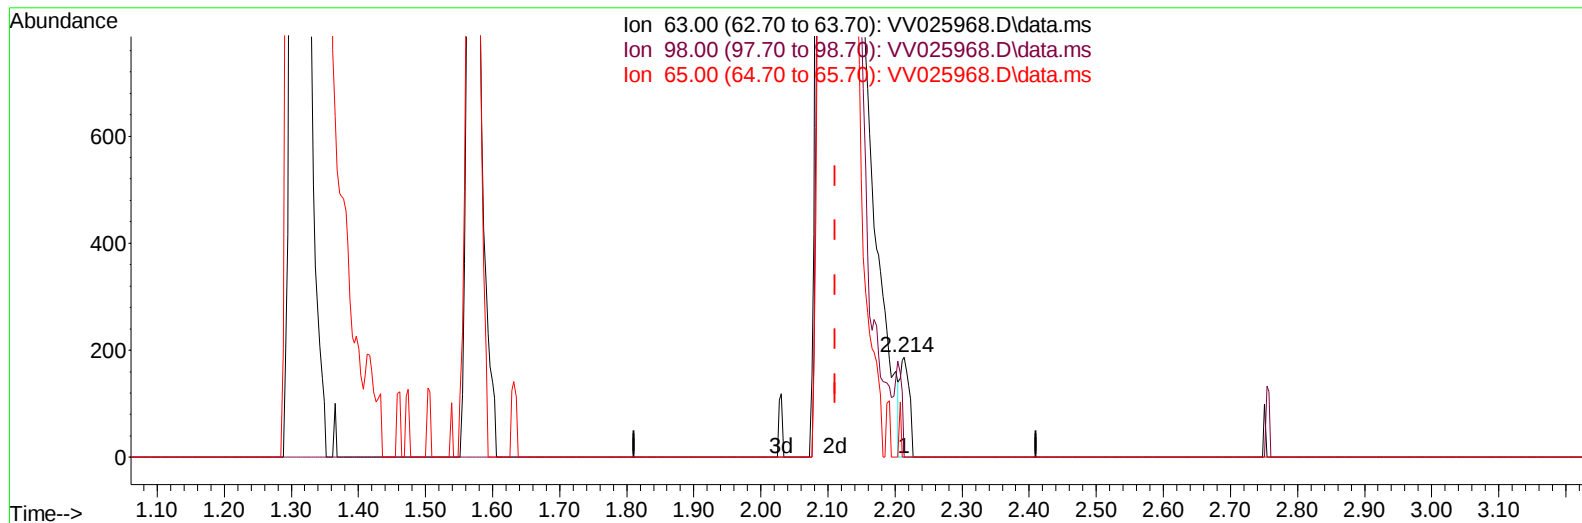

(11) 1,1-Dichloroethene-d2 (S)

2.214min (+ 0.103) 0.04 ug/L

response 177

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.70	78.53
65.00	24.30	22.60
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025968.D
 Acq On : 26 May 2022 19:10
 Operator : SY/MD
 Sample : N3039-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 27 01:31:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
 Supervised By :Mahesh Dadoda 05/27/2022

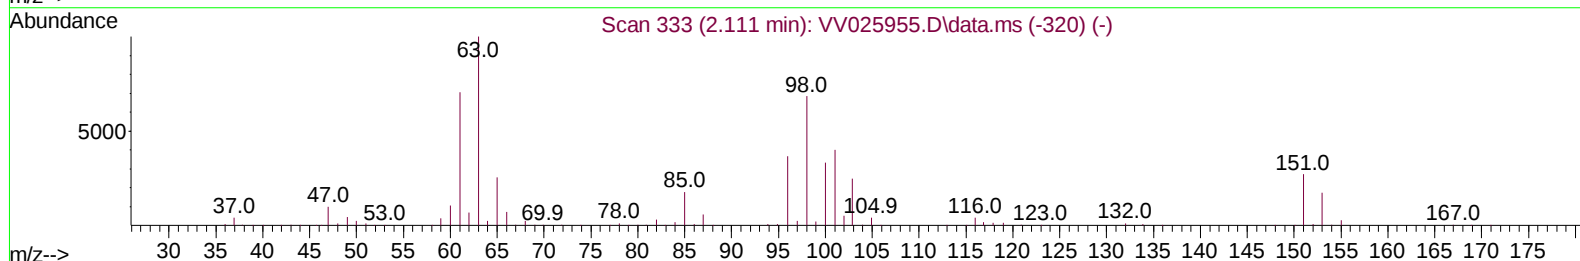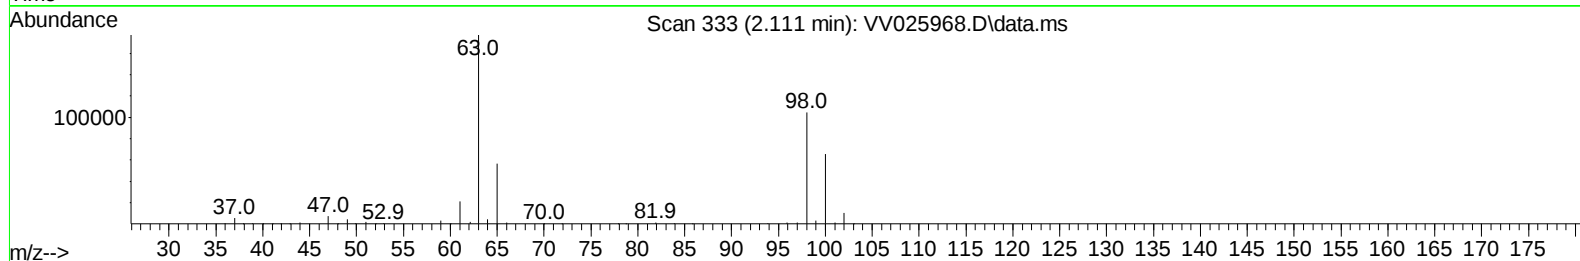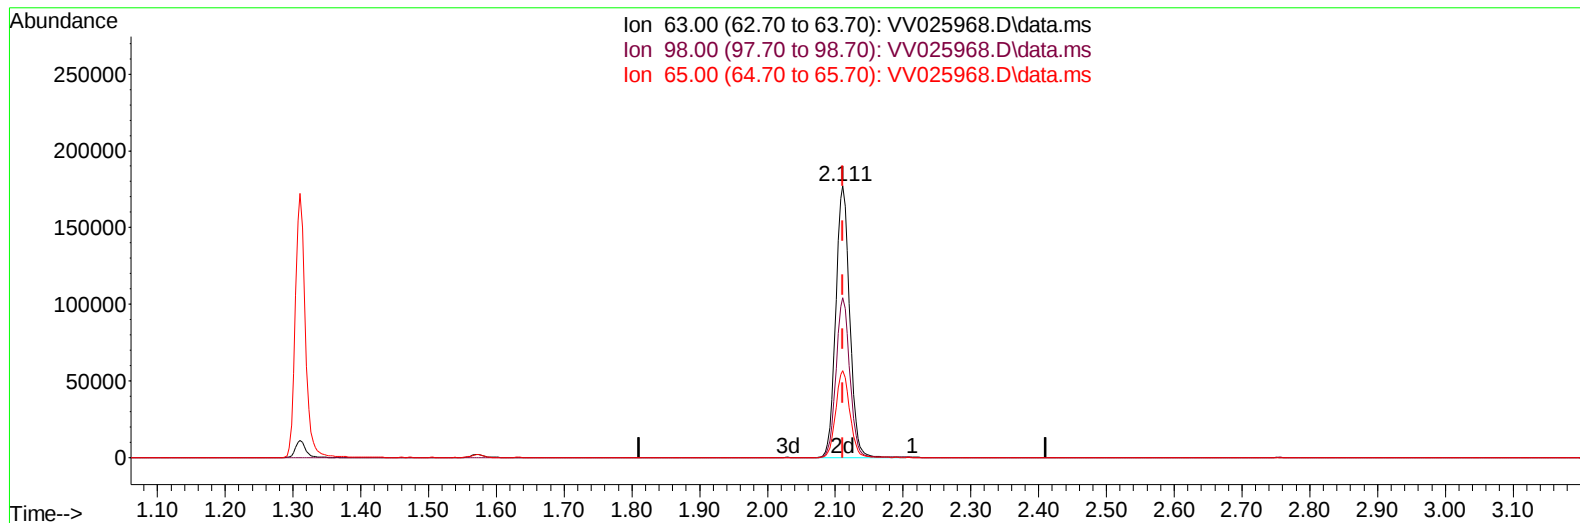

TIC: VV025968.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.111min (+ 0.000) 54.19 ug/L m

response 249938

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.70	0.06#
65.00	24.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025968.D
 Acq On : 26 May 2022 19:10
 Operator : SY/MD
 Sample : N3039-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 27 01:31:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	204346	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	204812	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	87119	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	176072	66.763	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	133.520%	
7) Chloroethane-d5	1.571	69	146419	63.220	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	126.440%	
11) 1,1-Dichloroethene-d2	2.111	63	249938m	54.187	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	108.380%	
21) 2-Butanone-d5	3.905	46	122502	108.374	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	108.370%	
24) Chloroform-d	4.349	84	262444	71.247	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	142.500%#	
26) 1,2-Dichloroethane-d4	5.034	65	165494	74.338	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	148.680%#	
32) Benzene-d6	5.050	84	535942	75.061	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	150.120%#	
36) 1,2-Dichloropropane-d6	6.069	67	171467	78.189	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	156.380%#	
41) Toluene-d8	7.317	98	449783	68.370	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	136.740%#	
43) trans-1,3-Dichloroprop...	7.622	79	62112	63.449	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	126.900%#	
47) 2-Hexanone-d5	8.091	63	103172	128.323	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	128.320%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	213252	72.919	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	145.840%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	156760	82.030	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	164.060%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025968.D
Acq On : 26 May 2022 19:10
Operator : SY/MD
Sample : N3039-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 27 01:31:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 27 01:28:09 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
Supervised By :Mahesh Dadoda 05/27/2022

