

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025956.D
 Acq On : 26 May 2022 14:20
 Operator : SY/MD
 Sample : VV0526WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB	301383	309928	19.03%	2.675%
2	1.571	157	165	182	rBV	242197	272955	16.76%	2.356%
3	2.108	322	332	356	rVB	515410	734295	45.08%	6.339%
4	2.477	444	447	448	rBV2	456	279	0.02%	0.002%
5	2.506	449	456	466	rVB3	5537	8950	0.55%	0.077%
6	2.606	484	487	488	rBV	706	431	0.03%	0.004%
7	2.658	501	503	504	rBV	318	160	0.01%	0.001%
8	2.709	517	519	521	rBV	243	151	0.01%	0.001%
9	2.754	530	533	536	rBV	411	313	0.02%	0.003%
10	2.799	545	547	550	rBV	364	199	0.01%	0.002%
11	2.850	561	563	566	rBV	321	144	0.01%	0.001%
12	2.998	607	609	611	rVB	419	187	0.01%	0.002%
13	3.204	667	673	677	rBV2	351	319	0.02%	0.003%
14	3.265	689	692	694	rVV	150	86	0.01%	0.001%
15	3.281	694	697	702	rVB2	270	265	0.02%	0.002%
16	3.355	717	720	722	rBV	272	165	0.01%	0.001%
17	3.397	731	733	738	rVB2	276	123	0.01%	0.001%
18	3.423	738	741	745	rBV2	195	176	0.01%	0.002%
19	3.542	774	778	783	rBV3	239	185	0.01%	0.002%
20	3.567	783	786	787	rBV	199	90	0.01%	0.001%
21	3.606	796	798	802	rBV	136	85	0.01%	0.001%
22	3.783	851	853	856	rVB	322	170	0.01%	0.001%
23	3.802	856	859	861	rBV2	150	90	0.01%	0.001%
24	3.821	863	865	867	rBV	272	123	0.01%	0.001%
25	3.902	879	890	930	rBV2	61693	276260	16.96%	2.385%
26	4.346	1013	1028	1054	rBV	259774	636619	39.09%	5.496%
27	4.702	1136	1139	1140	rBV	201	120	0.01%	0.001%
28	4.712	1140	1142	1144	rVV2	485	276	0.02%	0.002%
29	4.751	1148	1154	1155	rBV2	283	293	0.02%	0.003%
30	4.802	1167	1170	1171	rBV2	208	125	0.01%	0.001%
31	4.844	1182	1183	1186	rBV2	311	163	0.01%	0.001%
32	4.902	1198	1201	1202	rBV2	249	143	0.01%	0.001%
33	4.918	1204	1206	1207	rVB2	327	98	0.01%	0.001%
34	4.937	1207	1212	1213	rBV2	353	242	0.01%	0.002%
35	4.985	1223	1227	1228	rBV	319	178	0.01%	0.002%
36	5.043	1228	1245	1287	rVV2	634451	1628766	100.00%	14.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025956.D
 Acq On : 26 May 2022 14:20
 Operator : SY/MD
 Sample : VV0526WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.471	1377	1378	1381	rBV	309	116	0.01%	0.001%
38	5.497	1381	1386	1387	rBV3	429	328	0.02%	0.003%
39	5.551	1401	1403	1404	rBV	234	98	0.01%	0.001%
40	5.564	1404	1407	1408	rVV	339	132	0.01%	0.001%
41	5.612	1410	1422	1456	rBV	399728	812714	49.90%	7.016%
42	5.805	1480	1482	1484	rBV2	643	324	0.02%	0.003%
43	5.911	1503	1515	1525	rBV3	11877	25988	1.60%	0.224%
44	5.985	1536	1538	1539	rBV3	516	208	0.01%	0.002%
45	6.066	1547	1563	1595	rBV	353995	731599	44.92%	6.315%
46	6.313	1636	1640	1642	rBV3	616	448	0.03%	0.004%
47	6.342	1648	1649	1652	rBV	232	94	0.01%	0.001%
48	6.397	1662	1666	1670	rVB2	512	425	0.03%	0.004%
49	6.448	1677	1682	1685	rBV	430	401	0.02%	0.003%
50	6.481	1690	1692	1695	rVB	253	94	0.01%	0.001%
51	6.522	1700	1705	1706	rBV2	254	219	0.01%	0.002%
52	6.548	1711	1713	1714	rBV2	233	98	0.01%	0.001%
53	6.587	1722	1725	1728	rBV2	167	111	0.01%	0.001%
54	6.603	1728	1730	1731	rBV2	282	83	0.01%	0.001%
55	6.648	1741	1744	1746	rBV2	399	264	0.02%	0.002%
56	6.715	1763	1765	1772	rVB2	521	355	0.02%	0.003%
57	6.751	1772	1776	1777	rBV	252	159	0.01%	0.001%
58	6.825	1795	1799	1800	rBV	369	171	0.01%	0.001%
59	6.895	1818	1821	1822	rBV	172	99	0.01%	0.001%
60	6.921	1826	1829	1830	rBV2	144	92	0.01%	0.001%
61	6.982	1837	1848	1872	rBV	161911	301665	18.52%	2.604%
62	7.313	1939	1951	1972	rBV	737079	1268522	77.88%	10.950%
63	7.619	2036	2046	2074	rBV	114099	204412	12.55%	1.765%
64	7.870	2120	2124	2128	rVB4	784	586	0.04%	0.005%
65	8.088	2180	2192	2234	rBV	278612	602567	37.00%	5.202%
66	8.371	2279	2280	2284	rBV4	533	318	0.02%	0.003%
67	8.474	2310	2312	2314	rVB	463	168	0.01%	0.001%
68	8.509	2314	2323	2329	rBV6	651	1053	0.06%	0.009%
69	8.535	2329	2331	2334	rBV2	323	199	0.01%	0.002%
70	8.670	2372	2373	2375	rBV	211	113	0.01%	0.001%
71	8.702	2379	2383	2388	rBV3	385	309	0.02%	0.003%
72	8.850	2417	2429	2452	rBV	623462	1020837	62.68%	8.812%
73	9.146	2516	2521	2522	rBV2	642	440	0.03%	0.004%
74	9.220	2540	2544	2549	rVB3	451	433	0.03%	0.004%
75	9.265	2556	2558	2559	rBV	225	96	0.01%	0.001%
76	9.361	2582	2588	2590	rBV	273	213	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025956.D
 Acq On : 26 May 2022 14:20
 Operator : SY/MD
 Sample : VV0526WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.378	2591	2593	2595	rBV2	340	125	0.01%	0.001%
78	9.464	2618	2620	2623	rBV2	258	135	0.01%	0.001%
79	9.506	2630	2633	2635	rBV	334	249	0.02%	0.002%
80	9.535	2639	2642	2644	rBV2	254	161	0.01%	0.001%
81	9.551	2644	2647	2649	rBV2	478	297	0.02%	0.003%
82	9.612	2663	2666	2670	rBV	466	332	0.02%	0.003%
83	9.657	2677	2680	2681	rBV	252	131	0.01%	0.001%
84	9.731	2701	2703	2704	rBV	241	99	0.01%	0.001%
85	9.815	2726	2729	2730	rBV	291	155	0.01%	0.001%
86	9.934	2764	2766	2768	rVB	749	228	0.01%	0.002%
87	10.123	2816	2825	2835	rBV4	4066	6026	0.37%	0.052%
88	10.214	2841	2853	2877	rBV	444666	700732	43.02%	6.049%
89	10.400	2910	2911	2914	rBV2	193	112	0.01%	0.001%
90	10.683	2997	2999	3005	rBV2	362	286	0.02%	0.002%
91	10.840	3046	3048	3050	rBV	414	211	0.01%	0.002%
92	10.914	3066	3071	3081	rVB7	2475	3580	0.22%	0.031%
93	11.146	3137	3143	3148	rVB6	1112	1543	0.09%	0.013%
94	11.246	3163	3174	3193	rBV	608420	944300	57.98%	8.152%
95	11.496	3248	3252	3256	rBV2	580	578	0.04%	0.005%
96	11.622	3279	3291	3315	rBV	694656	1074365	65.96%	9.274%
97	11.831	3354	3356	3357	rBV2	358	152	0.01%	0.001%
98	12.644	3607	3609	3610	rBV2	468	204	0.01%	0.002%
99	12.969	3708	3710	3714	rBV2	425	274	0.02%	0.002%
100	13.217	3784	3787	3788	rBV2	519	311	0.02%	0.003%




Sum of corrected areas: 11584289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025956.D
Acq On : 26 May 2022 14:20
Operator : SY/MD
Sample : VV0526WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

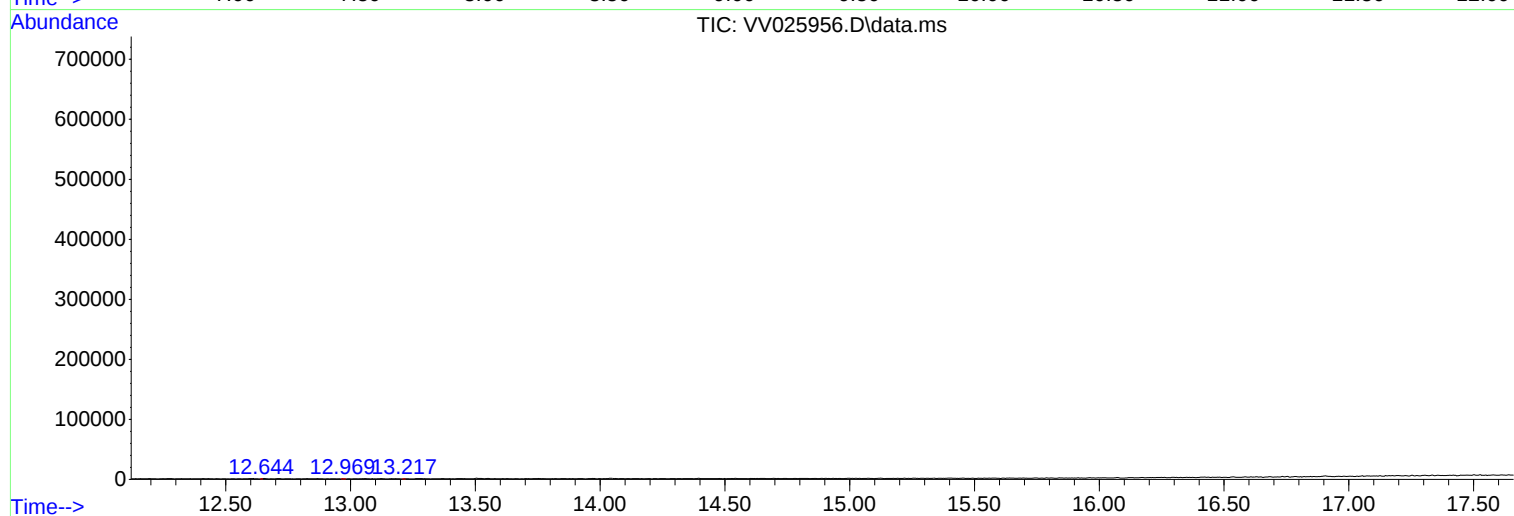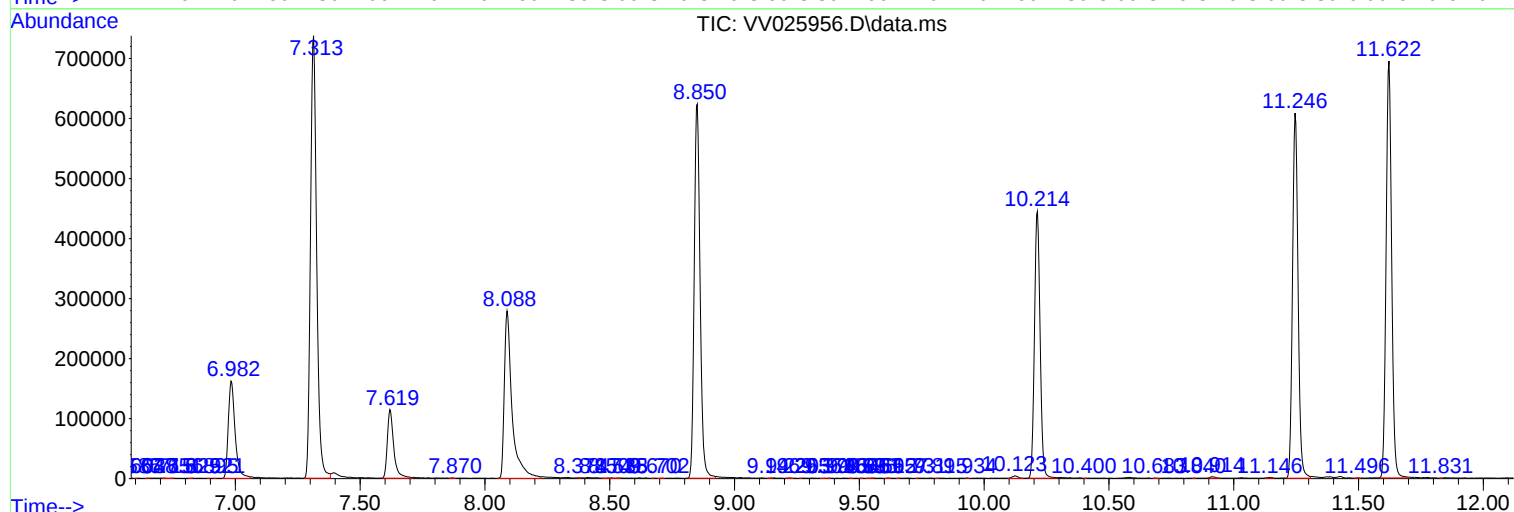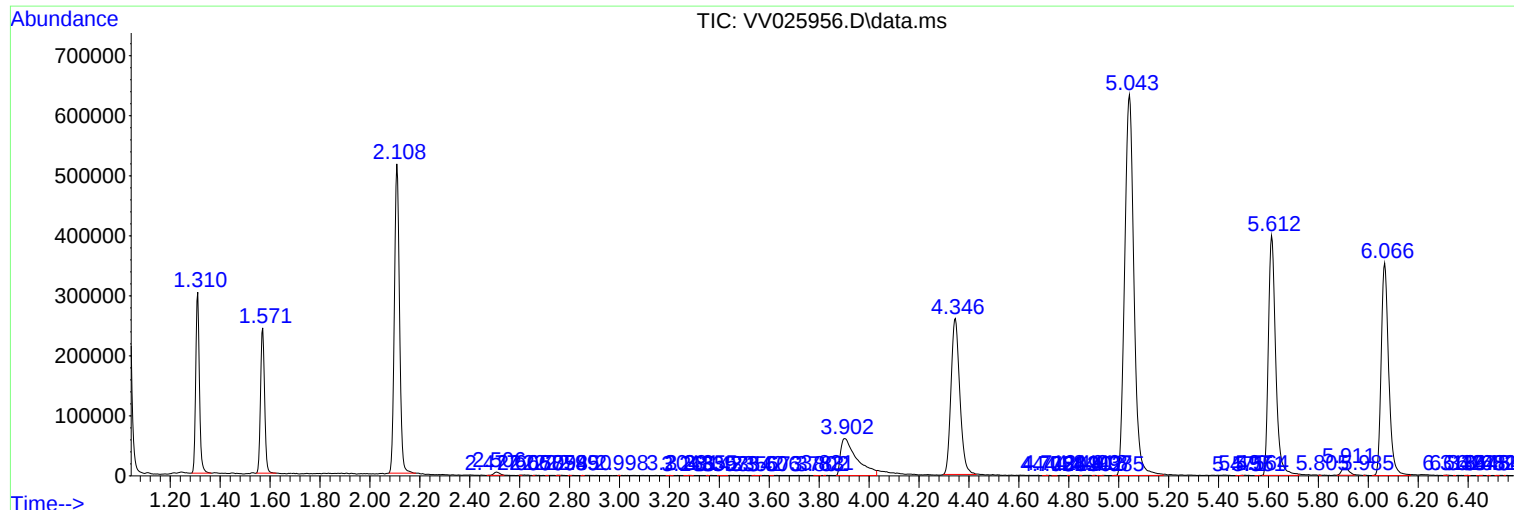

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025956.D
Acq On : 26 May 2022 14:20
Operator : SY/MD
Sample : VV0526WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025956.D
Acq On : 26 May 2022 14:20
Operator : SY/MD
Sample : VV0526WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------