

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	104	rVB	283957	290371	18.99%	2.601%
2	1.571	158	165	179	rVB	232424	261640	17.11%	2.344%
3	2.108	323	332	351	rBV	481303	686464	44.89%	6.150%
4	2.375	413	415	418	rBV3	680	423	0.03%	0.004%
5	2.510	448	457	469	rBV8	2066	3369	0.22%	0.030%
6	2.761	533	535	536	rBV8	456	186	0.01%	0.002%
7	2.828	553	556	559	rBV2	278	165	0.01%	0.001%
8	2.876	567	571	575	rVB3	282	245	0.02%	0.002%
9	2.899	575	578	583	rBV2	285	241	0.02%	0.002%
10	2.931	583	588	591	rVB2	371	317	0.02%	0.003%
11	3.024	612	617	619	rBV2	350	220	0.01%	0.002%
12	3.066	628	630	634	rVB2	325	201	0.01%	0.002%
13	3.095	634	639	640	rBV2	255	193	0.01%	0.002%
14	3.150	653	656	659	rBV	281	212	0.01%	0.002%
15	3.198	668	671	674	rVB2	253	147	0.01%	0.001%
16	3.397	731	733	735	rBV	283	172	0.01%	0.002%
17	3.468	752	755	759	rVB3	303	228	0.01%	0.002%
18	3.503	765	766	769	rVB	352	135	0.01%	0.001%
19	3.529	769	774	777	rBV2	379	328	0.02%	0.003%
20	3.580	786	790	793	rBV2	215	224	0.01%	0.002%
21	3.593	793	794	801	rVB2	371	276	0.02%	0.002%
22	3.635	801	807	809	rBV2	182	204	0.01%	0.002%
23	3.786	850	854	858	rBV2	273	187	0.01%	0.002%
24	3.818	861	864	866	rVV2	252	144	0.01%	0.001%
25	3.905	877	891	943	rBV	56272	271320	17.74%	2.431%
26	4.349	1014	1029	1053	rBV	246077	604035	39.50%	5.411%
27	4.648	1120	1122	1125	rVB4	523	313	0.02%	0.003%
28	4.670	1125	1129	1133	rBV3	369	360	0.02%	0.003%
29	4.722	1142	1145	1150	rVB3	512	455	0.03%	0.004%
30	4.796	1164	1168	1171	rBV2	620	408	0.03%	0.004%
31	4.838	1177	1181	1184	rVB2	290	151	0.01%	0.001%
32	4.912	1202	1204	1206	rBV2	306	167	0.01%	0.001%
33	4.931	1208	1210	1214	rBV3	217	145	0.01%	0.001%
34	4.950	1214	1216	1221	rVB	367	183	0.01%	0.002%
35	4.973	1221	1223	1226	rBV2	299	180	0.01%	0.002%
36	5.043	1228	1245	1275	rBV2	597838	1529319	100.00%	13.701%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.342	1336	1338	1340	rVB2	457	156	0.01%	0.001%
38	5.359	1340	1343	1345	rBV	323	236	0.02%	0.002%
39	5.452	1370	1372	1375	rBV2	327	172	0.01%	0.002%
40	5.487	1381	1383	1386	rVB2	382	166	0.01%	0.001%
41	5.503	1386	1388	1393	rVB3	507	276	0.02%	0.002%
42	5.526	1393	1395	1399	rVB2	475	224	0.01%	0.002%
43	5.568	1406	1408	1410	rVB	470	196	0.01%	0.002%
44	5.616	1410	1423	1453	rBV	395748	808404	52.86%	7.242%
45	5.908	1504	1514	1530	rBV4	14070	29776	1.95%	0.267%
46	6.069	1550	1564	1592	rBV	335630	698387	45.67%	6.257%
47	6.204	1604	1606	1608	rBV3	845	494	0.03%	0.004%
48	6.320	1640	1642	1646	rVB2	484	248	0.02%	0.002%
49	6.349	1646	1651	1653	rBV2	290	269	0.02%	0.002%
50	6.423	1672	1674	1679	rVB3	327	269	0.02%	0.002%
51	6.449	1679	1682	1685	rVB3	608	359	0.02%	0.003%
52	6.484	1690	1693	1695	rBV2	294	159	0.01%	0.001%
53	6.722	1765	1767	1769	rVV2	421	215	0.01%	0.002%
54	6.748	1772	1775	1778	rVB2	239	157	0.01%	0.001%
55	6.822	1795	1798	1803	rBV2	331	281	0.02%	0.003%
56	6.850	1803	1807	1808	rBV	235	168	0.01%	0.002%
57	6.985	1838	1849	1868	rBV	152970	283275	18.52%	2.538%
58	7.169	1904	1906	1910	rVB3	710	380	0.02%	0.003%
59	7.239	1927	1928	1930	rBV2	243	138	0.01%	0.001%
60	7.313	1940	1951	1971	rBV	684682	1191369	77.90%	10.673%
61	7.622	2037	2047	2076	rBV	105786	192209	12.57%	1.722%
62	7.866	2121	2123	2128	rBV4	395	341	0.02%	0.003%
63	7.937	2135	2145	2156	rBV3	14100	24250	1.59%	0.217%
64	8.088	2183	2192	2236	rBV	251196	549819	35.95%	4.926%
65	8.619	2354	2357	2361	rVB2	522	391	0.03%	0.004%
66	8.638	2361	2363	2366	rVB3	413	152	0.01%	0.001%
67	8.667	2369	2372	2373	rBV2	538	352	0.02%	0.003%
68	8.850	2416	2429	2455	rBV	628348	1025246	67.04%	9.185%
69	9.095	2502	2505	2509	rBV5	634	466	0.03%	0.004%
70	9.188	2532	2534	2537	rBV	394	172	0.01%	0.002%
71	9.204	2537	2539	2542	rBV2	318	180	0.01%	0.002%
72	9.262	2552	2557	2559	rBV2	349	233	0.02%	0.002%
73	9.275	2559	2561	2564	rVV	329	143	0.01%	0.001%
74	9.342	2581	2582	2586	rBV2	331	197	0.01%	0.002%
75	9.426	2603	2608	2610	rBV2	371	350	0.02%	0.003%
76	9.545	2640	2645	2648	rBV2	598	480	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052622\
 Data File : VW025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.690	2688	2690	2694	rBV	291	190	0.01%	0.002%
78	9.809	2725	2727	2735	rVB2	459	342	0.02%	0.003%
79	9.882	2748	2750	2755	rVB3	525	267	0.02%	0.002%
80	10.014	2788	2791	2793	rBV2	377	249	0.02%	0.002%
81	10.127	2816	2826	2834	rBV3	3505	4679	0.31%	0.042%
82	10.159	2834	2836	2840	rBV3	240	172	0.01%	0.002%
83	10.214	2841	2853	2871	rBV	415369	654524	42.80%	5.864%
84	10.384	2897	2906	2916	rVB3	12603	19551	1.28%	0.175%
85	10.461	2927	2930	2934	rBV3	262	250	0.02%	0.002%
86	10.497	2937	2941	2947	rBV2	494	499	0.03%	0.004%
87	10.529	2948	2951	2955	rVB2	474	273	0.02%	0.002%
88	10.558	2958	2960	2962	rBV	517	312	0.02%	0.003%
89	10.690	2996	3001	3005	rBV3	423	388	0.03%	0.003%
90	10.799	3032	3035	3038	rVB2	544	321	0.02%	0.003%
91	10.873	3057	3058	3061	rBV	324	149	0.01%	0.001%
92	11.143	3136	3142	3145	rBV6	1521	1842	0.12%	0.017%
93	11.246	3163	3174	3196	rBV	599068	927164	60.63%	8.306%
94	11.529	3253	3262	3280	rBV	27166	50193	3.28%	0.450%
95	11.622	3280	3291	3311	rVV	660145	1018331	66.59%	9.123%
96	12.095	3433	3438	3442	rBV3	1218	1126	0.07%	0.010%
97	12.249	3478	3486	3495	rBV2	2762	4306	0.28%	0.039%
98	12.345	3508	3516	3527	rBV4	8127	12635	0.83%	0.113%
99	12.423	3538	3540	3542	rVB2	360	156	0.01%	0.001%
100	12.921	3693	3695	3699	rBV	346	198	0.01%	0.002%




Sum of corrected areas: 11162200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025957.D
Acq On : 26 May 2022 14:48
Operator : SY/MD
Sample : N3039-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

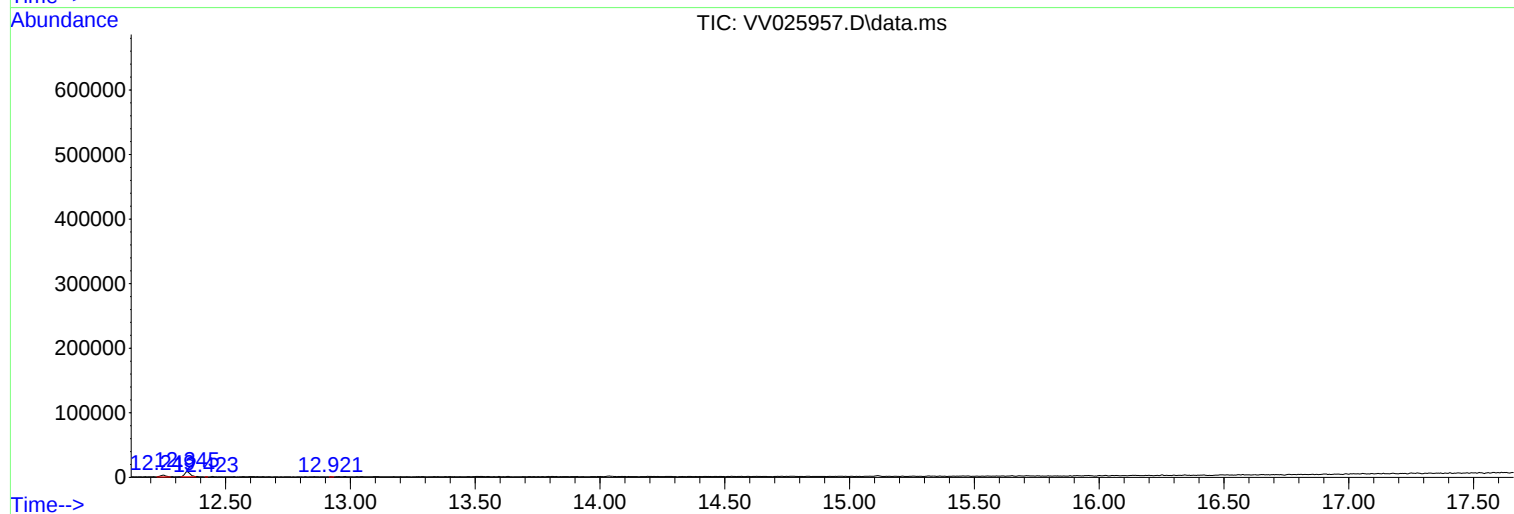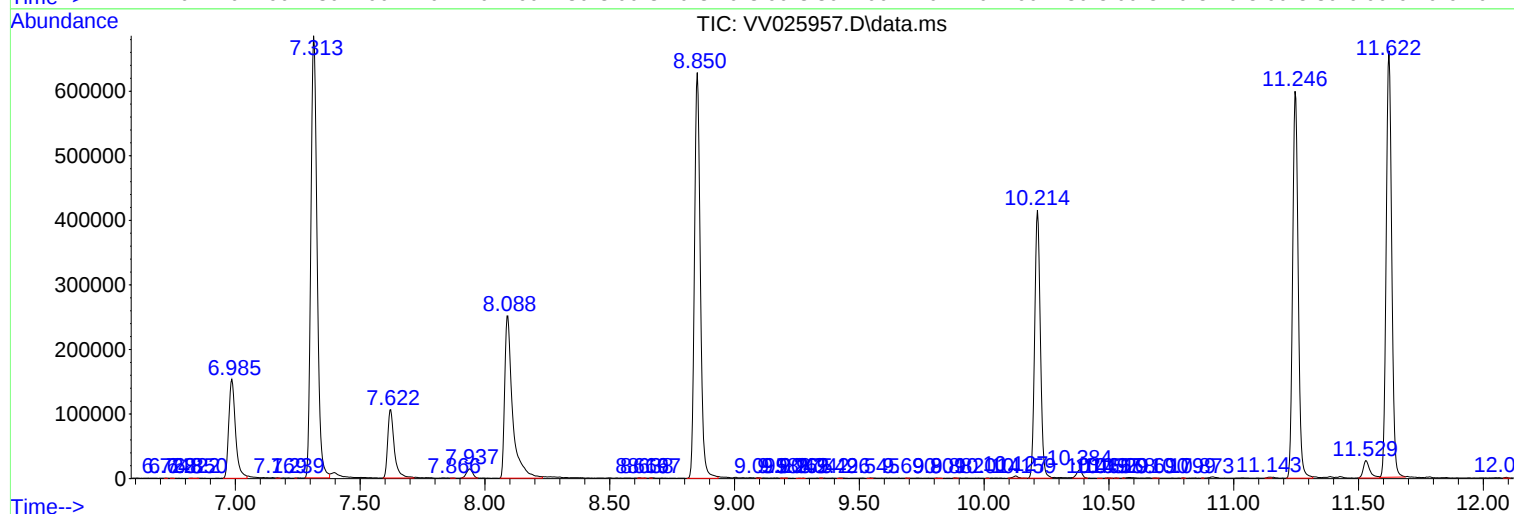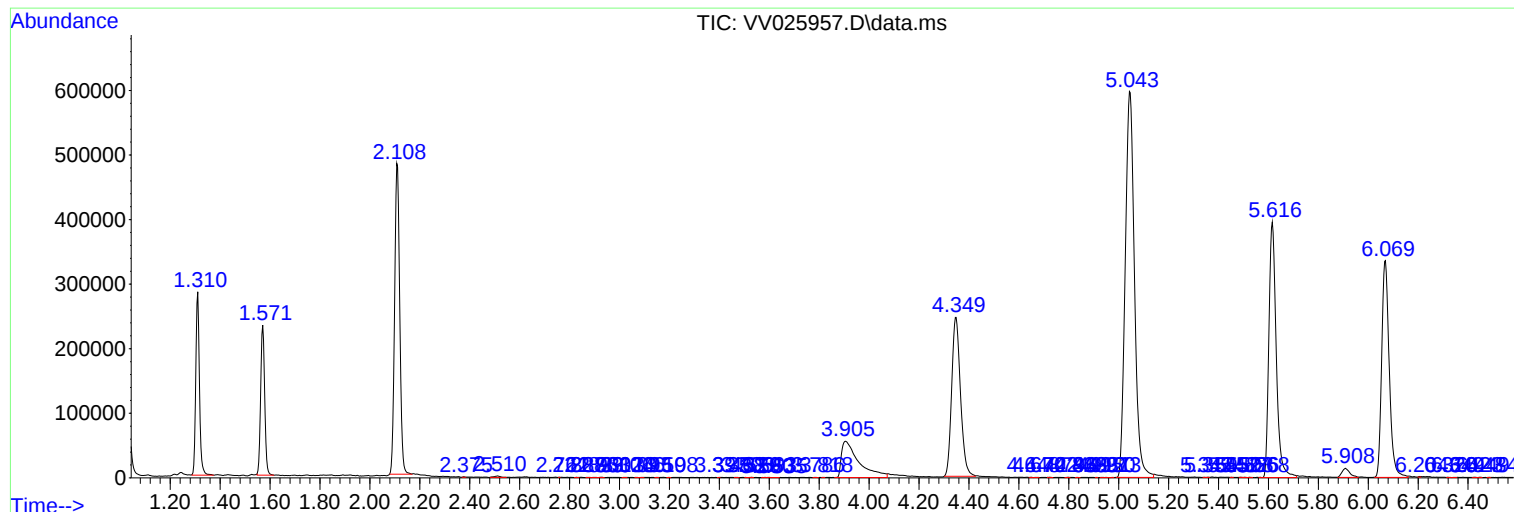

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025957.D
Acq On : 26 May 2022 14:48
Operator : SY/MD
Sample : N3039-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JR7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.529	2.71 ug/L	50193	1,4-Dichlorobenzene-d4	11.246

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	83
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	83
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
5	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64

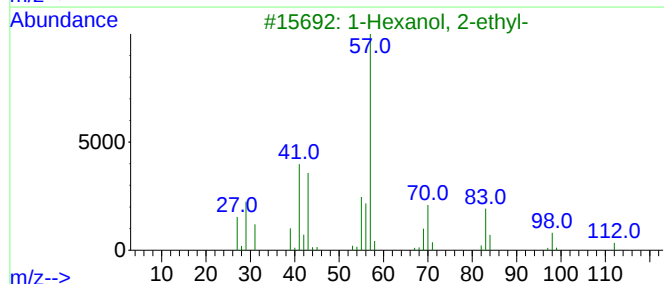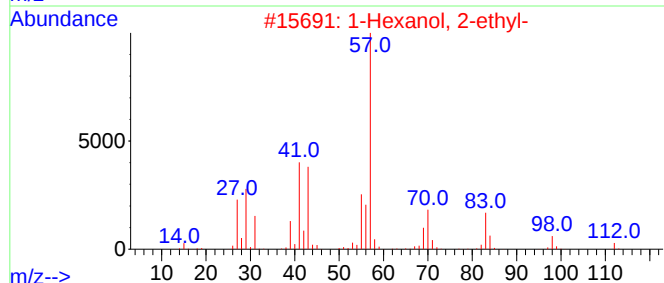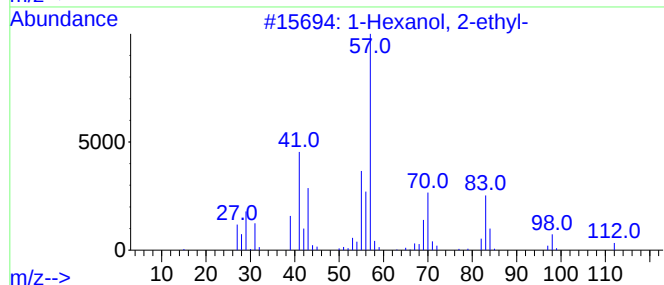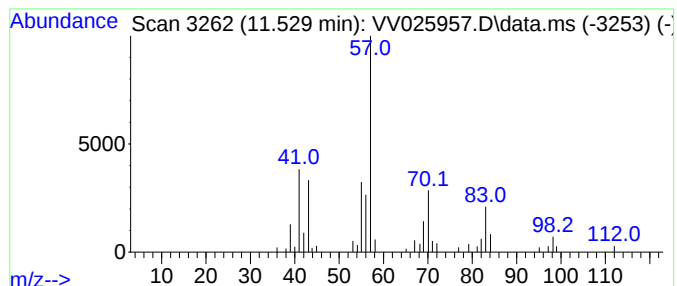

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025957.D
Acq On : 26 May 2022 14:48
Operator : SY/MD
Sample : N3039-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.529	2.7	ug/L	50193	3	11.246	927164	50.0