

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025961.D
 Acq On : 26 May 2022 16:23
 Operator : SY/MD
 Sample : N3039-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	88222	90630	21.38%	2.919%
2	1.568	158	164	177	rVB	68208	76519	18.05%	2.465%
3	2.108	323	332	349	rVB	136172	194475	45.87%	6.265%
4	2.462	440	442	445	rBV2	434	241	0.06%	0.008%
5	2.503	452	455	456	rBV2	798	401	0.09%	0.013%
6	2.584	479	480	482	rBV	359	144	0.03%	0.005%
7	2.674	505	508	509	rBV	231	104	0.02%	0.003%
8	2.696	513	515	520	rVB	615	391	0.09%	0.013%
9	2.761	533	535	539	rVB3	318	199	0.05%	0.006%
10	2.777	539	540	544	rVB	308	126	0.03%	0.004%
11	2.796	544	546	549	rVB2	294	131	0.03%	0.004%
12	2.815	549	552	554	rBV2	390	225	0.05%	0.007%
13	3.008	605	612	615	rBV2	370	343	0.08%	0.011%
14	3.105	639	642	643	rBV	285	138	0.03%	0.004%
15	3.127	647	649	651	rBV	338	135	0.03%	0.004%
16	3.243	681	685	691	rBV2	329	399	0.09%	0.013%
17	3.458	750	752	753	rBV	286	115	0.03%	0.004%
18	3.516	768	770	772	rVB	262	110	0.03%	0.004%
19	3.532	772	775	778	rVB	311	255	0.06%	0.008%
20	3.555	778	782	787	rBV2	191	220	0.05%	0.007%
21	3.915	877	894	919	rBV2	30181	115938	27.35%	3.735%
22	4.352	1015	1030	1054	rBV2	69179	177086	41.77%	5.704%
23	4.526	1082	1084	1087	rBV2	488	285	0.07%	0.009%
24	4.642	1117	1120	1122	rVB3	233	145	0.03%	0.005%
25	4.654	1122	1124	1128	rBV2	377	233	0.05%	0.008%
26	4.706	1137	1140	1142	rBV3	213	168	0.04%	0.005%
27	4.754	1152	1155	1160	rBV3	370	377	0.09%	0.012%
28	4.828	1174	1178	1180	rBV2	289	216	0.05%	0.007%
29	4.918	1203	1206	1209	rBV2	221	197	0.05%	0.006%
30	4.947	1212	1215	1219	rVB2	454	333	0.08%	0.011%
31	4.973	1219	1223	1224	rBV	329	232	0.05%	0.007%
32	5.050	1230	1247	1279	rBV2	162518	423936	100.00%	13.656%
33	5.265	1313	1314	1319	rVB2	378	230	0.05%	0.007%
34	5.326	1330	1333	1337	rVB3	400	264	0.06%	0.009%
35	5.365	1341	1345	1349	rVV3	357	359	0.08%	0.012%
36	5.384	1349	1351	1354	rVB3	287	150	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025961.D
 Acq On : 26 May 2022 16:23
 Operator : SY/MD
 Sample : N3039-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.449	1369	1371	1373	rBV2	289	139	0.03%	0.004%
38	5.523	1392	1394	1395	rBV	279	128	0.03%	0.004%
39	5.619	1413	1424	1455	rBV	121095	254148	59.95%	8.187%
40	5.851	1493	1496	1497	rBV	299	157	0.04%	0.005%
41	5.873	1501	1503	1508	rBV	384	275	0.06%	0.009%
42	5.921	1508	1518	1529	rVB8	3547	7718	1.82%	0.249%
43	5.966	1529	1532	1537	rVB4	299	241	0.06%	0.008%
44	6.072	1552	1565	1585	rBV	89834	192659	45.45%	6.206%
45	6.223	1609	1612	1613	rBV	344	132	0.03%	0.004%
46	6.256	1620	1622	1626	rVB2	279	170	0.04%	0.005%
47	6.297	1631	1635	1637	rBV	304	211	0.05%	0.007%
48	6.410	1664	1670	1671	rBV	457	341	0.08%	0.011%
49	6.439	1675	1679	1680	rBV	214	128	0.03%	0.004%
50	6.529	1705	1707	1710	rBV2	241	124	0.03%	0.004%
51	6.545	1710	1712	1716	rVB2	332	173	0.04%	0.006%
52	6.728	1767	1769	1771	rBV2	314	183	0.04%	0.006%
53	6.796	1787	1790	1795	rVB2	164	182	0.04%	0.006%
54	6.831	1795	1801	1804	rBV2	230	271	0.06%	0.009%
55	6.924	1827	1830	1836	rVB2	214	153	0.04%	0.005%
56	6.992	1838	1851	1867	rBV2	34821	68093	16.06%	2.193%
57	7.185	1906	1911	1914	rBV2	409	339	0.08%	0.011%
58	7.201	1914	1916	1919	rVV2	342	181	0.04%	0.006%
59	7.268	1933	1937	1940	rBV2	164	147	0.03%	0.005%
60	7.317	1940	1952	1971	rBV	160186	286905	67.68%	9.242%
61	7.587	2031	2036	2039	rBV3	304	331	0.08%	0.011%
62	7.629	2040	2049	2063	rBV2	22111	41066	9.69%	1.323%
63	7.834	2109	2113	2114	rBV	239	131	0.03%	0.004%
64	7.847	2114	2117	2118	rBV	183	106	0.03%	0.003%
65	7.944	2141	2147	2154	rVB4	1354	1879	0.44%	0.061%
66	7.976	2154	2157	2162	rVV2	310	199	0.05%	0.006%
67	8.014	2166	2169	2172	rVB	339	201	0.05%	0.006%
68	8.063	2181	2184	2186	rBV2	249	165	0.04%	0.005%
69	8.095	2186	2194	2231	rBV	54908	135475	31.96%	4.364%
70	8.429	2296	2298	2303	rBV2	372	217	0.05%	0.007%
71	8.477	2310	2313	2315	rBV2	360	172	0.04%	0.006%
72	8.538	2329	2332	2336	rBV2	322	235	0.06%	0.008%
73	8.638	2361	2363	2366	rBV2	223	131	0.03%	0.004%
74	8.674	2369	2374	2375	rBV	328	239	0.06%	0.008%
75	8.683	2375	2377	2379	rVB	253	105	0.02%	0.003%
76	8.741	2391	2395	2397	rBV2	400	276	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025961.D
 Acq On : 26 May 2022 16:23
 Operator : SY/MD
 Sample : N3039-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	8.780	2404	2407	2412	rBV	278	191	0.05%	0.006%
78	8.854	2419	2430	2458	rBV	185885	319915	75.46%	10.305%
79	9.162	2524	2526	2527	rVB	350	112	0.03%	0.004%
80	9.239	2546	2550	2555	rBV3	582	522	0.12%	0.017%
81	9.284	2561	2564	2566	rBV	241	141	0.03%	0.005%
82	9.349	2581	2584	2586	rBV	334	185	0.04%	0.006%
83	9.571	2650	2653	2655	rBV2	411	238	0.06%	0.008%
84	9.696	2688	2692	2697	rVB2	324	272	0.06%	0.009%
85	9.751	2706	2709	2714	rVB	309	266	0.06%	0.009%
86	9.786	2716	2720	2723	rBV	288	256	0.06%	0.008%
87	9.979	2777	2780	2784	rBV	441	292	0.07%	0.009%
88	10.156	2833	2835	2838	rBV2	158	103	0.02%	0.003%
89	10.217	2843	2854	2873	rVV	113906	184589	43.54%	5.946%
90	10.365	2898	2900	2901	rBV	439	205	0.05%	0.007%
91	10.426	2916	2919	2921	rBV	231	125	0.03%	0.004%
92	10.847	3046	3050	3053	rBV	519	363	0.09%	0.012%
93	11.140	3139	3141	3145	rBV2	323	251	0.06%	0.008%
94	11.207	3159	3162	3164	rBV2	355	214	0.05%	0.007%
95	11.249	3164	3175	3193	rBV	168297	270270	63.75%	8.706%
96	11.426	3227	3230	3232	rBV3	711	458	0.11%	0.015%
97	11.538	3259	3265	3274	rVB6	2302	3728	0.88%	0.120%
98	11.625	3280	3292	3308	rBV	146337	241566	56.98%	7.782%
99	12.747	3639	3641	3643	rVB	478	214	0.05%	0.007%
100	13.406	3843	3846	3849	rBV	480	271	0.06%	0.009%




Sum of corrected areas: 3104323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025961.D
Acq On : 26 May 2022 16:23
Operator : SY/MD
Sample : N3039-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

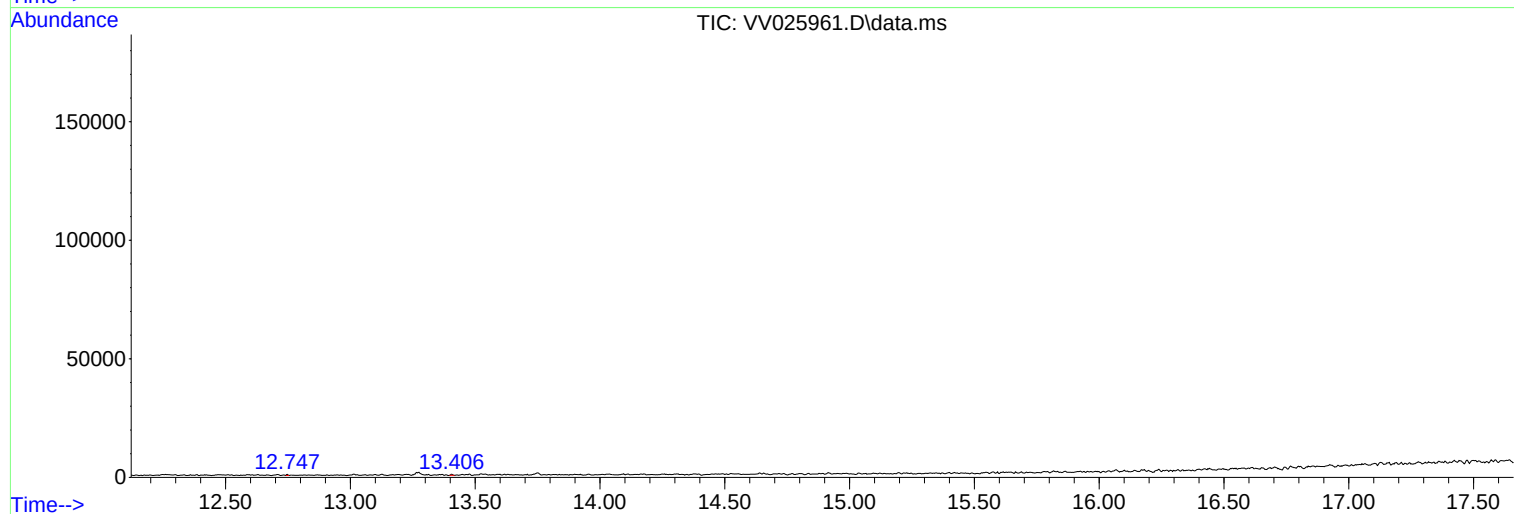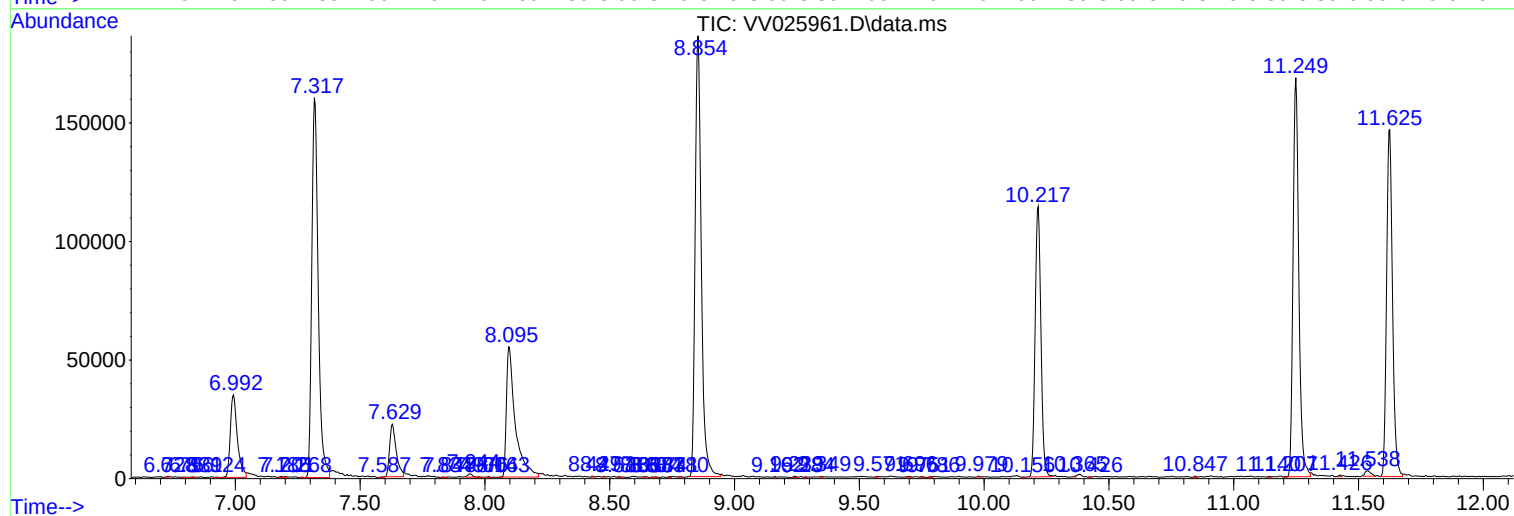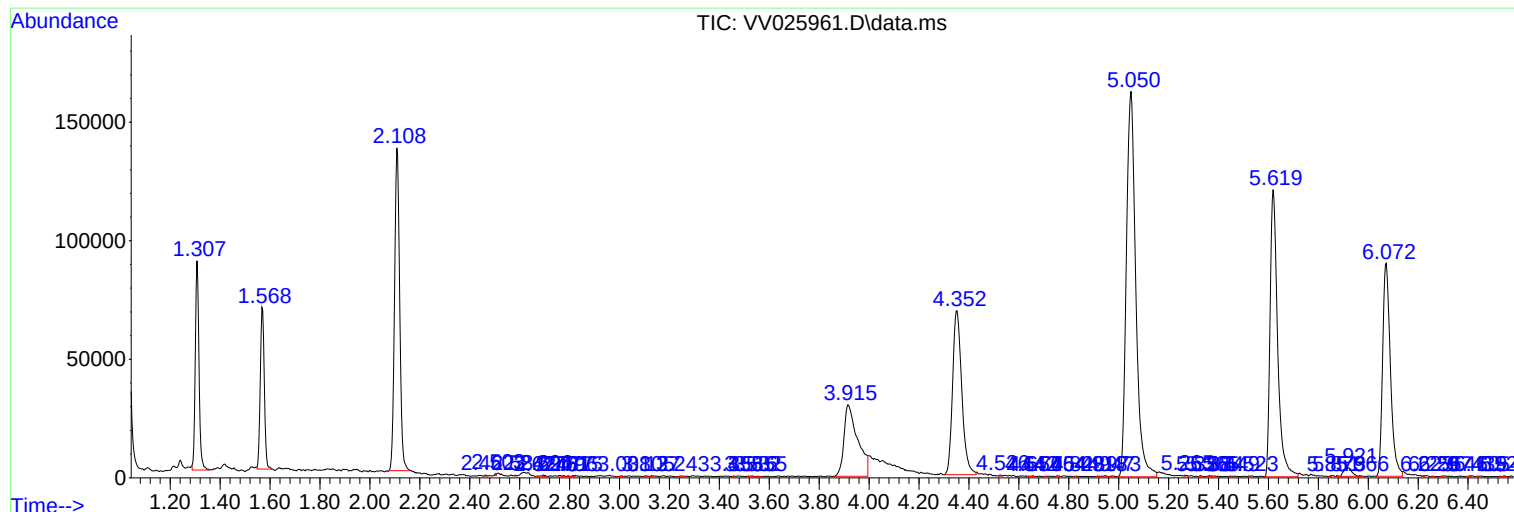

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025961.D
Acq On : 26 May 2022 16:23
Operator : SY/MD
Sample : N3039-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025961.D
Acq On : 26 May 2022 16:23
Operator : SY/MD
Sample : N3039-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc