

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025964.D
 Acq On : 26 May 2022 17:35
 Operator : SY/MD
 Sample : N3039-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M

Title : VOC Analysis

Signal : TIC: VV025964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB	292339	294715	18.20%	2.578%
2	1.571	158	165	178	rVB	242266	270915	16.73%	2.370%
3	2.111	323	333	355	rBV	494786	711007	43.90%	6.221%
4	2.429	429	432	436	rBV4	803	722	0.04%	0.006%
5	2.584	478	480	481	rBV	366	200	0.01%	0.002%
6	2.712	516	520	521	rBV2	471	306	0.02%	0.003%
7	2.806	547	549	550	rBV	396	139	0.01%	0.001%
8	2.838	556	559	562	rBV2	254	147	0.01%	0.001%
9	3.044	619	623	629	rBV3	262	327	0.02%	0.003%
10	3.117	643	646	650	rBV2	278	164	0.01%	0.001%
11	3.214	674	676	680	rVB	309	152	0.01%	0.001%
12	3.236	680	683	686	rVB2	221	151	0.01%	0.001%
13	3.262	686	691	692	rBV	230	147	0.01%	0.001%
14	3.339	712	715	717	rBV	200	127	0.01%	0.001%
15	3.371	723	725	727	rVB	359	153	0.01%	0.001%
16	3.416	735	739	742	rBV2	247	208	0.01%	0.002%
17	3.462	751	753	758	rBV2	296	222	0.01%	0.002%
18	3.548	774	780	781	rBV	307	221	0.01%	0.002%
19	3.590	791	793	796	rVB2	347	152	0.01%	0.001%
20	3.613	796	800	802	rBV	362	303	0.02%	0.003%
21	3.670	813	818	821	rBV	287	268	0.02%	0.002%
22	3.687	821	823	827	rVV2	279	189	0.01%	0.002%
23	3.709	827	830	832	rBV2	230	150	0.01%	0.001%
24	3.796	854	857	862	rBV	237	195	0.01%	0.002%
25	3.912	878	893	923	rBV2	70407	294692	18.20%	2.578%
26	4.352	1014	1030	1054	rBV	264273	653603	40.36%	5.718%
27	4.690	1131	1135	1136	rBV2	246	206	0.01%	0.002%
28	4.786	1163	1165	1167	rBV2	312	154	0.01%	0.001%
29	4.815	1172	1174	1177	rVV2	251	103	0.01%	0.001%
30	4.876	1190	1193	1198	rVB4	504	466	0.03%	0.004%
31	4.934	1208	1211	1213	rBV2	311	200	0.01%	0.002%
32	5.047	1229	1246	1277	rBV2	638190	1619549	100.00%	14.169%
33	5.365	1342	1345	1346	rBV2	479	276	0.02%	0.002%
34	5.429	1363	1365	1368	rBV4	512	299	0.02%	0.003%
35	5.519	1391	1393	1397	rVB2	279	113	0.01%	0.001%
36	5.561	1401	1406	1408	rVB3	579	356	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052622\
 Data File : VW025964.D
 Acq On : 26 May 2022 17:35
 Operator : SY/MD
 Sample : N3039-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.619	1412	1424	1452	rBV	380978	783697	48.39%	6.856%
38	5.857	1496	1498	1500	rBV	429	238	0.01%	0.002%
39	5.908	1504	1514	1527	rBV4	15024	32213	1.99%	0.282%
40	6.069	1550	1564	1594	rBV	364043	742269	45.83%	6.494%
41	6.346	1648	1650	1654	rVB2	475	267	0.02%	0.002%
42	6.368	1654	1657	1663	rBV3	806	706	0.04%	0.006%
43	6.394	1663	1665	1667	rVB3	442	138	0.01%	0.001%
44	6.442	1676	1680	1681	rBV	346	174	0.01%	0.002%
45	6.455	1682	1684	1687	rVB2	337	166	0.01%	0.001%
46	6.471	1687	1689	1691	rBV2	470	223	0.01%	0.002%
47	6.561	1714	1717	1718	rBV	247	125	0.01%	0.001%
48	6.641	1739	1742	1744	rBV2	486	306	0.02%	0.003%
49	6.690	1756	1757	1760	rBV2	345	195	0.01%	0.002%
50	6.751	1774	1776	1777	rBV	281	113	0.01%	0.001%
51	6.793	1787	1789	1791	rVV	279	128	0.01%	0.001%
52	6.809	1791	1794	1803	rVV4	572	616	0.04%	0.005%
53	6.924	1828	1830	1832	rBV	283	113	0.01%	0.001%
54	6.985	1838	1849	1881	rBV	160485	304674	18.81%	2.666%
55	7.272	1935	1938	1940	rBV3	317	245	0.02%	0.002%
56	7.317	1940	1952	1972	rBV	718027	1239831	76.55%	10.847%
57	7.622	2037	2047	2070	rBV	108851	200565	12.38%	1.755%
58	7.918	2131	2139	2140	rBV3	591	782	0.05%	0.007%
59	7.937	2141	2145	2155	rVB4	1907	2489	0.15%	0.022%
60	7.979	2156	2158	2159	rBV2	420	147	0.01%	0.001%
61	8.034	2170	2175	2178	rVB2	391	354	0.02%	0.003%
62	8.053	2178	2181	2182	rBV	288	169	0.01%	0.001%
63	8.092	2183	2193	2230	rBV	280454	625191	38.60%	5.470%
64	8.487	2313	2316	2318	rBV3	418	256	0.02%	0.002%
65	8.532	2325	2330	2333	rBV2	912	833	0.05%	0.007%
66	8.648	2364	2366	2369	rBV3	287	159	0.01%	0.001%
67	8.747	2395	2397	2400	rBV3	271	157	0.01%	0.001%
68	8.799	2408	2413	2416	rBV3	312	307	0.02%	0.003%
69	8.850	2416	2429	2457	rBV	616200	1001745	61.85%	8.764%
70	9.140	2517	2519	2521	rBV3	529	270	0.02%	0.002%
71	9.201	2534	2538	2540	rBV	289	198	0.01%	0.002%
72	9.236	2546	2549	2552	rBV2	321	224	0.01%	0.002%
73	9.313	2570	2573	2574	rBV	324	158	0.01%	0.001%
74	9.358	2584	2587	2589	rVB2	580	252	0.02%	0.002%
75	9.371	2589	2591	2594	rBV2	339	213	0.01%	0.002%
76	9.526	2636	2639	2641	rVB2	244	107	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025964.D
 Acq On : 26 May 2022 17:35
 Operator : SY/MD
 Sample : N3039-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.548	2644	2646	2652	rBV3	745	656	0.04%	0.006%
78	9.580	2654	2656	2658	rBV	369	181	0.01%	0.002%
79	9.635	2669	2673	2675	rBV2	300	223	0.01%	0.002%
80	9.899	2753	2755	2757	rBV	225	136	0.01%	0.001%
81	9.992	2781	2784	2786	rBV2	215	158	0.01%	0.001%
82	10.021	2792	2793	2796	rBV	347	106	0.01%	0.001%
83	10.095	2812	2816	2817	rBV2	232	144	0.01%	0.001%
84	10.124	2817	2825	2834	rVV5	3217	4710	0.29%	0.041%
85	10.214	2841	2853	2873	rBV	449209	717846	44.32%	6.280%
86	10.413	2913	2915	2917	rBV	355	164	0.01%	0.001%
87	10.522	2948	2949	2951	rBV	243	109	0.01%	0.001%
88	10.783	3027	3030	3031	rBV2	231	134	0.01%	0.001%
89	10.998	3093	3097	3100	rBV2	238	262	0.02%	0.002%
90	11.030	3101	3107	3116	rVB5	814	1208	0.07%	0.011%
91	11.062	3116	3117	3119	rBV	479	124	0.01%	0.001%
92	11.146	3136	3143	3150	rBV6	1210	1640	0.10%	0.014%
93	11.246	3163	3174	3201	rBV	550289	866055	53.48%	7.577%
94	11.535	3258	3264	3277	rBV7	3043	5583	0.34%	0.049%
95	11.622	3279	3291	3308	rBV	664655	1035605	63.94%	9.060%
96	11.786	3337	3342	3348	rVB6	1108	1442	0.09%	0.013%
97	12.011	3411	3412	3413	rBV6	301	115	0.01%	0.001%
98	12.304	3500	3503	3506	rVB	522	318	0.02%	0.003%
99	12.545	3576	3578	3582	rVB	494	298	0.02%	0.003%
100	12.567	3582	3585	3588	rBV	584	499	0.03%	0.004%




Sum of corrected areas: 11430026

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025964.D
Acq On : 26 May 2022 17:35
Operator : SY/MD
Sample : N3039-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

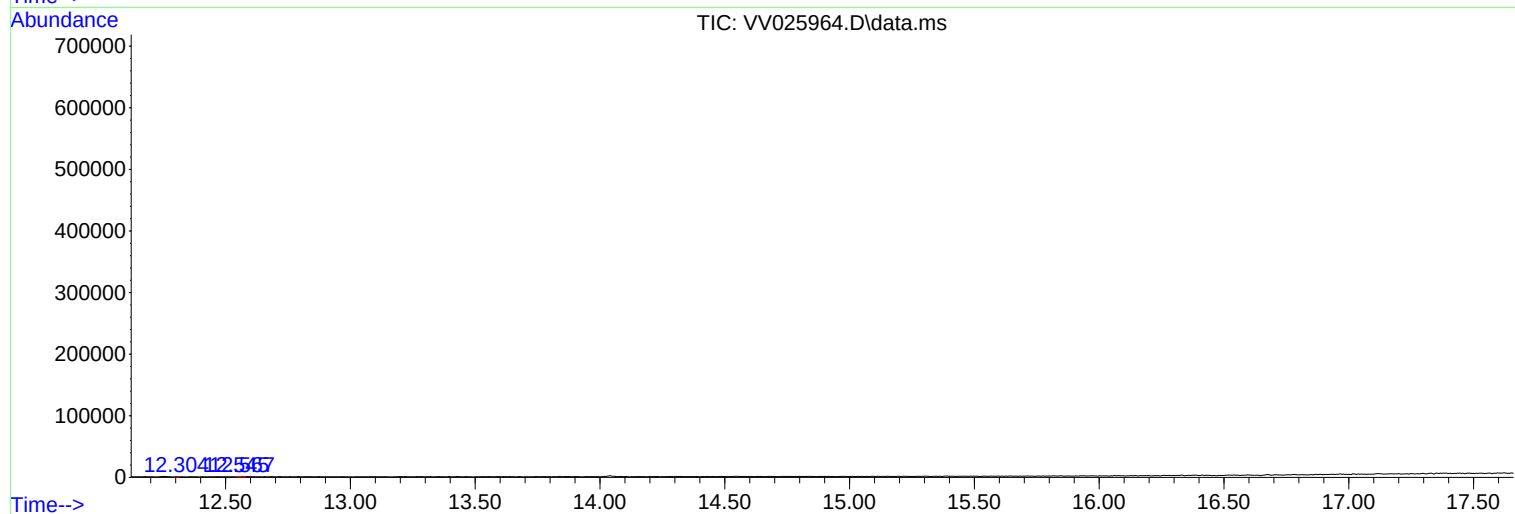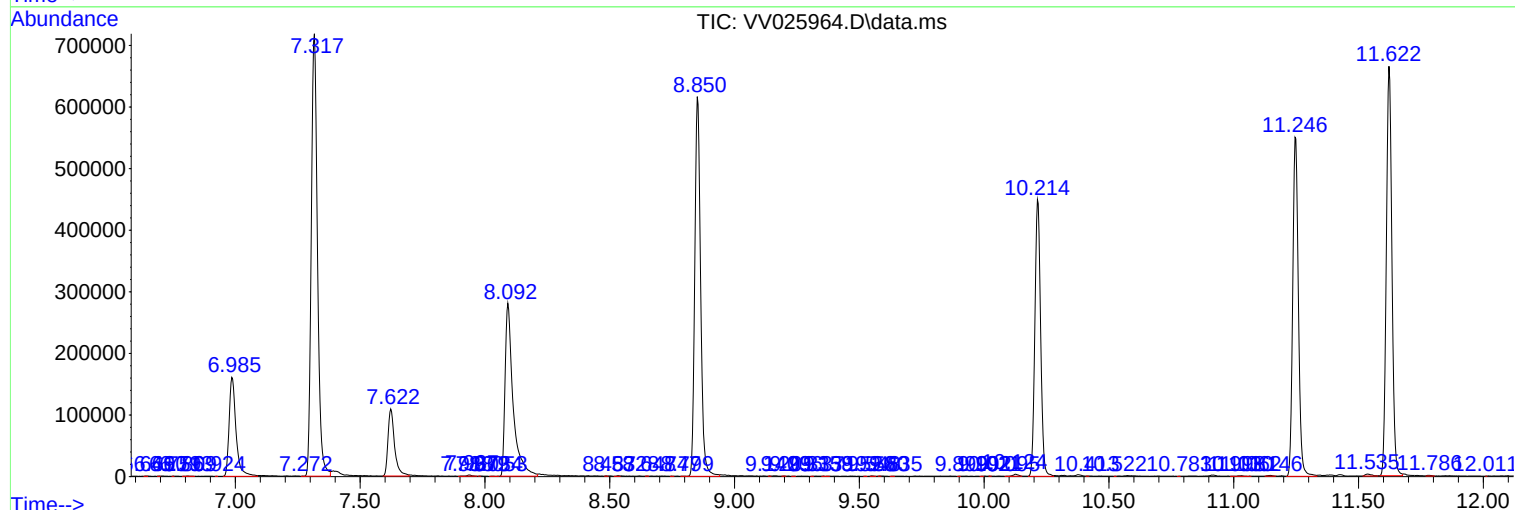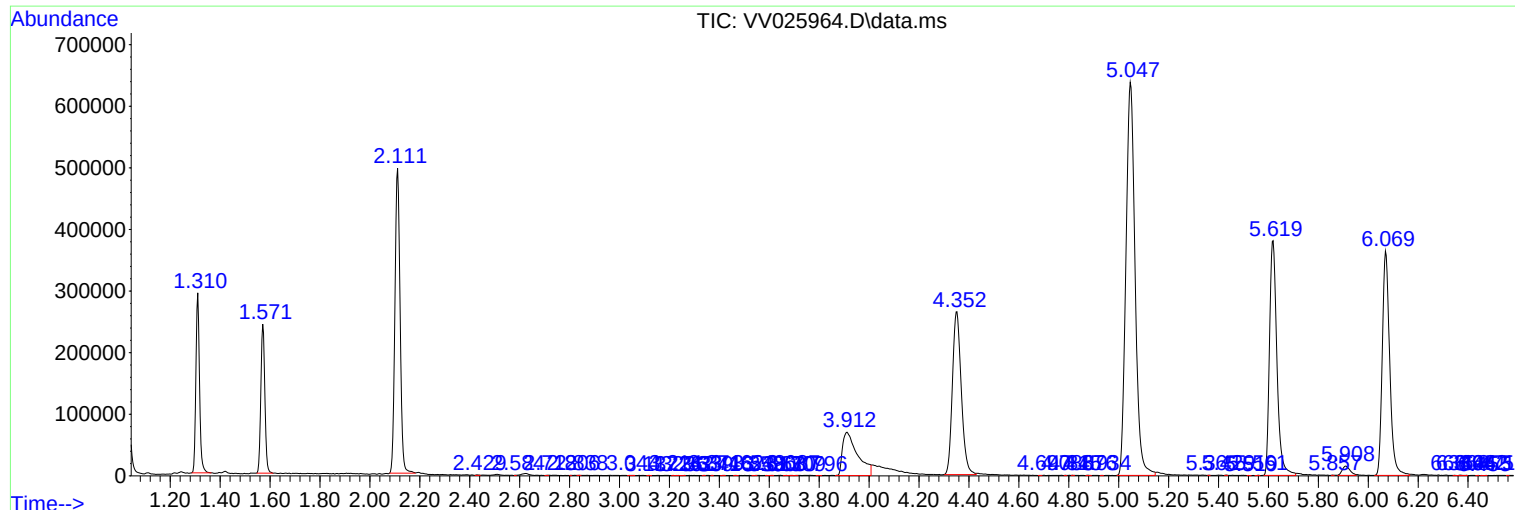

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025964.D
Acq On : 26 May 2022 17:35
Operator : SY/MD
Sample : N3039-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025964.D
Acq On : 26 May 2022 17:35
Operator : SY/MD
Sample : N3039-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc