


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025954.D
 Acq On : 26 May 2022 11:33
 Operator : SY/MD
 Sample : BFB283
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB283

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis
 Last Update : Fri May 27 01:28:09 2022

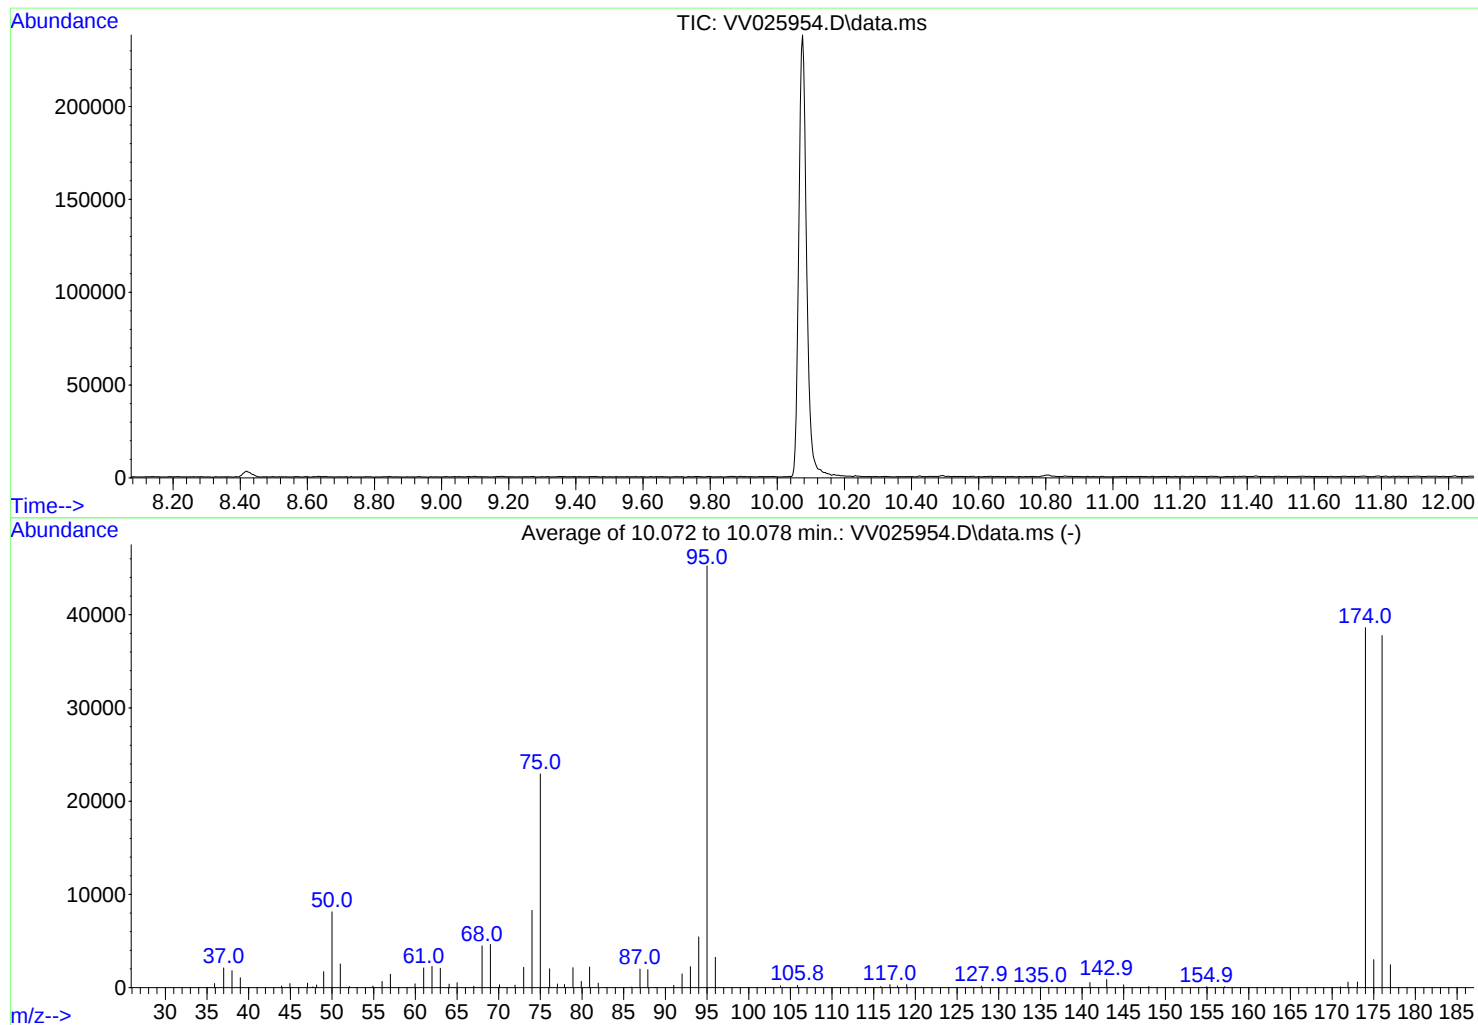

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	8145	PASS
75	95	30	80	50.7	22939	PASS
95	95	100	100	100.0	45245	PASS
96	95	5	9	7.2	3270	PASS
173	174	0.00	2	1.6	607	PASS
174	95	50	120	85.3	38616	PASS
175	174	5	9	7.8	3000	PASS
176	174	95	105	97.8	37768	PASS
177	176	5	10	6.5	2455	PASS

m/z	Abundance
40.00	262.0
43.90	490.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.90	469.0
37.00	2213.0
38.00	1871.0
39.00	983.0
39.90	271.0
44.00	614.0
44.90	547.0
47.10	520.0
48.10	347.0
49.00	1740.0
50.00	8153.0
51.00	2571.0
52.10	133.0
54.90	183.0
56.00	623.0
57.00	1517.0
60.00	422.0
61.00	2102.0
62.00	2272.0
63.00	2097.0
64.00	375.0
65.00	466.0
67.00	147.0
68.00	4579.0
69.00	4625.0
70.10	305.0
72.00	312.0
73.00	2080.0
74.00	8202.0
75.00	22928.0
76.10	2192.0
77.00	322.0
77.90	353.0
78.90	2166.0
79.90	681.0
80.90	2238.0
82.00	500.0
85.90	121.0
87.00	2093.0
87.90	2021.0
88.80	123.0
91.00	201.0
92.00	1531.0
93.00	2241.0
94.00	5538.0
95.00	45392.0
96.00	3218.0
103.90	187.0
105.90	259.0
116.00	133.0
117.00	340.0
117.80	191.0
118.90	313.0
127.90	168.0
136.90	118.0
140.90	530.0
143.00	884.0
145.00	336.0
155.00	147.0
157.10	102.0
171.90	564.0
173.00	557.0
174.00	38264.0
175.00	2992.0
176.00	37064.0
177.00	2501.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.90	479.0
37.00	2154.0
38.00	1856.0
39.00	1145.0
40.00	267.0
44.00	651.0
45.00	461.0
47.10	488.0
48.10	316.0
49.00	1771.0
50.00	8365.0
51.00	2581.0
52.10	120.0
52.90	104.0
54.90	173.0
56.00	673.0
57.00	1493.0
59.90	426.0
61.00	2176.0
62.00	2371.0
63.00	2145.0
64.10	404.0
65.00	532.0
67.00	160.0
68.00	4652.0
69.00	4802.0
70.10	300.0
71.90	287.0
73.00	2269.0
74.00	8546.0
75.00	23816.0
76.10	2134.0
77.10	314.0
77.90	357.0
78.90	2232.0
79.90	717.0
80.90	2306.0
82.00	469.0
85.90	108.0
86.90	2050.0
87.90	2000.0
91.00	257.0
92.00	1513.0
93.00	2338.0
94.00	5652.0
95.00	46744.0
96.00	3368.0
103.80	194.0
105.80	255.0
115.80	123.0
116.90	326.0
117.80	168.0
119.00	343.0
127.90	173.0
135.00	127.0
141.00	586.0
143.00	898.0
144.00	106.0
145.00	326.0
148.00	157.0
154.90	107.0
157.10	121.0
171.00	129.0
171.90	630.0
173.10	621.0
174.00	39800.0
175.00	3128.0
176.00	39112.0
177.00	2543.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.90	399.0
37.00	1945.0
38.00	1756.0
39.00	1086.0
40.00	249.0
44.00	709.0
45.00	331.0
47.00	431.0
47.70	250.0
48.20	230.0
49.00	1651.0
50.00	7917.0
51.00	2455.0
52.10	101.0
54.90	139.0
56.00	696.0
57.00	1318.0
59.90	387.0
61.00	2075.0
62.00	2227.0
63.00	1996.0
64.10	380.0
65.00	577.0
67.00	138.0
68.00	4199.0
69.00	4458.0
70.10	301.0
71.90	251.0
73.00	2179.0
74.00	8139.0
75.00	22072.0
76.10	1775.0
76.90	254.0
77.20	280.0
77.90	324.0
78.90	2068.0
79.90	630.0
80.90	2093.0
81.90	476.0
82.80	116.0
86.90	1842.0
87.90	1746.0
91.00	268.0
92.00	1409.0
93.00	2189.0
94.00	5148.0
95.00	43600.0
96.00	3224.0
103.70	197.0
105.80	233.0
115.70	106.0
116.90	335.0
117.90	153.0
119.00	308.0
127.90	158.0
135.00	104.0
141.00	528.0
142.90	834.0
145.00	264.0
148.00	184.0
154.90	100.0
157.10	111.0
171.00	115.0
171.90	612.0
173.00	642.0
174.00	37784.0
175.00	2881.0
176.00	37128.0
177.00	2322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283