

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052722\
 Data File : VW025974.D
 Acq On : 27 May 2022 13:03
 Operator : SY/MD
 Sample : N3039-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ0

Quant Time: May 27 22:35:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 22:34:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	318928	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	316935	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	144354	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	168571	40.954	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.900%		
7) Chloroethane-d5	1.568	69	139097	38.481	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.960%		
11) 1,1-Dichloroethene-d2	2.108	63	253578	35.225	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.440%		
21) 2-Butanone-d5	3.908	46	116156	65.841	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	65.840%		
24) Chloroform-d	4.349	84	266013	46.271	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.540%		
26) 1,2-Dichloroethane-d4	5.031	65	164985	47.484	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.960%		
32) Benzene-d6	5.050	84	546714	49.481	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.960%		
36) 1,2-Dichloropropane-d6	6.069	67	172131	50.723	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.440%		
41) Toluene-d8	7.313	98	471927	46.358	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.720%		
43) trans-1,3-Dichloroprop...	7.622	79	66032	43.590	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.180%		
47) 2-Hexanone-d5	8.092	63	98266	78.982	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.980%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	210311	46.473	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.940%		
66) 1,2-Dichlorobenzene-d4	11.622	152	171236	54.077	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.160%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	2433	0.795	ug/L	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025974.D
Acq On : 27 May 2022 13:03
Operator : SY/MD
Sample : N3039-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ0

Quant Time: May 27 22:35:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 27 22:34:02 2022
Response via : Initial Calibration

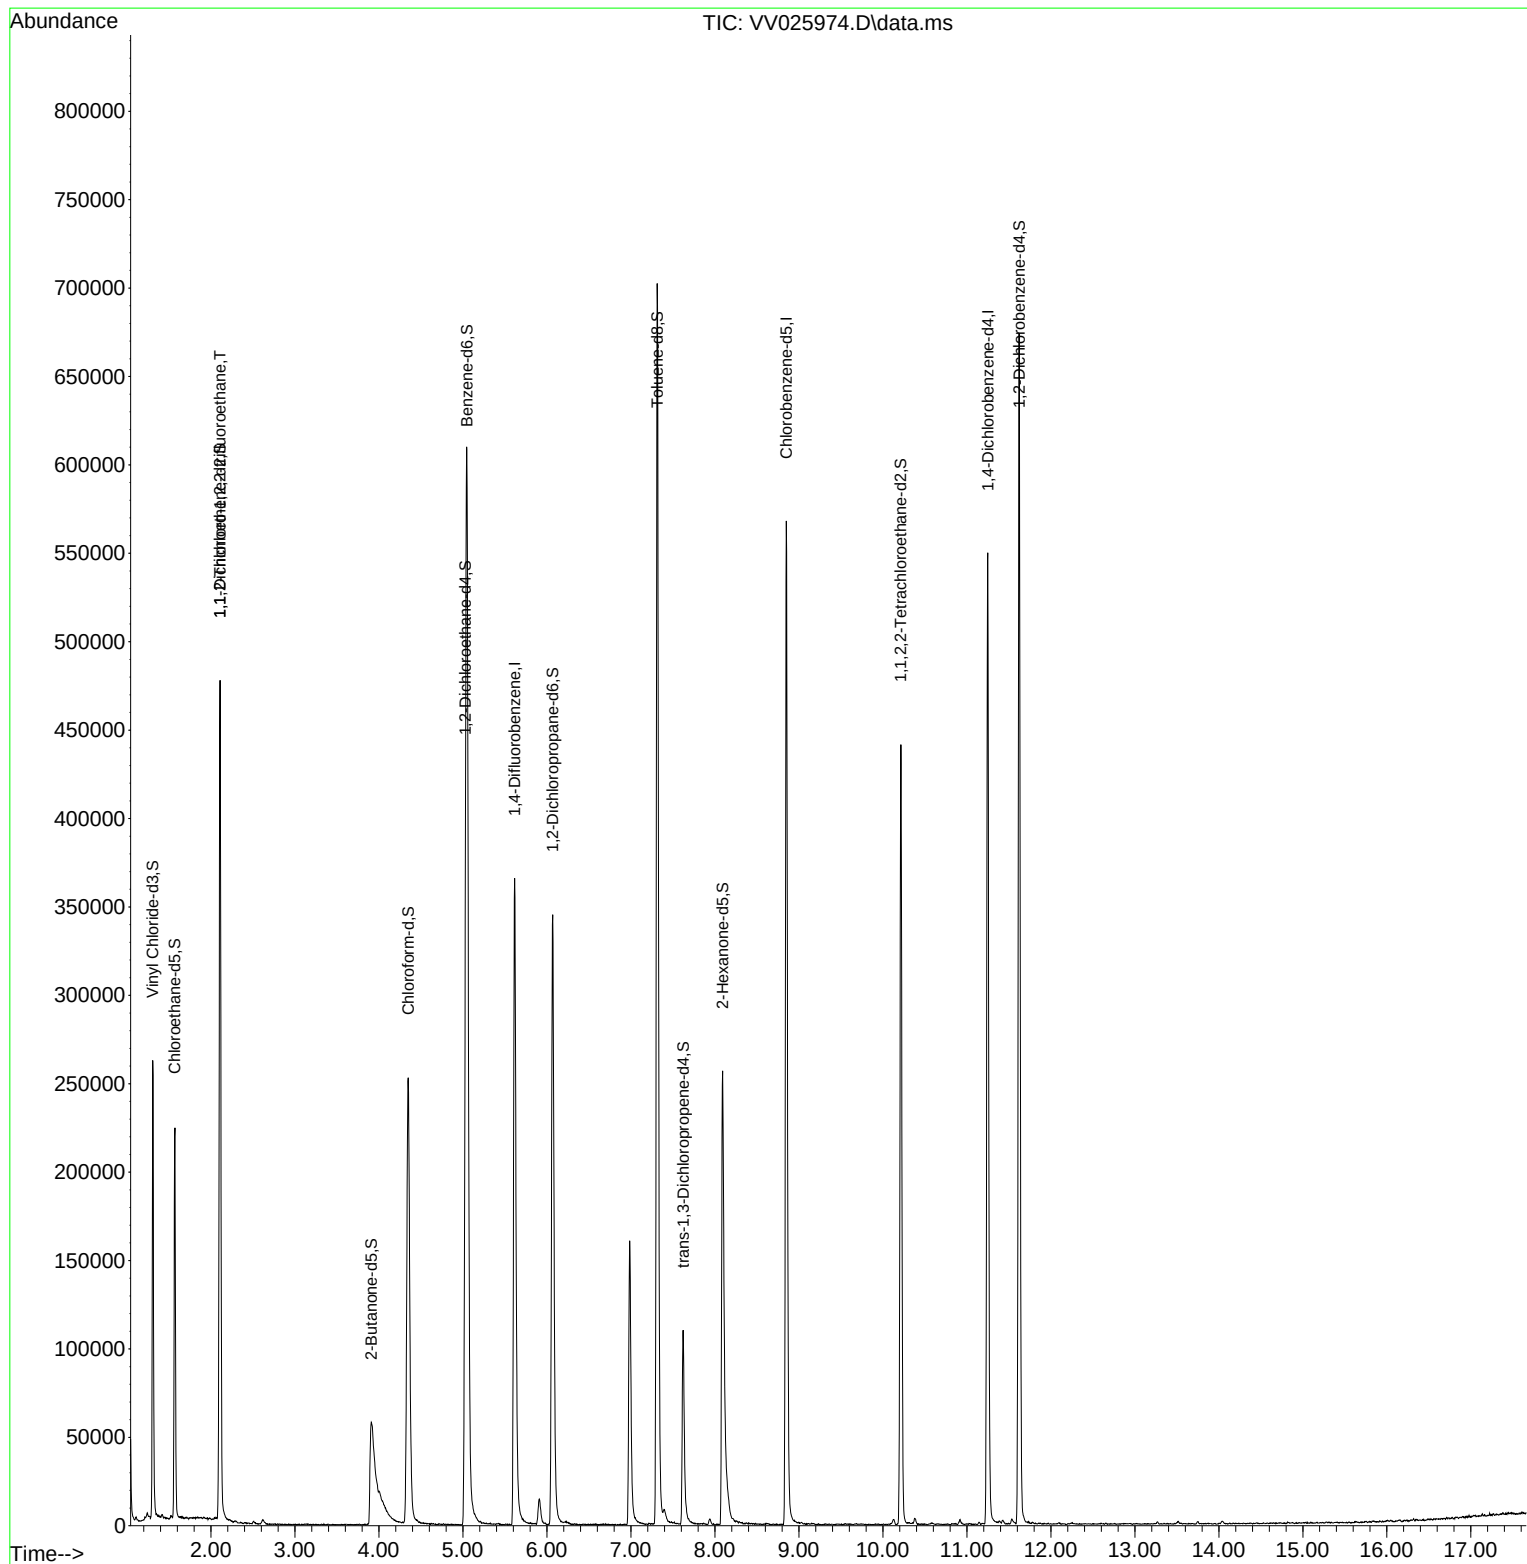

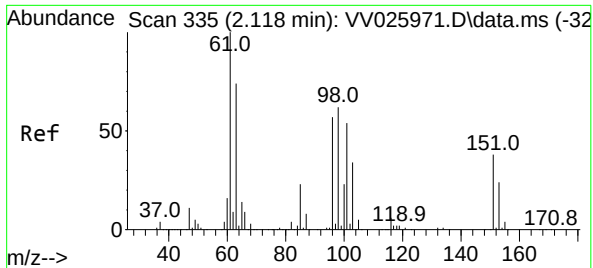

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.795 ug/L
 RT: 2.108 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV025974.D
 Acq: 27 May 2022 13:03

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ0

Tgt Ion:101 Resp: 2433
 Ion Ratio Lower Upper
 101 100
 85 0.0 34.6 51.8#
 151 0.0 54.3 81.5#

