

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052722\
 Data File : VW025975.D
 Acq On : 27 May 2022 13:27
 Operator : SY/MD
 Sample : N3039-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ6

Quant Time: May 27 22:35:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 22:34:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	323978	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	324692	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	144333	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	162926	38.966	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.940%
7) Chloroethane-d5	1.571	69	136803	37.257	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	74.520%
11) 1,1-Dichloroethene-d2	2.108	63	238189	32.571	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.140%
21) 2-Butanone-d5	3.905	46	140281	78.276	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.280%
24) Chloroform-d	4.349	84	261950	44.854	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.700%
26) 1,2-Dichloroethane-d4	5.034	65	160336	45.427	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.860%
32) Benzene-d6	5.050	84	533652	47.145	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.300%
36) 1,2-Dichloropropane-d6	6.069	67	169935	48.880	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.760%
41) Toluene-d8	7.317	98	455382	43.664	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.320%
43) trans-1,3-Dichloroprop...	7.622	79	65000	41.884	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.760%
47) 2-Hexanone-d5	8.092	63	109658	86.033	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.030%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	216124	46.616	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.240%
66) 1,2-Dichlorobenzene-d4	11.622	152	164809	52.055	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.120%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.111	101	2200	0.707	ug/L	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025975.D
Acq On : 27 May 2022 13:27
Operator : SY/MD
Sample : N3039-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ6

Quant Time: May 27 22:35:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 27 22:34:02 2022
Response via : Initial Calibration

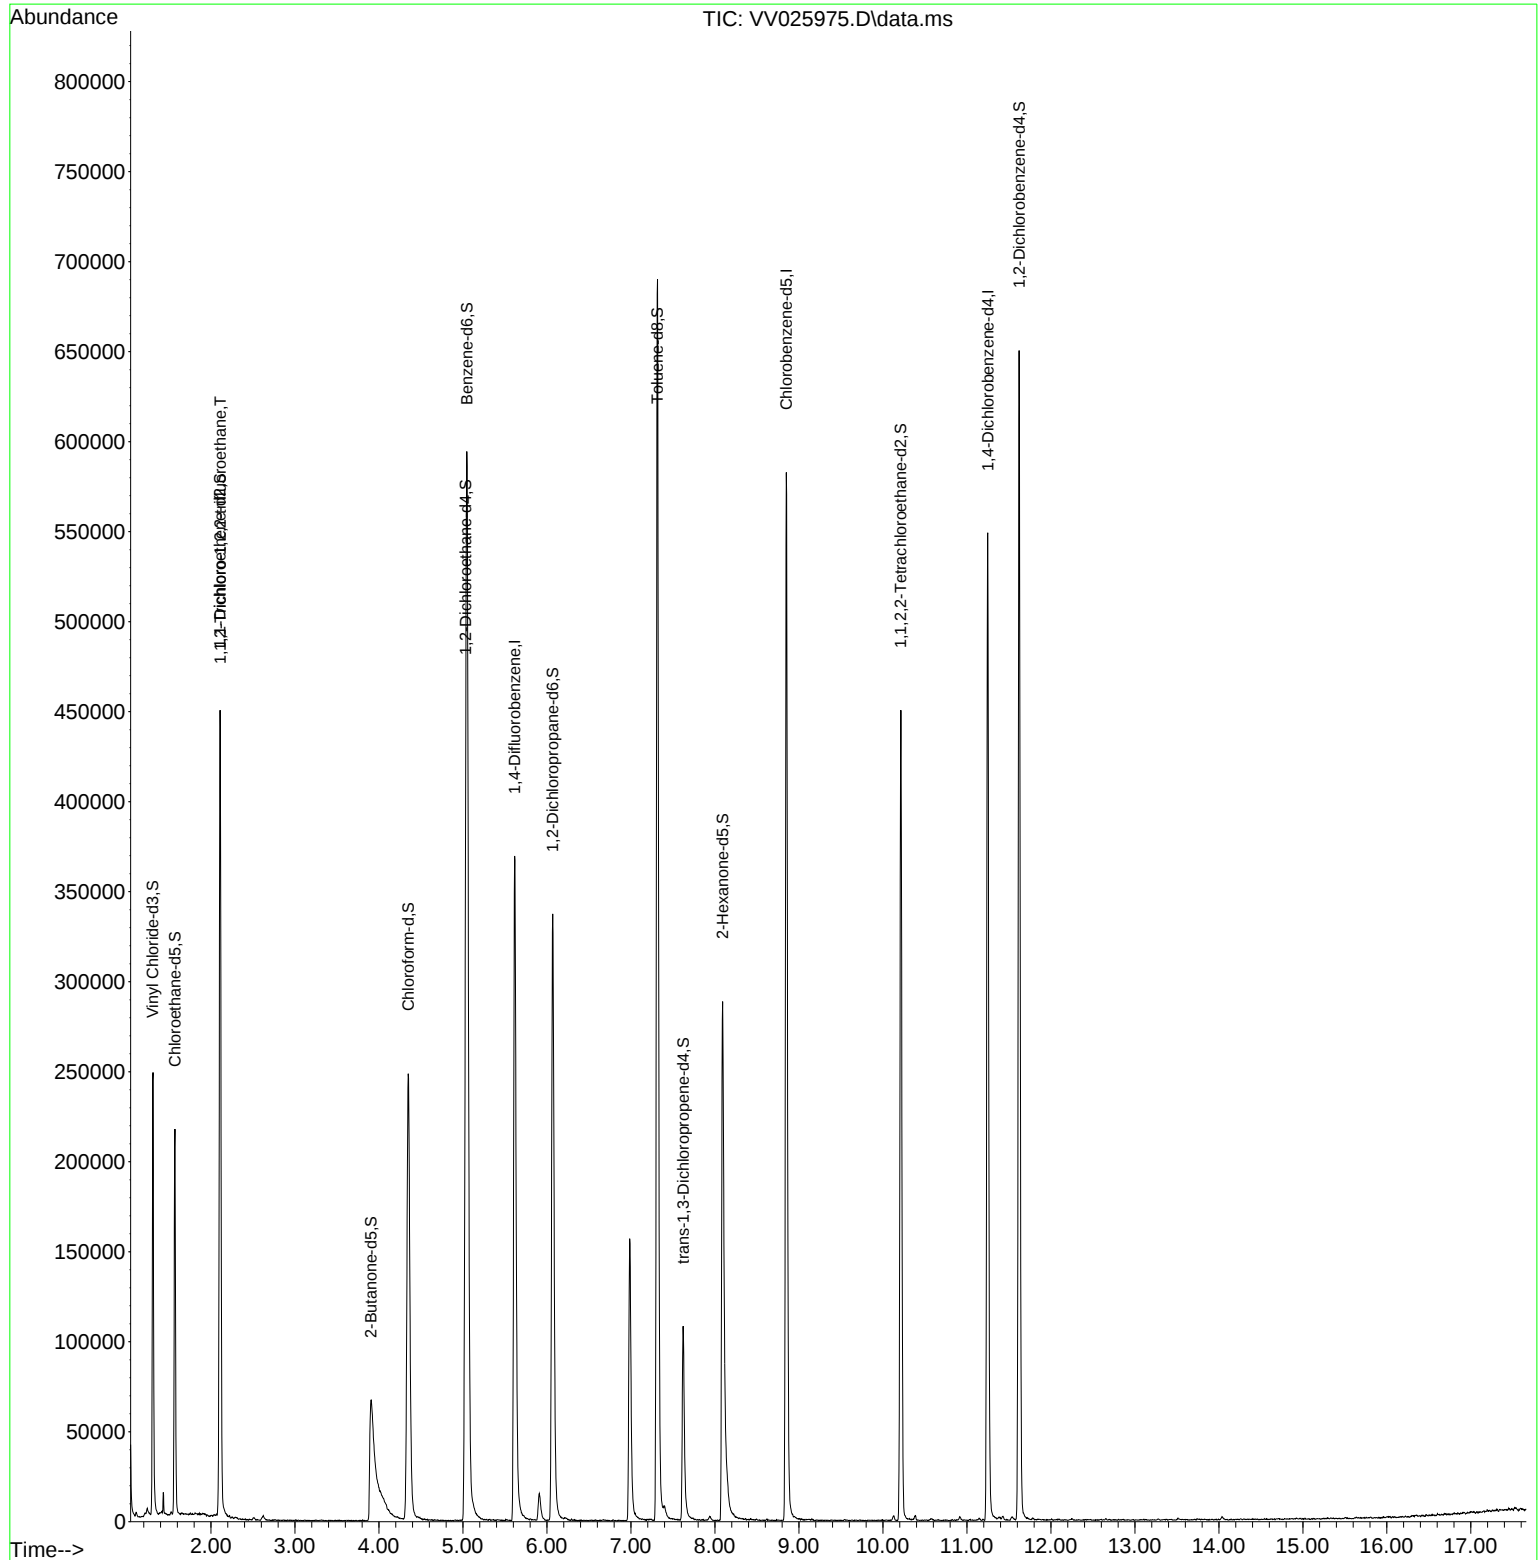

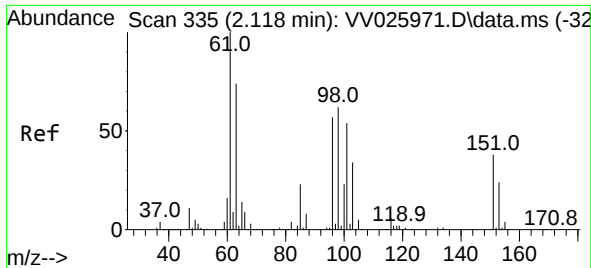

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.707 ug/L
 RT: 2.111 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV025975.D
 Acq: 27 May 2022 13:27

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ6

Tgt Ion:101 Resp: 2200
 Ion Ratio Lower Upper
 101 100
 85 0.0 34.6 51.8#
 151 0.0 54.3 81.5#

