

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025973.D
 Acq On : 27 May 2022 12:37
 Operator : SY/MD
 Sample : VV0527WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	99	rVB	243830	262435	17.04%	2.377%
2	1.571	158	165	185	rVB	216975	245333	15.93%	2.222%
3	2.108	323	332	360	rVB	445634	650392	42.23%	5.892%
4	2.696	513	515	516	rBV	326	123	0.01%	0.001%
5	2.822	551	554	555	rBV	222	117	0.01%	0.001%
6	2.851	558	563	567	rBV3	502	581	0.04%	0.005%
7	2.886	572	574	576	rBV2	248	133	0.01%	0.001%
8	3.040	621	622	626	rBV2	283	194	0.01%	0.002%
9	3.182	662	666	667	rBV2	480	286	0.02%	0.003%
10	3.240	680	684	687	rBV	391	327	0.02%	0.003%
11	3.317	705	708	712	rBV2	216	197	0.01%	0.002%
12	3.343	714	716	718	rVV	272	97	0.01%	0.001%
13	3.401	729	734	736	rBV	260	271	0.02%	0.002%
14	3.481	755	759	760	rBV	178	119	0.01%	0.001%
15	3.491	760	762	764	rVV2	429	254	0.02%	0.002%
16	3.516	767	770	775	rBV2	414	308	0.02%	0.003%
17	3.571	783	787	790	rVB3	332	243	0.02%	0.002%
18	3.597	792	795	800	rVB4	351	298	0.02%	0.003%
19	3.626	802	804	807	rBV	244	145	0.01%	0.001%
20	3.703	826	828	829	rBV	175	75	0.00%	0.001%
21	3.825	863	866	870	rBV2	231	163	0.01%	0.001%
22	3.860	875	877	878	rBV2	200	93	0.01%	0.001%
23	3.905	881	891	922	rBV	57380	229703	14.91%	2.081%
24	4.349	1015	1029	1059	rBV	248800	608410	39.50%	5.512%
25	4.600	1104	1107	1113	rBV3	447	489	0.03%	0.004%
26	4.671	1125	1129	1132	rBV3	487	390	0.03%	0.004%
27	4.693	1132	1136	1137	rVB2	493	335	0.02%	0.003%
28	4.796	1165	1168	1171	rVB3	467	225	0.01%	0.002%
29	4.838	1173	1181	1185	rBV3	370	437	0.03%	0.004%
30	4.860	1185	1188	1190	rBV2	489	295	0.02%	0.003%
31	4.963	1216	1220	1225	rBV4	407	409	0.03%	0.004%
32	5.047	1229	1246	1288	rBV2	596491	1540252	100.00%	13.953%
33	5.372	1344	1347	1352	rVB3	480	433	0.03%	0.004%
34	5.507	1385	1389	1391	rBV3	405	287	0.02%	0.003%
35	5.552	1401	1403	1405	rVB2	310	125	0.01%	0.001%
36	5.619	1411	1424	1462	rBV	376700	772558	50.16%	6.999%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025973.D
 Acq On : 27 May 2022 12:37
 Operator : SY/MD
 Sample : VV0527WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.912	1504	1515	1532	rBV3	12398	26948	1.75%	0.244%
38	6.069	1550	1564	1591	rBV	341982	703934	45.70%	6.377%
39	6.294	1632	1634	1635	rBV	296	108	0.01%	0.001%
40	6.336	1642	1647	1650	rBV2	401	347	0.02%	0.003%
41	6.481	1690	1692	1697	rVB3	267	267	0.02%	0.002%
42	6.523	1701	1705	1710	rBV4	523	446	0.03%	0.004%
43	6.574	1718	1721	1722	rBV	313	142	0.01%	0.001%
44	6.664	1745	1749	1751	rBV2	303	246	0.02%	0.002%
45	6.677	1751	1753	1755	rBV2	209	104	0.01%	0.001%
46	6.738	1770	1772	1773	rBV2	264	115	0.01%	0.001%
47	6.780	1783	1785	1788	rVB2	397	213	0.01%	0.002%
48	6.812	1793	1795	1796	rBV2	232	71	0.00%	0.001%
49	6.841	1802	1804	1810	rVB2	472	345	0.02%	0.003%
50	6.867	1810	1812	1813	rBV2	434	209	0.01%	0.002%
51	6.986	1838	1849	1874	rBV	164072	302545	19.64%	2.741%
52	7.317	1939	1952	1973	rBV	690362	1204377	78.19%	10.911%
53	7.622	2037	2047	2071	rBV	110004	201569	13.09%	1.826%
54	7.831	2110	2112	2114	rVB2	548	289	0.02%	0.003%
55	7.844	2114	2116	2117	rBV	354	179	0.01%	0.002%
56	7.931	2138	2143	2146	rBV3	720	646	0.04%	0.006%
57	8.021	2168	2171	2172	rBV	400	120	0.01%	0.001%
58	8.034	2172	2175	2176	rBV	174	103	0.01%	0.001%
59	8.040	2176	2177	2180	rBB2	458	142	0.01%	0.001%
60	8.092	2183	2193	2230	rBV	283992	633710	41.14%	5.741%
61	8.416	2289	2294	2296	rBV3	715	649	0.04%	0.006%
62	8.680	2371	2376	2377	rBV2	256	180	0.01%	0.002%
63	8.696	2377	2381	2383	rBV3	526	327	0.02%	0.003%
64	8.780	2405	2407	2410	rVB2	216	104	0.01%	0.001%
65	8.805	2413	2415	2417	rBV	208	100	0.01%	0.001%
66	8.850	2418	2429	2456	rBV	590815	972928	63.17%	8.814%
67	9.095	2503	2505	2508	rBV3	476	305	0.02%	0.003%
68	9.211	2538	2541	2543	rBV2	454	367	0.02%	0.003%
69	9.275	2559	2561	2563	rBV2	266	163	0.01%	0.001%
70	9.342	2579	2582	2585	rBV3	601	307	0.02%	0.003%
71	9.420	2604	2606	2607	rBV	189	66	0.00%	0.001%
72	9.548	2642	2646	2649	rBV3	552	507	0.03%	0.005%
73	9.625	2668	2670	2675	rVB3	412	283	0.02%	0.003%
74	9.686	2686	2689	2691	rBV2	445	208	0.01%	0.002%
75	9.706	2693	2695	2698	rVB	237	101	0.01%	0.001%
76	9.725	2699	2701	2702	rBV	330	129	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025973.D
 Acq On : 27 May 2022 12:37
 Operator : SY/MD
 Sample : VV0527WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.764	2708	2713	2716	rBV3	405	345	0.02%	0.003%
78	9.815	2725	2729	2731	rBV3	394	333	0.02%	0.003%
79	9.966	2774	2776	2778	rBV	173	105	0.01%	0.001%
80	10.127	2817	2826	2838	rVB6	2688	4621	0.30%	0.042%
81	10.172	2838	2840	2841	rBV	303	105	0.01%	0.001%
82	10.214	2841	2853	2873	rBV	452842	715078	46.43%	6.478%
83	10.426	2916	2919	2922	rBV2	340	223	0.01%	0.002%
84	10.477	2932	2935	2938	rBV2	384	259	0.02%	0.002%
85	10.680	2996	2998	3001	rBV2	257	181	0.01%	0.002%
86	10.693	3001	3002	3004	rVV2	310	105	0.01%	0.001%
87	10.780	3026	3029	3030	rBV2	341	180	0.01%	0.002%
88	10.838	3044	3047	3050	rVB2	403	225	0.01%	0.002%
89	10.854	3050	3052	3055	rBV	287	225	0.01%	0.002%
90	10.918	3067	3072	3083	rVB7	3022	4530	0.29%	0.041%
91	11.027	3100	3106	3108	rBV4	465	547	0.04%	0.005%
92	11.143	3136	3142	3149	rBV8	1484	2434	0.16%	0.022%
93	11.246	3164	3174	3194	rBV	569273	885240	57.47%	8.019%
94	11.622	3278	3291	3313	rBV	664299	1041772	67.64%	9.437%
95	12.005	3408	3410	3416	rBV3	421	303	0.02%	0.003%
96	12.278	3493	3495	3501	rVB3	489	327	0.02%	0.003%
97	12.329	3509	3511	3513	rBV2	425	267	0.02%	0.002%
98	13.506	3871	3877	3884	rBV2	4445	6378	0.41%	0.058%
99	13.718	3941	3943	3946	rBV	391	255	0.02%	0.002%
100	13.747	3946	3952	3962	rVB5	2968	4205	0.27%	0.038%




Sum of corrected areas: 11038674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025973.D
Acq On : 27 May 2022 12:37
Operator : SY/MD
Sample : VV0527WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

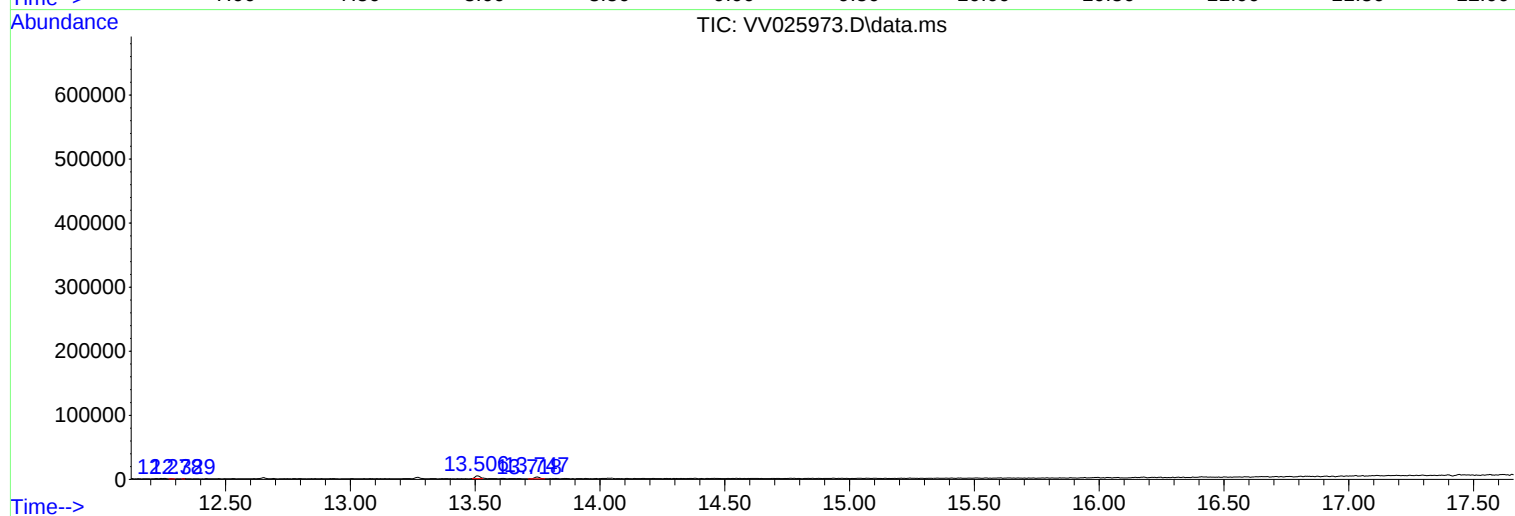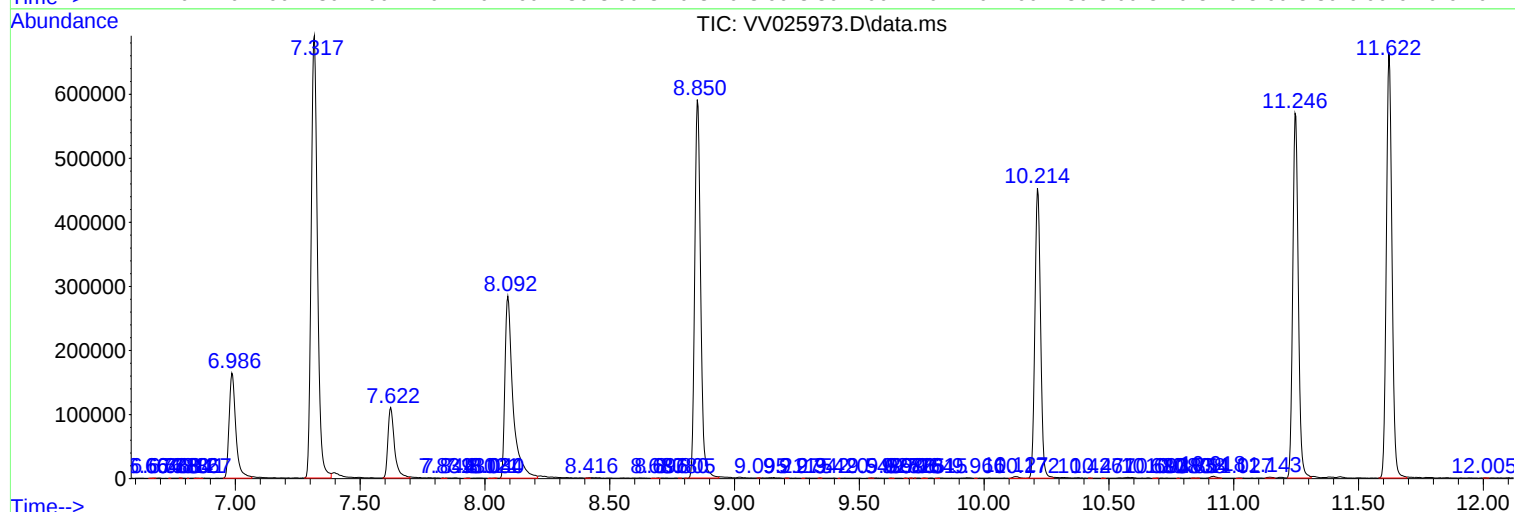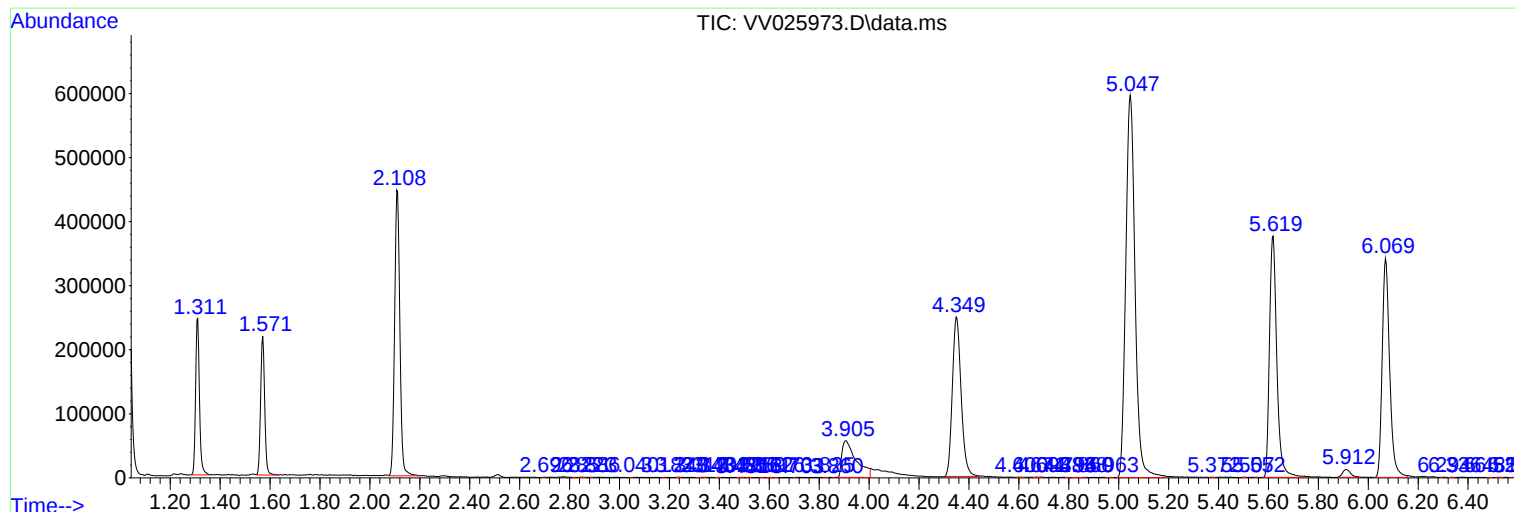

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025973.D
Acq On : 27 May 2022 12:37
Operator : SY/MD
Sample : VV0527WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025973.D
Acq On : 27 May 2022 12:37
Operator : SY/MD
Sample : VV0527WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc