

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025974.D
 Acq On : 27 May 2022 13:03
 Operator : SY/MD
 Sample : N3039-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rBV	256956	263073	16.88%	2.404%
2	1.571	157	165	179	rVB	220146	246607	15.83%	2.253%
3	2.108	322	332	356	rVB	474247	677267	43.46%	6.189%
4	2.507	451	456	465	rVB7	1411	2148	0.14%	0.020%
5	2.699	514	516	519	rBV2	374	187	0.01%	0.002%
6	2.793	541	545	548	rBV4	562	431	0.03%	0.004%
7	2.835	555	558	560	rVB2	289	153	0.01%	0.001%
8	2.851	560	563	564	rBV	293	154	0.01%	0.001%
9	2.921	583	585	589	rVB2	353	177	0.01%	0.002%
10	2.973	597	601	602	rBV2	335	150	0.01%	0.001%
11	2.989	602	606	608	rVV	330	189	0.01%	0.002%
12	3.005	608	611	614	rVB2	325	217	0.01%	0.002%
13	3.034	617	620	623	rBV3	277	206	0.01%	0.002%
14	3.050	623	625	628	rVB2	418	167	0.01%	0.002%
15	3.082	631	635	636	rBV	339	183	0.01%	0.002%
16	3.317	701	708	713	rBV2	347	428	0.03%	0.004%
17	3.391	729	731	737	rVB3	347	329	0.02%	0.003%
18	3.552	778	781	783	rBV2	297	186	0.01%	0.002%
19	3.738	836	839	842	rVV2	307	241	0.02%	0.002%
20	3.767	845	848	853	rVB3	393	328	0.02%	0.003%
21	3.809	858	861	865	rBV2	231	157	0.01%	0.001%
22	3.834	865	869	873	rVB2	486	345	0.02%	0.003%
23	3.863	873	878	879	rBV3	508	340	0.02%	0.003%
24	3.908	881	892	918	rBV2	57629	241591	15.50%	2.208%
25	4.349	1014	1029	1059	rBV	251037	619989	39.79%	5.665%
26	4.625	1112	1115	1118	rBV3	543	273	0.02%	0.002%
27	4.712	1140	1142	1145	rBV	459	243	0.02%	0.002%
28	4.767	1155	1159	1165	rVB4	630	477	0.03%	0.004%
29	4.796	1165	1168	1172	rBV3	271	269	0.02%	0.002%
30	5.043	1225	1245	1274	rBV2	609711	1558283	100.00%	14.239%
31	5.400	1354	1356	1359	rBV	395	231	0.01%	0.002%
32	5.468	1375	1377	1380	rBV2	260	157	0.01%	0.001%
33	5.510	1386	1390	1394	rBV3	507	471	0.03%	0.004%
34	5.551	1399	1403	1406	rBV2	475	312	0.02%	0.003%
35	5.616	1411	1423	1453	rBV	365537	743461	47.71%	6.794%
36	5.908	1503	1514	1531	rBV4	14414	32820	2.11%	0.300%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025974.D
 Acq On : 27 May 2022 13:03
 Operator : SY/MD
 Sample : N3039-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.998	1540	1542	1544	rVB	363	169	0.01%	0.002%
38	6.018	1544	1548	1550	rBV3	410	333	0.02%	0.003%
39	6.069	1550	1564	1595	rBV	344847	710915	45.62%	6.496%
40	6.304	1635	1637	1640	rBV2	330	166	0.01%	0.002%
41	6.391	1660	1664	1669	rBV2	294	267	0.02%	0.002%
42	6.426	1673	1675	1680	rBV4	252	239	0.02%	0.002%
43	6.522	1702	1705	1709	rVB3	408	239	0.02%	0.002%
44	6.551	1713	1714	1717	rVV	297	179	0.01%	0.002%
45	6.584	1721	1724	1727	rVB2	589	288	0.02%	0.003%
46	6.606	1727	1731	1732	rVB	303	181	0.01%	0.002%
47	6.629	1735	1738	1739	rBV	305	193	0.01%	0.002%
48	6.654	1743	1746	1748	rBV	322	227	0.01%	0.002%
49	6.812	1792	1795	1801	rVB2	332	224	0.01%	0.002%
50	6.844	1802	1805	1808	rVV	255	162	0.01%	0.001%
51	6.870	1808	1813	1817	rVV2	410	323	0.02%	0.003%
52	6.985	1838	1849	1878	rBV	160705	303367	19.47%	2.772%
53	7.207	1916	1918	1919	rBV2	610	237	0.02%	0.002%
54	7.246	1927	1930	1931	rBV2	521	294	0.02%	0.003%
55	7.313	1940	1951	1971	rBV	701394	1222111	78.43%	11.167%
56	7.622	2037	2047	2065	rBV	109776	195737	12.56%	1.789%
57	7.866	2120	2123	2128	rBV2	681	586	0.04%	0.005%
58	7.940	2137	2146	2157	rBV3	3208	5505	0.35%	0.050%
59	7.982	2157	2159	2164	rVB3	731	440	0.03%	0.004%
60	8.011	2164	2168	2170	rBV	287	184	0.01%	0.002%
61	8.030	2173	2174	2177	rVB	376	154	0.01%	0.001%
62	8.047	2177	2179	2183	rBV3	339	290	0.02%	0.003%
63	8.092	2183	2193	2229	rBV	256503	566669	36.36%	5.178%
64	8.481	2312	2314	2318	rBV3	610	361	0.02%	0.003%
65	8.538	2330	2332	2335	rBV	331	217	0.01%	0.002%
66	8.577	2339	2344	2346	rBV3	441	378	0.02%	0.003%
67	8.612	2352	2355	2358	rBV2	539	350	0.02%	0.003%
68	8.680	2372	2376	2378	rBV2	279	185	0.01%	0.002%
69	8.776	2403	2406	2407	rBV	387	217	0.01%	0.002%
70	8.850	2418	2429	2458	rBV	567661	937255	60.15%	8.564%
71	9.088	2501	2503	2506	rBV2	536	249	0.02%	0.002%
72	9.153	2521	2523	2527	rBV2	538	377	0.02%	0.003%
73	9.442	2611	2613	2616	rBV2	475	304	0.02%	0.003%
74	9.548	2643	2646	2647	rBV2	454	211	0.01%	0.002%
75	9.577	2653	2655	2658	rBV2	286	160	0.01%	0.001%
76	9.831	2729	2734	2735	rBV2	250	175	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025974.D
 Acq On : 27 May 2022 13:03
 Operator : SY/MD
 Sample : N3039-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.940	2766	2768	2771	rBV2	288	165	0.01%	0.002%
78	10.066	2804	2807	2811	rBV2	266	255	0.02%	0.002%
79	10.085	2811	2813	2815	rBV3	305	182	0.01%	0.002%
80	10.172	2838	2840	2841	rBV	432	174	0.01%	0.002%
81	10.214	2842	2853	2875	rVV	440927	681764	43.75%	6.230%
82	10.426	2917	2919	2921	rVB	506	218	0.01%	0.002%
83	10.484	2935	2937	2939	rBV2	333	160	0.01%	0.001%
84	10.497	2939	2941	2944	rVV	309	175	0.01%	0.002%
85	10.561	2952	2961	2962	rBV4	474	616	0.04%	0.006%
86	10.821	3039	3042	3045	rBV3	507	318	0.02%	0.003%
87	10.870	3055	3057	3061	rVB3	681	396	0.03%	0.004%
88	10.918	3063	3072	3077	rBV5	2796	4017	0.26%	0.037%
89	11.024	3102	3105	3107	rBV	477	290	0.02%	0.003%
90	11.143	3137	3142	3148	rVB3	1314	1536	0.10%	0.014%
91	11.178	3151	3153	3154	rBV	420	162	0.01%	0.001%
92	11.249	3163	3175	3201	rBV	549388	855736	54.92%	7.819%
93	11.622	3279	3291	3316	rBV	673476	1051177	67.46%	9.605%
94	12.130	3447	3449	3451	rBV3	375	201	0.01%	0.002%
95	12.651	3607	3611	3618	rBV4	668	774	0.05%	0.007%
96	12.715	3629	3631	3635	rVB2	432	192	0.01%	0.002%
97	12.985	3710	3715	3717	rBV2	471	406	0.03%	0.004%
98	13.474	3864	3867	3870	rBV3	472	321	0.02%	0.003%
99	13.754	3947	3954	3959	rVB3	1368	1654	0.11%	0.015%
100	14.413	4156	4159	4162	rBV	528	432	0.03%	0.004%


Sum of corrected areas: 10943679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025974.D
Acq On : 27 May 2022 13:03
Operator : SY/MD
Sample : N3039-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

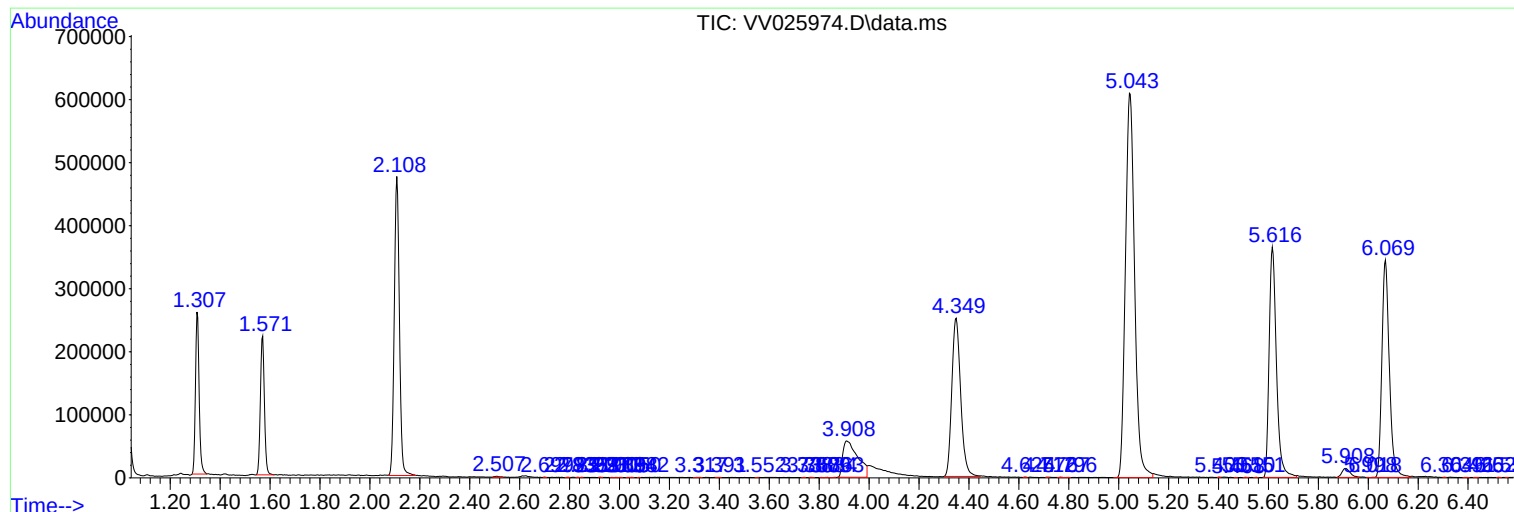

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025974.D
Acq On : 27 May 2022 13:03
Operator : SY/MD
Sample : N3039-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025974.D
Acq On : 27 May 2022 13:03
Operator : SY/MD
Sample : N3039-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc