

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025976.D
 Acq On : 27 May 2022 14:09
 Operator : SY/MD
 Sample : N3039-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rBV	243118	251659	17.18%	2.425%
2	1.568	157	164	179	rVB	212109	236207	16.12%	2.276%
3	2.105	321	331	354	rBV	441385	632516	43.17%	6.095%
4	2.423	425	430	432	rBV3	581	558	0.04%	0.005%
5	2.654	501	502	508	rVB3	635	360	0.02%	0.003%
6	2.680	508	510	513	rBV2	330	230	0.02%	0.002%
7	2.741	526	529	532	rBV2	508	355	0.02%	0.003%
8	2.806	547	549	551	rBV2	274	134	0.01%	0.001%
9	3.121	644	647	650	rBV2	338	259	0.02%	0.002%
10	3.195	667	670	671	rBV	345	151	0.01%	0.001%
11	3.230	678	681	683	rBV2	449	228	0.02%	0.002%
12	3.246	683	686	689	rVB2	467	299	0.02%	0.003%
13	3.262	689	691	696	rVB2	423	273	0.02%	0.003%
14	3.298	698	702	704	rVB3	306	203	0.01%	0.002%
15	3.359	717	721	722	rBV3	271	166	0.01%	0.002%
16	3.384	726	729	732	rBV	413	329	0.02%	0.003%
17	3.429	742	743	750	rVV3	140	131	0.01%	0.001%
18	3.471	753	756	758	rVB	209	135	0.01%	0.001%
19	3.532	769	775	779	rBV3	306	313	0.02%	0.003%
20	3.574	785	788	792	rVB	283	183	0.01%	0.002%
21	3.712	827	831	834	rBV2	245	218	0.01%	0.002%
22	3.777	849	851	854	rVB	342	162	0.01%	0.002%
23	3.796	854	857	859	rBV	365	235	0.02%	0.002%
24	3.841	869	871	874	rBV	189	123	0.01%	0.001%
25	3.854	874	875	879	rVB	303	137	0.01%	0.001%
26	3.899	879	889	915	rBV	54630	202933	13.85%	1.955%
27	4.343	1013	1027	1059	rVB	234699	577730	39.43%	5.567%
28	4.603	1106	1108	1111	rBV3	365	276	0.02%	0.003%
29	4.654	1122	1124	1125	rBV	274	139	0.01%	0.001%
30	4.818	1171	1175	1177	rBV	294	178	0.01%	0.002%
31	4.883	1192	1195	1196	rBV	230	156	0.01%	0.002%
32	4.908	1201	1203	1205	rVB	507	158	0.01%	0.002%
33	5.040	1228	1244	1282	rBV2	570611	1465200	100.00%	14.119%
34	5.355	1339	1342	1343	rBV2	469	201	0.01%	0.002%
35	5.371	1343	1347	1352	rVB4	420	418	0.03%	0.004%
36	5.426	1363	1364	1369	rVV3	367	174	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052722\
 Data File : VW025976.D
 Acq On : 27 May 2022 14:09
 Operator : SY/MD
 Sample : N3039-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.484	1377	1382	1384	rBV4	638	515	0.04%	0.005%
38	5.568	1403	1408	1410	rBV2	322	266	0.02%	0.003%
39	5.613	1410	1422	1445	rBV	357410	718772	49.06%	6.926%
40	5.786	1473	1476	1481	rVB4	968	807	0.06%	0.008%
41	5.905	1501	1513	1533	rBV3	13029	29867	2.04%	0.288%
42	6.066	1549	1563	1592	rBV	322165	668209	45.61%	6.439%
43	6.310	1638	1639	1642	rBV2	287	142	0.01%	0.001%
44	6.400	1665	1667	1671	rBV2	300	218	0.01%	0.002%
45	6.420	1671	1673	1677	rVB2	370	232	0.02%	0.002%
46	6.449	1677	1682	1685	rBV3	335	345	0.02%	0.003%
47	6.487	1691	1694	1696	rVB2	333	190	0.01%	0.002%
48	6.503	1697	1699	1703	rVB2	351	160	0.01%	0.002%
49	6.542	1709	1711	1715	rBV2	363	205	0.01%	0.002%
50	6.680	1753	1754	1761	rVB4	316	260	0.02%	0.003%
51	6.735	1768	1771	1775	rBV2	405	269	0.02%	0.003%
52	6.783	1784	1786	1788	rBV	287	121	0.01%	0.001%
53	6.796	1788	1790	1794	rBV3	256	156	0.01%	0.002%
54	6.857	1808	1809	1812	rVB	378	138	0.01%	0.001%
55	6.982	1838	1848	1877	rVV	151721	284629	19.43%	2.743%
56	7.313	1937	1951	1971	rBV	653604	1140462	77.84%	10.989%
57	7.619	2036	2046	2069	rBV	103855	186227	12.71%	1.794%
58	7.818	2105	2108	2110	rBV2	430	357	0.02%	0.003%
59	7.879	2125	2127	2130	rBV2	472	271	0.02%	0.003%
60	7.912	2133	2137	2139	rBV3	509	375	0.03%	0.004%
61	8.014	2168	2169	2174	rVB	234	166	0.01%	0.002%
62	8.037	2174	2176	2178	rBV	369	155	0.01%	0.001%
63	8.088	2182	2192	2224	rBV	259790	562561	38.39%	5.421%
64	8.387	2283	2285	2288	rBV2	584	332	0.02%	0.003%
65	8.468	2307	2310	2312	rBV	329	235	0.02%	0.002%
66	8.513	2320	2324	2327	rBV2	682	505	0.03%	0.005%
67	8.596	2348	2350	2352	rBV2	315	139	0.01%	0.001%
68	8.683	2374	2377	2381	rBV2	250	141	0.01%	0.001%
69	8.850	2417	2429	2459	rBV	557991	920349	62.81%	8.868%
70	9.117	2510	2512	2513	rBV	417	135	0.01%	0.001%
71	9.175	2528	2530	2533	rBV2	389	243	0.02%	0.002%
72	9.201	2536	2538	2542	rVB2	429	216	0.01%	0.002%
73	9.275	2559	2561	2564	rBV	212	146	0.01%	0.001%
74	9.326	2574	2577	2581	rVB	486	238	0.02%	0.002%
75	9.384	2591	2595	2597	rBV	356	230	0.02%	0.002%
76	9.429	2606	2609	2613	rBV2	432	299	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
 Data File : VV025976.D
 Acq On : 27 May 2022 14:09
 Operator : SY/MD
 Sample : N3039-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.471	2618	2622	2625	rBV	447	323	0.02%	0.003%
78	9.529	2636	2640	2644	rBV2	412	443	0.03%	0.004%
79	9.683	2687	2688	2691	rBV	210	134	0.01%	0.001%
80	9.860	2740	2743	2745	rBV	275	158	0.01%	0.002%
81	9.908	2755	2758	2759	rBV	316	135	0.01%	0.001%
82	9.992	2782	2784	2787	rBV2	538	233	0.02%	0.002%
83	10.008	2787	2789	2795	rVB3	423	258	0.02%	0.002%
84	10.124	2815	2825	2836	rBV7	2750	4734	0.32%	0.046%
85	10.214	2839	2853	2870	rBV	421776	660535	45.08%	6.365%
86	10.567	2959	2963	2964	rBV2	830	542	0.04%	0.005%
87	10.641	2984	2986	2990	rBV2	284	165	0.01%	0.002%
88	10.657	2990	2991	2997	rVB2	630	310	0.02%	0.003%
89	10.690	2998	3001	3003	rBV2	425	301	0.02%	0.003%
90	10.718	3008	3010	3014	rBV2	351	273	0.02%	0.003%
91	10.821	3039	3042	3043	rBV2	359	204	0.01%	0.002%
92	10.854	3049	3052	3054	rBV2	725	401	0.03%	0.004%
93	10.998	3093	3097	3100	rBV2	353	246	0.02%	0.002%
94	11.140	3136	3141	3149	rVB6	1277	1769	0.12%	0.017%
95	11.191	3154	3157	3160	rBV2	717	502	0.03%	0.005%
96	11.246	3163	3174	3202	rBV	540231	838742	57.24%	8.082%
97	11.622	3279	3291	3316	rBV	631487	973691	66.45%	9.382%
98	11.844	3356	3360	3362	rBV2	757	599	0.04%	0.006%
99	12.236	3479	3482	3484	rBV2	528	403	0.03%	0.004%
100	13.361	3829	3832	3834	rBV2	473	323	0.02%	0.003%




Sum of corrected areas: 10377834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025976.D
Acq On : 27 May 2022 14:09
Operator : SY/MD
Sample : N3039-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

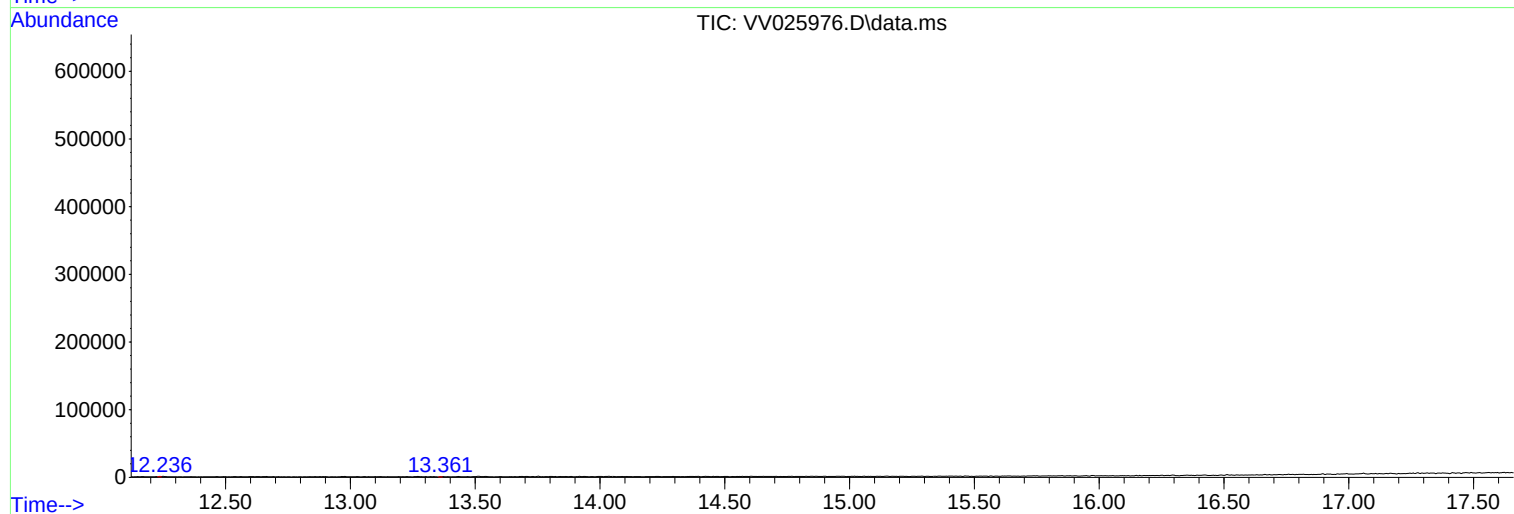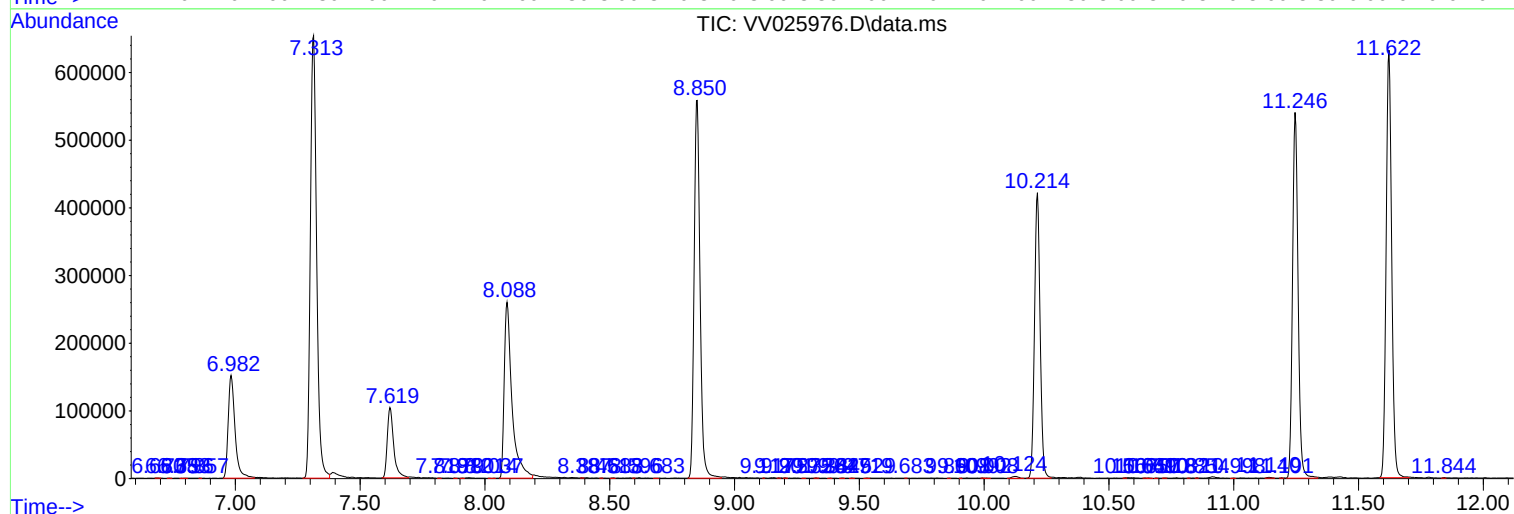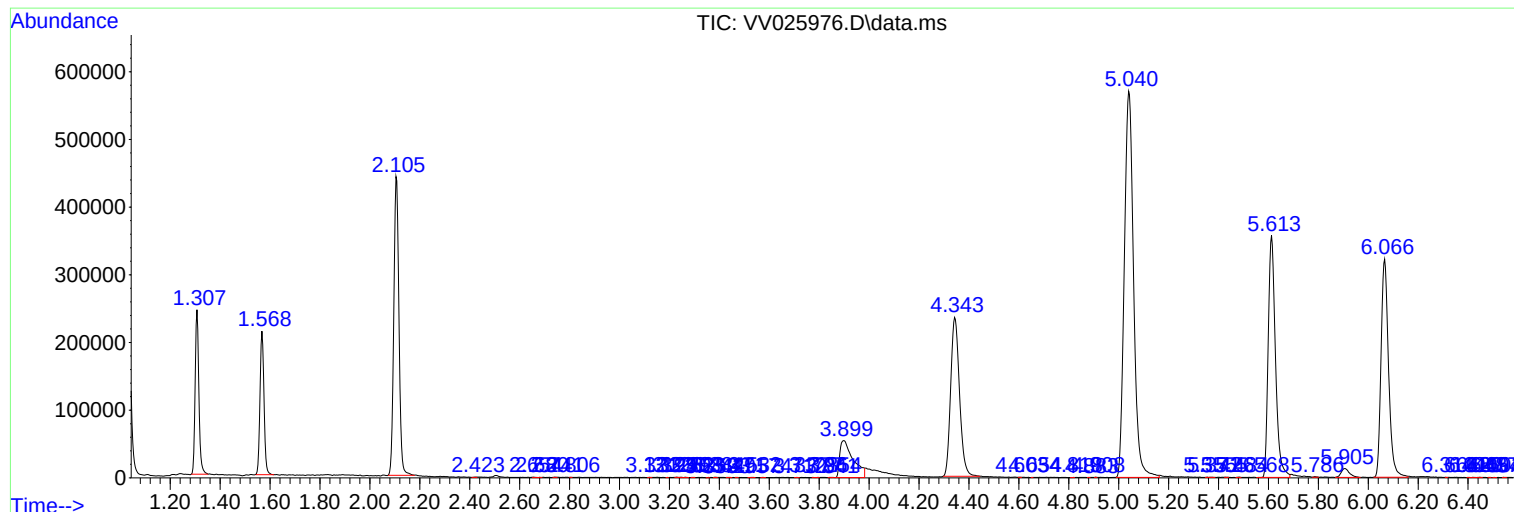

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025976.D
Acq On : 27 May 2022 14:09
Operator : SY/MD
Sample : N3039-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025976.D
Acq On : 27 May 2022 14:09
Operator : SY/MD
Sample : N3039-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc