


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052722\
Data File : VV025970.D
Acq On : 27 May 2022 08:53
Operator : SY/MD
Sample : BFB284
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB284

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Title : VOC Analysis
Last Update : Fri May 27 22:34:02 2022

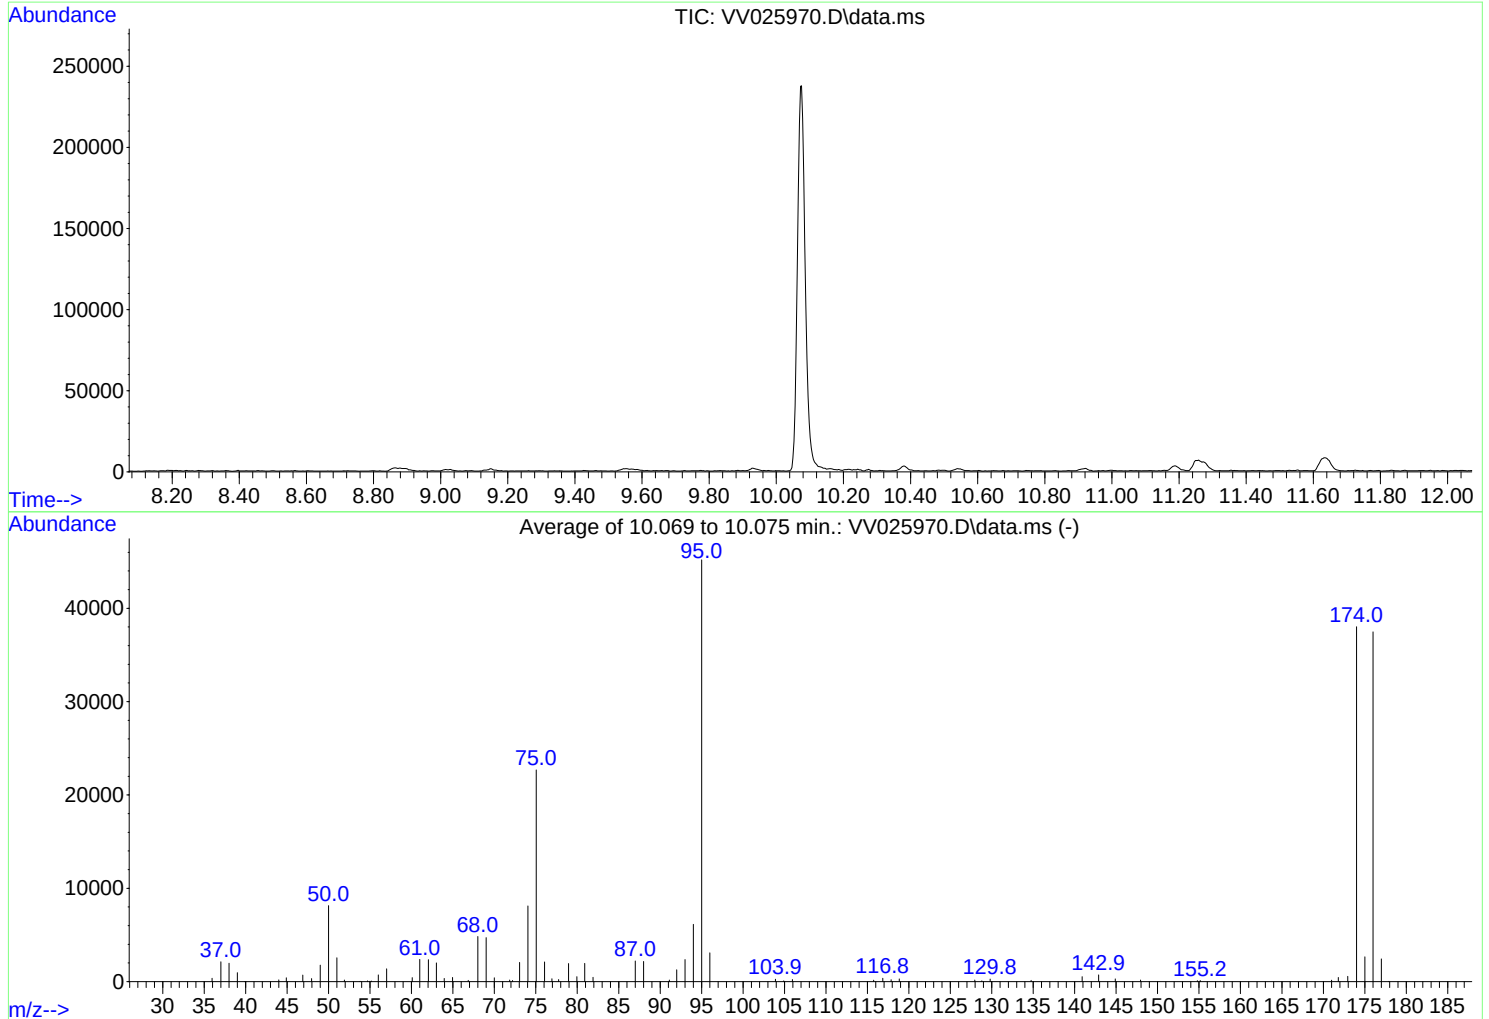

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	8142	PASS
75	95	30	80	50.2	22683	PASS
95	95	100	100	100.0	45192	PASS
96	95	5	9	6.8	3088	PASS
173	174	0.00	2	1.5	575	PASS
174	95	50	120	84.1	38024	PASS
175	174	5	9	7.0	2664	PASS
176	174	95	105	98.5	37469	PASS
177	176	5	10	6.5	2443	PASS

m/z	Abundance
40.00	257.0
44.00	418.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	360.0
37.00	2078.0
38.00	1765.0
39.00	850.0
39.90	255.0
44.00	650.0
44.90	325.0
46.90	624.0
48.00	290.0
49.00	1710.0
50.00	7924.0
51.00	2417.0
51.90	149.0
54.70	125.0
55.20	120.0
56.00	672.0
57.00	1352.0
60.10	418.0
61.00	2246.0
62.10	2248.0
63.00	1894.0
63.90	318.0
64.90	469.0
66.90	123.0
68.00	4551.0
69.00	4511.0
70.00	387.0
71.80	155.0
72.20	201.0
73.00	1935.0
74.00	7642.0
75.00	21344.0
76.00	2000.0
76.90	327.0
77.70	276.0
79.00	1665.0
79.90	472.0
80.90	1810.0
81.90	429.0
87.00	2092.0
88.00	1972.0
91.10	186.0
92.00	1099.0
93.00	2358.0
94.00	5623.0
95.00	42576.0
96.00	3051.0
103.90	275.0
106.00	195.0
115.70	128.0
116.90	338.0
117.90	188.0
118.80	286.0
127.90	154.0
129.80	257.0
134.80	126.0
140.90	499.0
142.90	614.0
144.90	272.0
147.90	169.0
154.80	107.0
155.20	134.0
171.00	147.0
171.80	421.0
172.90	431.0
174.00	34672.0
175.00	2570.0
176.00	34144.0
177.00	2399.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	359.0
37.00	2187.0
38.00	2012.0
39.00	1006.0
39.90	256.0
44.00	599.0
44.90	434.0
46.90	737.0
47.90	341.0
49.00	1819.0
50.00	8397.0
51.00	2573.0
51.90	177.0
54.70	109.0
55.10	101.0
56.00	769.0
57.00	1417.0
60.10	449.0
61.00	2452.0
62.10	2394.0
63.00	2040.0
64.00	336.0
65.00	463.0
66.80	153.0
68.00	5038.0
69.00	4807.0
70.00	408.0
71.80	183.0
72.20	179.0
73.00	2101.0
74.10	8497.0
75.00	23312.0
76.00	2163.0
77.00	308.0
77.70	234.0
78.90	1987.0
80.00	538.0
80.90	2004.0
81.90	456.0
87.00	2283.0
88.00	2295.0
91.10	183.0
92.00	1302.0
93.00	2494.0
94.00	6334.0
95.00	46712.0
96.00	3222.0
103.90	259.0
104.90	115.0
105.90	227.0
115.70	144.0
116.90	385.0
117.80	212.0
118.80	306.0
128.00	181.0
128.80	118.0
129.80	292.0
134.70	143.0
140.90	557.0
142.90	773.0
144.90	314.0
147.90	170.0
154.80	109.0
155.20	136.0
171.00	162.0
171.80	455.0
173.00	585.0
174.00	39296.0
175.00	2752.0
176.00	38736.0
177.00	2555.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
35.90	368.0
37.00	2117.0
38.00	2160.0
39.00	1001.0
39.90	271.0
44.00	553.0
44.90	472.0
46.90	767.0
47.90	329.0
49.00	1775.0
50.00	8104.0
51.00	2696.0
51.90	170.0
53.80	116.0
54.90	110.0
56.00	742.0
57.00	1335.0
60.10	443.0
61.00	2447.0
62.00	2417.0
63.00	2067.0
64.00	366.0
64.90	425.0
66.80	134.0
68.00	4928.0
69.00	4836.0
70.00	432.0
71.90	184.0
73.10	2152.0
74.00	8213.0
75.10	23392.0
76.10	2188.0
77.00	293.0
77.80	177.0
78.90	2178.0
80.00	576.0
80.90	2076.0
81.90	483.0
87.00	2240.0
88.00	2218.0
91.10	154.0
92.00	1408.0
93.00	2266.0
94.00	6433.0
95.00	46288.0
96.00	2991.0
103.90	221.0
104.90	124.0
105.90	242.0
115.80	178.0
116.80	384.0
117.80	218.0
118.90	285.0
128.00	197.0
128.80	145.0
129.80	280.0
134.70	138.0
140.90	559.0
142.90	795.0
144.90	313.0
148.00	178.0
154.80	117.0
155.10	113.0
171.00	155.0
171.80	477.0
173.00	709.0
174.00	40104.0
175.00	2670.0
176.00	39528.0
177.00	2375.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284