

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060822\
 Data File : VW026026.D
 Acq On : 08 Jun 2022 17:25
 Operator : SY/MD
 Sample : N3188-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B04

Quant Time: Jun 09 05:23:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 09 05:13:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	182387	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	174891	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71467	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	50175	4.686	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.800%	
7) Chloroethane-d5	1.580	69	54500	4.869	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	97.400%	
11) 1,1-Dichloroethene-d2	2.121	63	80013	3.235	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.800%	
20) 2-Butanone-d5	3.915	46	82259	51.947	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.900%	
24) Chloroform-d	4.362	84	112244	4.947	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.000%	
26) 1,2-Dichloroethane-d4	5.043	65	48785	5.271	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
32) Benzene-d6	5.059	84	202911	4.801	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6	6.075	67	66806	5.110	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.200%	
41) Toluene-d8	7.320	98	163906	4.389	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.800%	
43) trans-1,3-Dichloroprop...	7.632	79	16275	4.228	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.600%	
46) 2-Hexanone-d5	8.091	63	73880	43.614	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.220%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40870	4.636	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	58917	5.388	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.800%	
Target Compounds						
16) Methylene chloride	2.523	84	3316	0.227	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026026.D
Acq On : 08 Jun 2022 17:25
Operator : SY/MD
Sample : N3188-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B04


Quant Time: Jun 09 05:23:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 09 05:13:00 2022
Response via : Initial Calibration

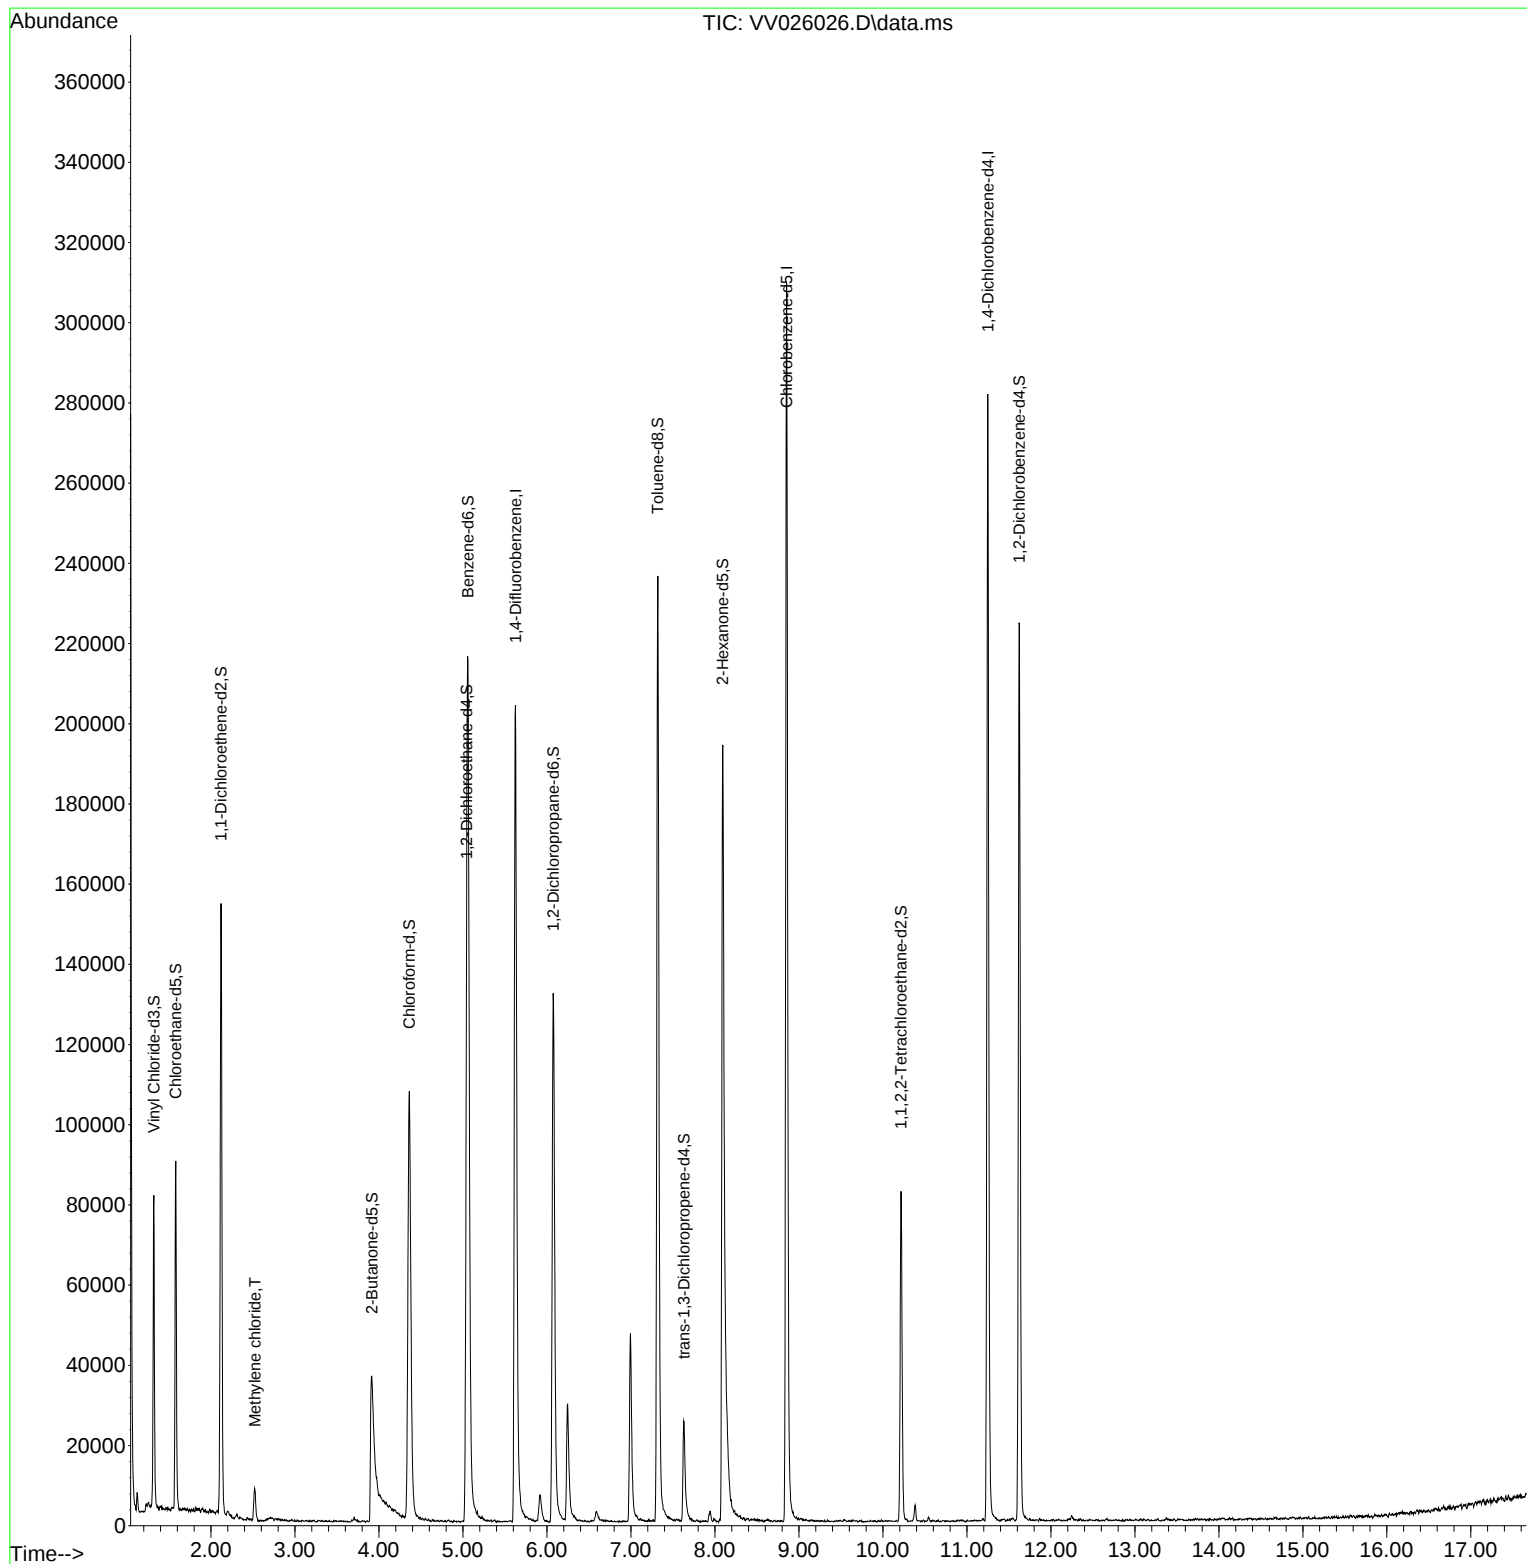

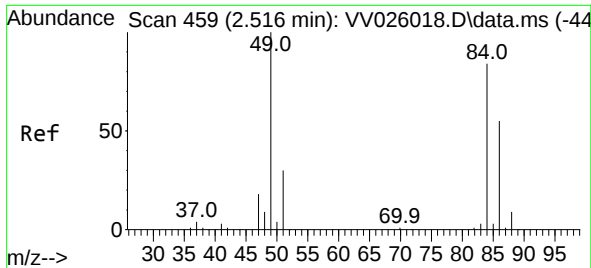

#16
Methylene chloride
Concen: 0.227 ug/L
RT: 2.523 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV026026.D
Acq: 08 Jun 2022 17:25

Instrument :
MSVOA_V
ClientSampleId :
H0B04

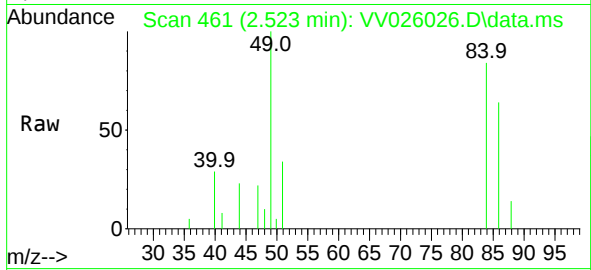

Tgt Ion: 84 Resp: 3316

Ion	Ratio	Lower	Upper
84	100		
86	76.2	45.6	84.6
49	119.4	82.9	153.9

