

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060822\
 Data File : VW026037.D
 Acq On : 08 Jun 2022 21:49
 Operator : SY/MD
 Sample : N3253-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DJ2

Quant Time: Jun 09 05:25:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 09 05:13:00 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	182357	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	174966	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68306	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	48337	4.515	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.400%	
7) Chloroethane-d5	1.581	69	53716	4.800	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.121	63	77028	3.115	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.400%	
20) 2-Butanone-d5	3.918	46	72208	45.608	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	91.220%	
24) Chloroform-d	4.362	84	110895	4.888	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.043	65	46084	4.980	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.600%	
32) Benzene-d6	5.059	84	198331	4.691	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.800%	
36) 1,2-Dichloropropane-d6	6.076	67	66563	5.089	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.800%	
41) Toluene-d8	7.320	98	150902	4.039	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.800%	
43) trans-1,3-Dichloroprop...	7.632	79	15076	3.915	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.200%	
46) 2-Hexanone-d5	8.092	63	71704	42.311	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.620%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41400	4.694	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	54548	5.220	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						
25) Chloroform	4.384	83	10711	0.415	ug/L	93
31) Carbon tetrachloride	4.834	117	14489	0.768	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026037.D
Acq On : 08 Jun 2022 21:49
Operator : SY/MD
Sample : N3253-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DJ2

Quant Time: Jun 09 05:25:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 09 05:13:00 2022
Response via : Initial Calibration

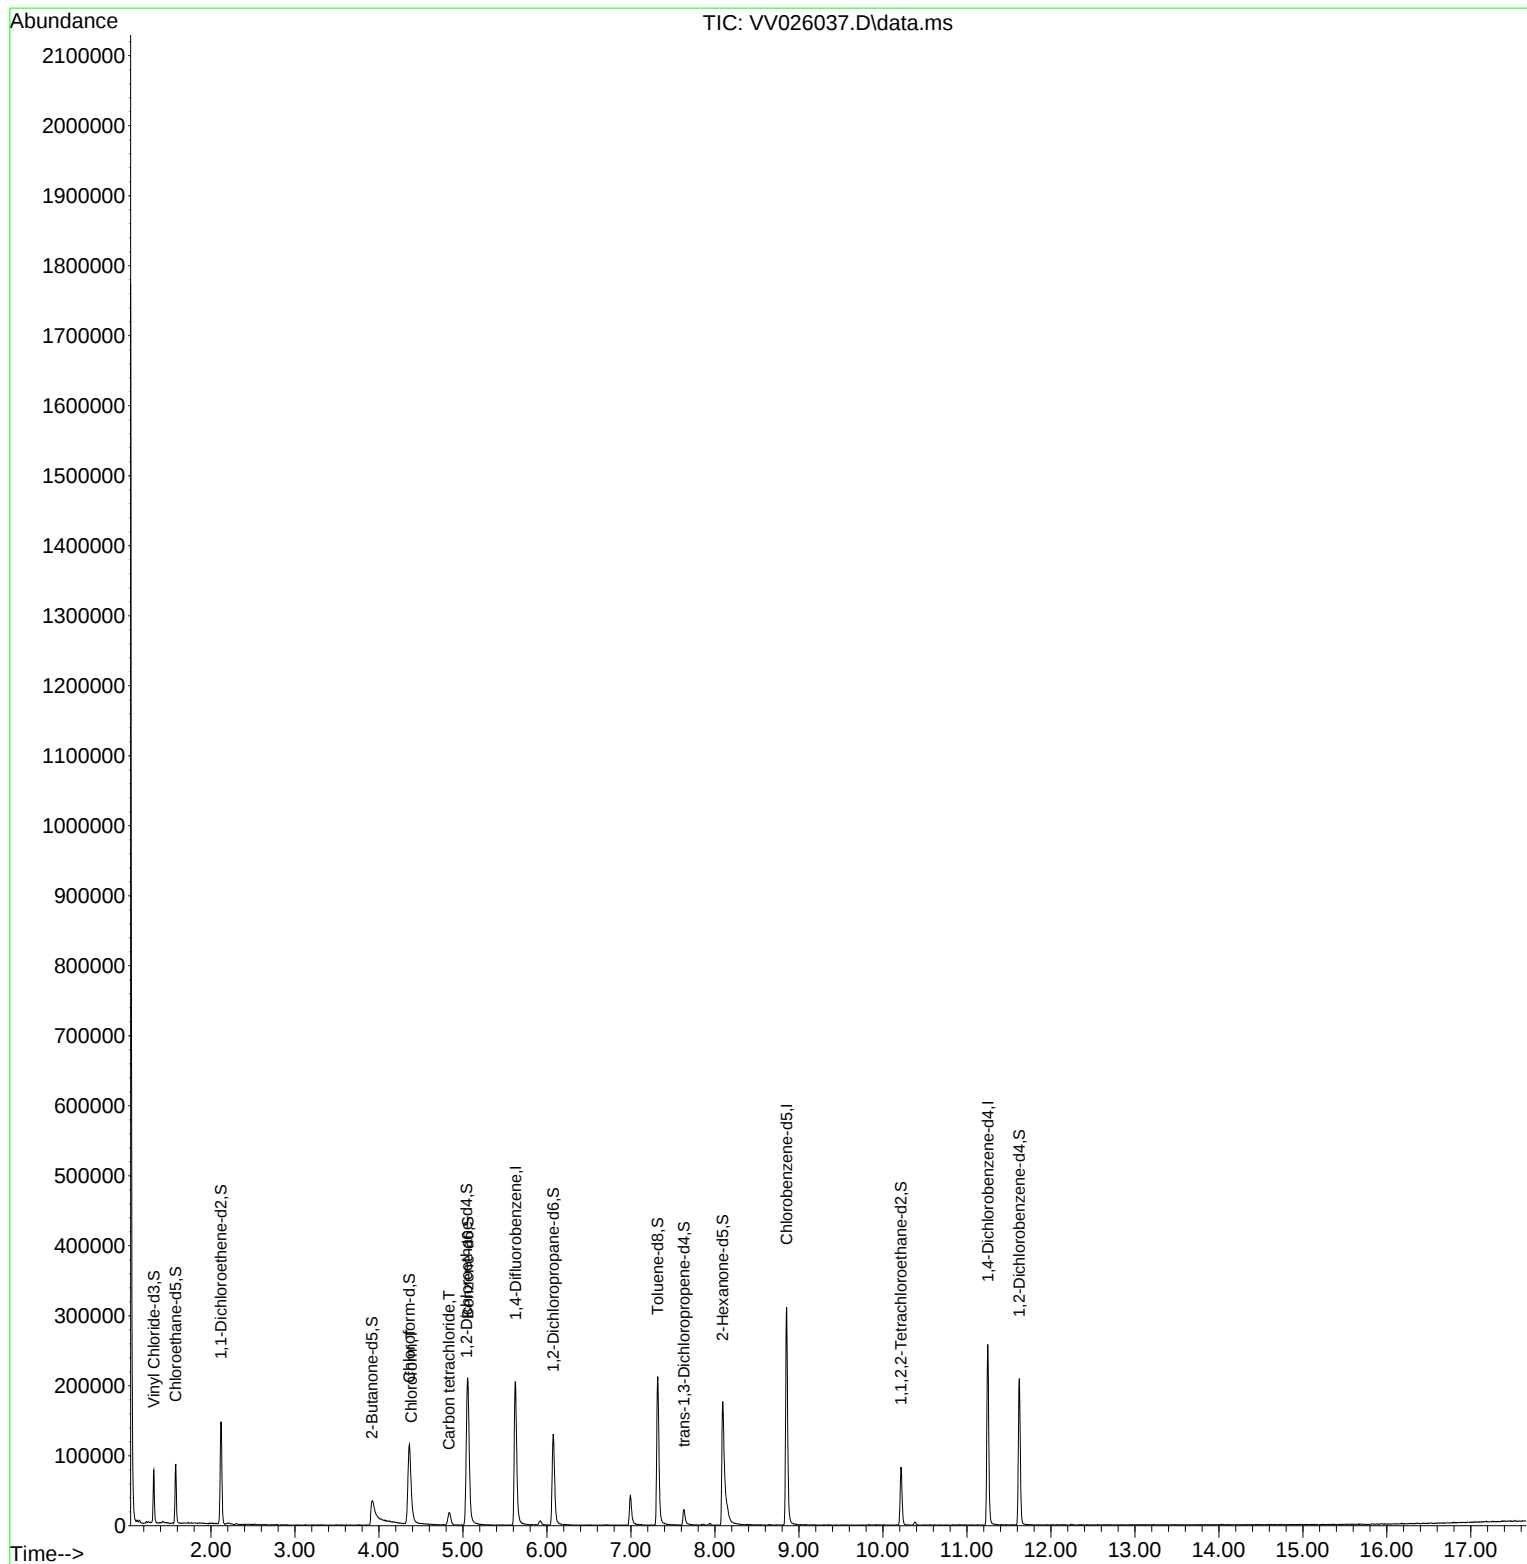

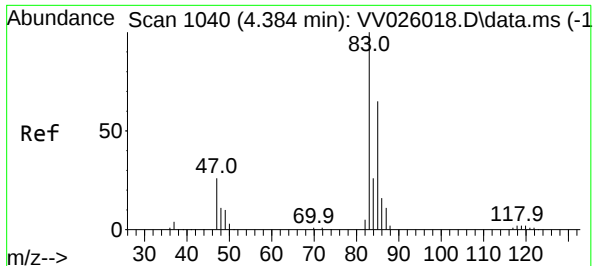

#25

Chloroform

Concen: 0.415 ug/L

RT: 4.384 min Scan# 1107

Delta R.T. 0.000 min

Lab File: VV026037.D

Acq: 08 Jun 2022 21:49

Instrument :

MSVOA_V

ClientSampleId :





C0DJ2

Tgt Ion: 83 Resp: 10711

Ion Ratio Lower Upper

83 100

85 58.8 45.2 84.0

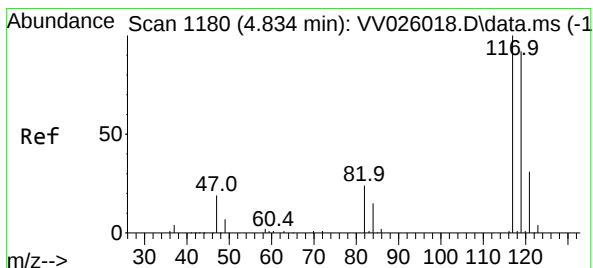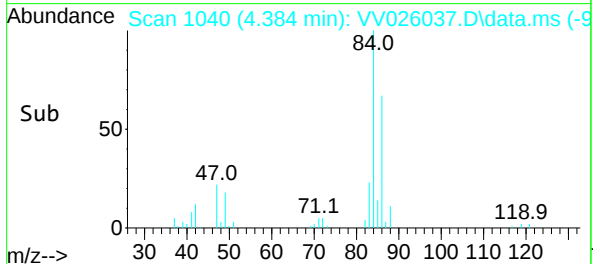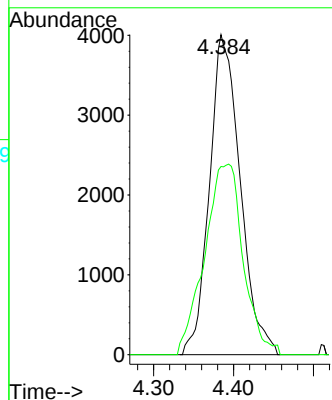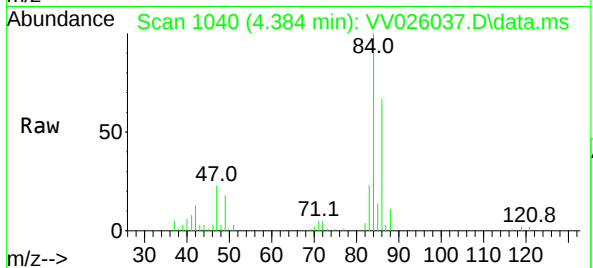

#31

Carbon tetrachloride

Concen: 0.768 ug/L

RT: 4.834 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VV026037.D

Acq: 08 Jun 2022 21:49

Tgt Ion: 117 Resp: 14489

Ion Ratio Lower Upper

117 100

119 89.6 78.7 118.1

