

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060822\
 Data File : VW026038.D
 Acq On : 08 Jun 2022 22:13
 Operator : SY/MD
 Sample : N3253-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DJ5

Quant Time: Jun 09 05:25:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 09 05:13:00 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	182348	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	171358	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69931	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	47498	4.437	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.800%	
7) Chloroethane-d5	1.580	69	53418	4.773	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.400%	
11) 1,1-Dichloroethene-d2	2.121	63	76128	3.079	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.600%	
20) 2-Butanone-d5	3.908	46	72718	45.932	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	91.860%	
24) Chloroform-d	4.362	84	109327	4.819	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	5.043	65	46221	4.995	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.800%	
32) Benzene-d6	5.059	84	200858	4.851	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
36) 1,2-Dichloropropane-d6	6.075	67	65933	5.147	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.000%	
41) Toluene-d8	7.320	98	149021	4.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.400%	
43) trans-1,3-Dichloroprop...	7.628	79	15477	4.104	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.091	63	70483	42.467	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.940%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40130	4.646	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	53733	5.022	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.400%	
Target Compounds						
13) Acetone	2.191	43	13152	10.416	ug/L	83
21) 2-Butanone	4.011	43	13702	8.331	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026038.D
Acq On : 08 Jun 2022 22:13
Operator : SY/MD
Sample : N3253-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DJ5

Quant Time: Jun 09 05:25:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 09 05:13:00 2022
Response via : Initial Calibration




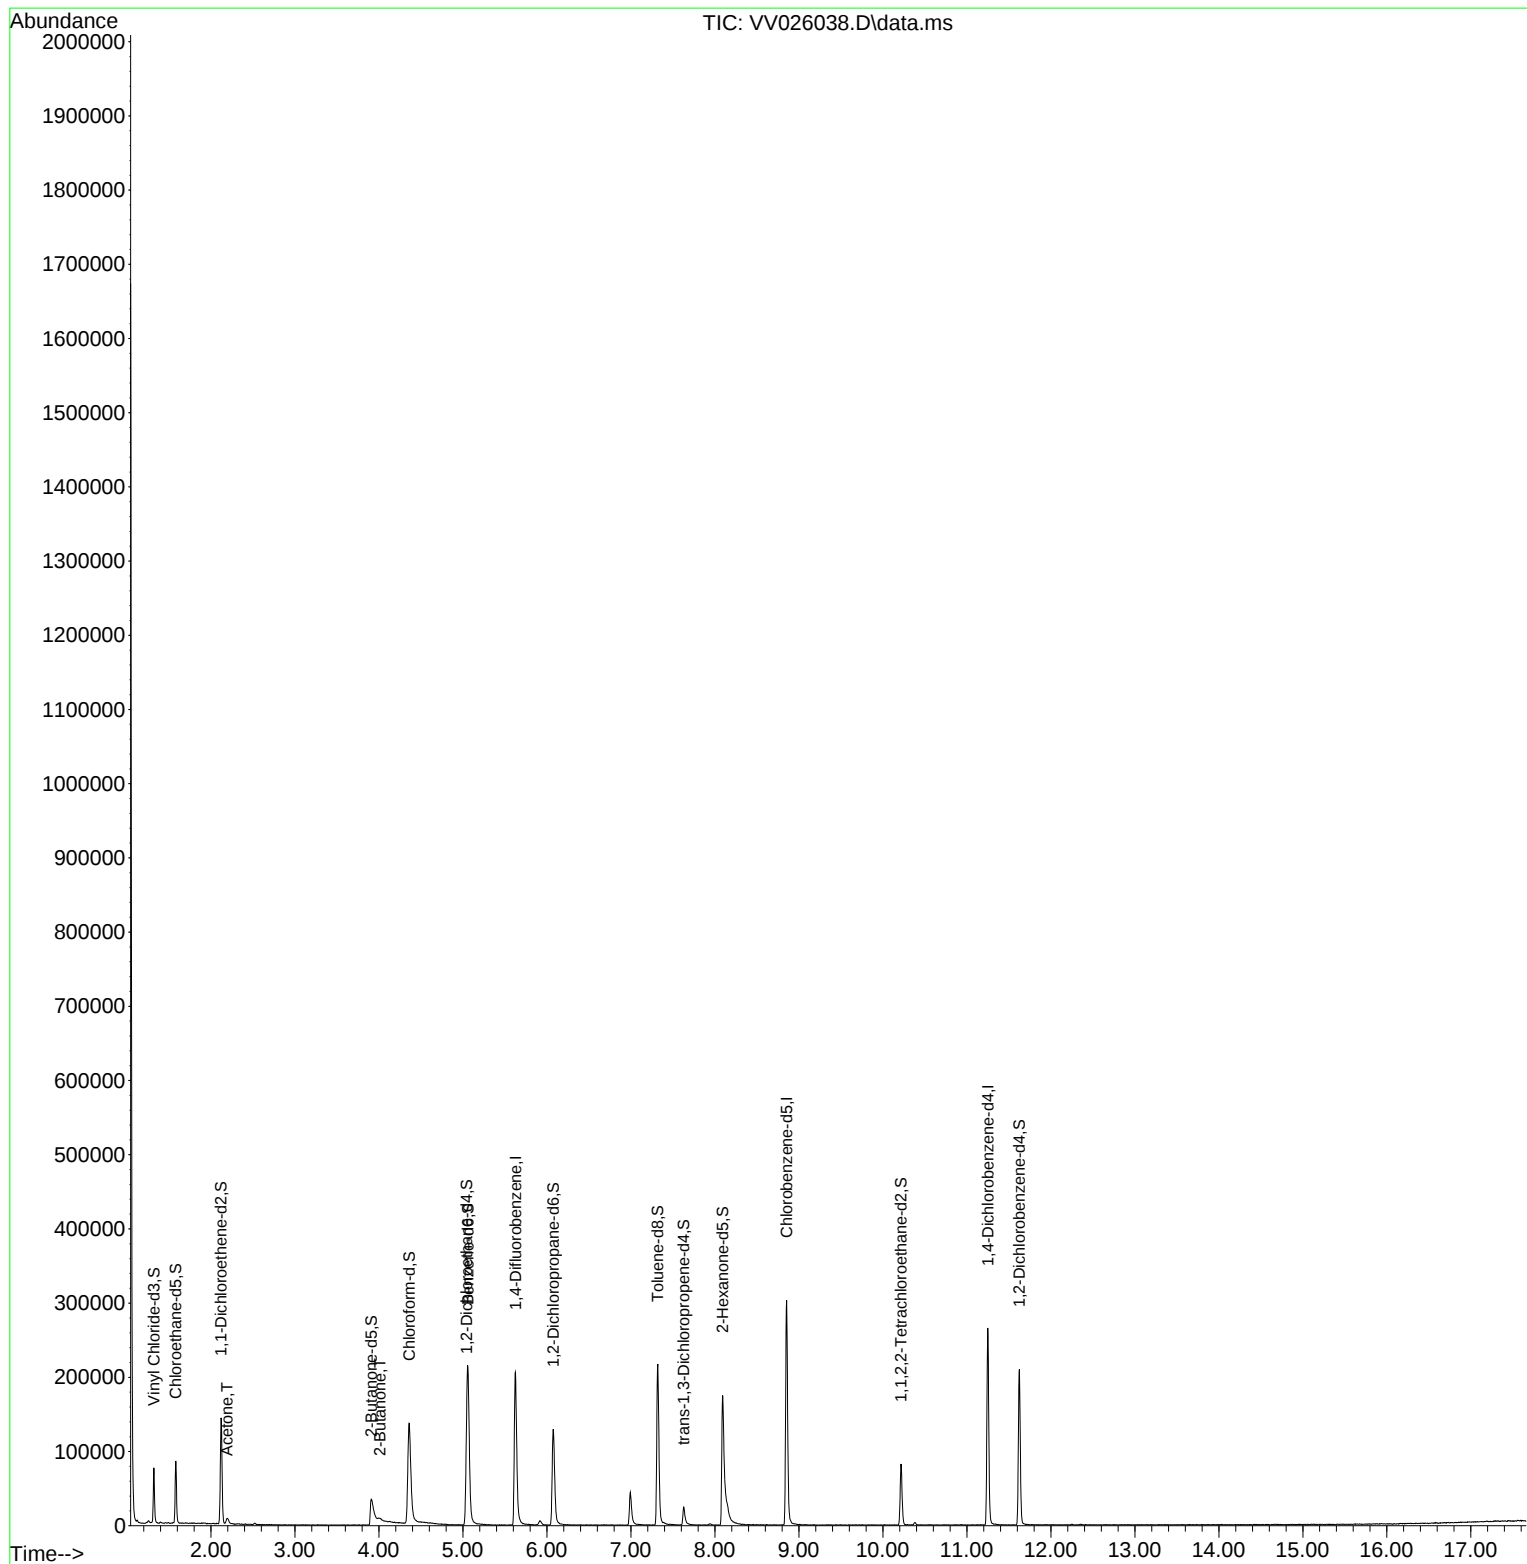


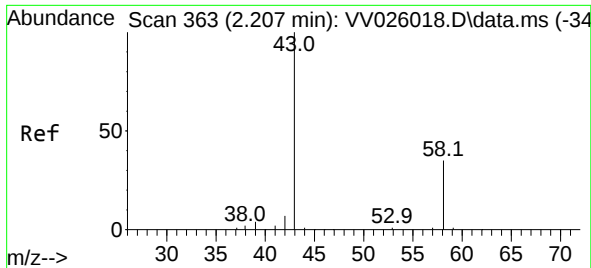

#13
Acetone
Concen: 10.416 ug/L
RT: 2.191 min Scan# 31
Delta R.T. -0.016 min
Lab File: VV026038.D
Acq: 08 Jun 2022 22:13

Instrument :
MSVOA_V
ClientSampleId :
C0DJ5

Tgt Ion: 43 Resp: 13152
Ion Ratio Lower Upper
43 100
58 32.1 0.0 47.6

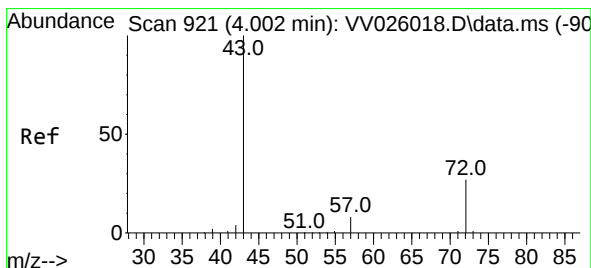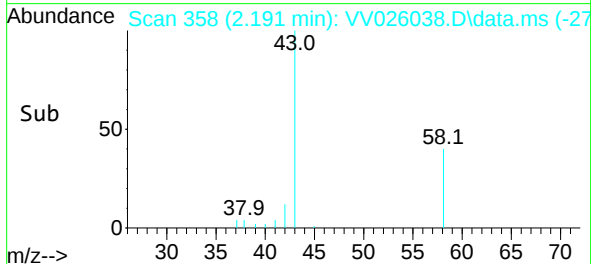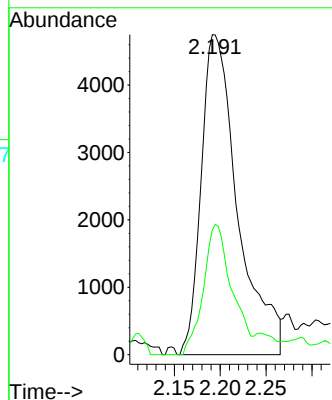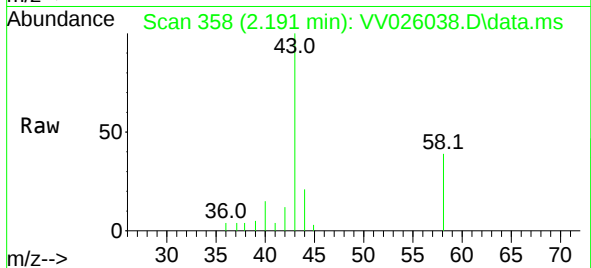

#21
2-Butanone
Concen: 8.331 ug/L
RT: 4.011 min Scan# 924
Delta R.T. 0.010 min
Lab File: VV026038.D
Acq: 08 Jun 2022 22:13

Tgt Ion: 43 Resp: 13702
Ion Ratio Lower Upper
43 100
72 18.4 11.9 35.7

