

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
 Data File : VV026020.D
 Acq On : 08 Jun 2022 15:01
 Operator : SY/MD
 Sample : N3256-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	76	86	97	rBV2	95258	129425	22.24%	2.521%
2	1.580	160	168	179	rVB	93850	105197	18.08%	2.049%
3	2.121	325	336	351	rVB	164008	238870	41.04%	4.652%
4	2.304	384	393	403	rBV	14692	22070	3.79%	0.430%
5	2.519	448	460	475	rVB3	15367	27667	4.75%	0.539%
6	3.056	615	627	637	rBV4	5023	9347	1.61%	0.182%
7	3.905	882	891	924	rBV2	31831	120970	20.79%	2.356%
8	4.358	1015	1032	1065	rVB5	128893	422001	72.51%	8.218%
9	5.053	1232	1248	1271	rBV2	230249	577276	99.19%	11.242%
10	5.619	1410	1424	1453	rBV	237920	489420	84.09%	9.531%
11	5.915	1506	1516	1525	rBV7	6599	13207	2.27%	0.257%
12	6.072	1552	1565	1585	rBV	137862	288010	49.49%	5.609%
13	6.989	1839	1850	1874	rBV	49652	98050	16.85%	1.910%
14	7.317	1941	1952	1970	rBV	256185	452398	77.73%	8.810%
15	7.397	1972	1977	1991	rVB3	6900	13435	2.31%	0.262%
16	7.625	2038	2048	2066	rBV	27919	54397	9.35%	1.059%
17	8.091	2183	2193	2238	rBV	186401	468856	80.56%	9.131%
18	8.850	2417	2429	2454	rBV	353925	581992	100.00%	11.334%
19	10.214	2842	2853	2868	rBV2	84904	136620	23.47%	2.661%
20	11.246	3164	3174	3192	rBV	313600	493726	84.83%	9.615%
21	11.622	3280	3291	3314	rBV	244961	391878	67.33%	7.632%




Sum of corrected areas: 5134812

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026020.D
Acq On : 08 Jun 2022 15:01
Operator : SY/MD
Sample : N3256-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

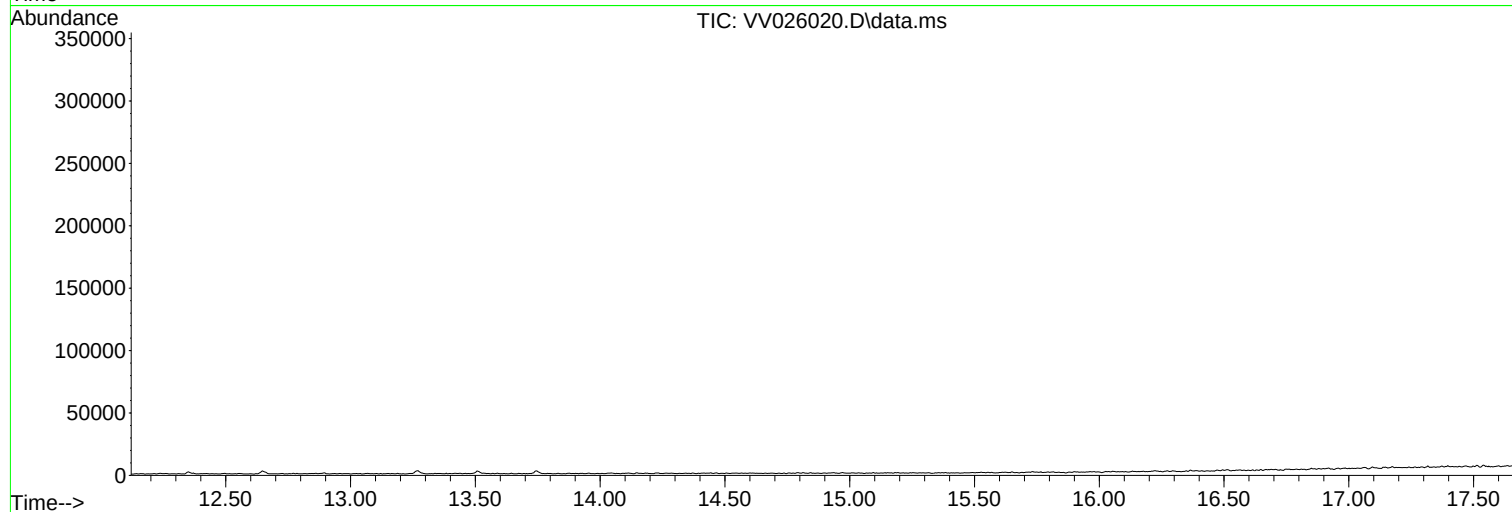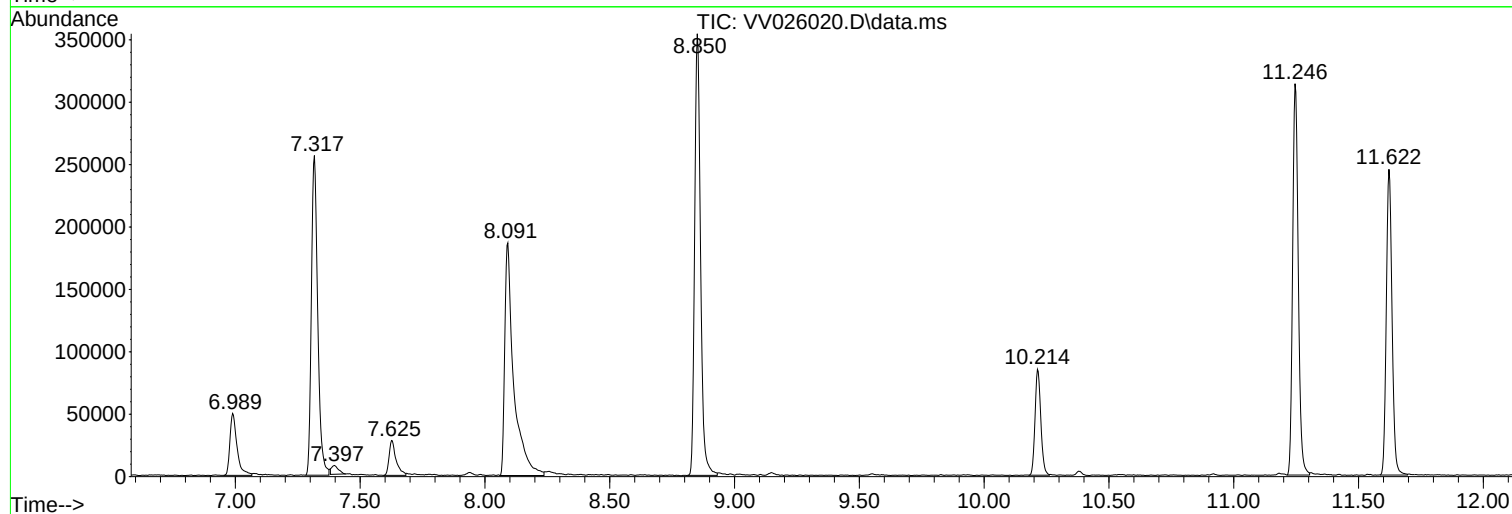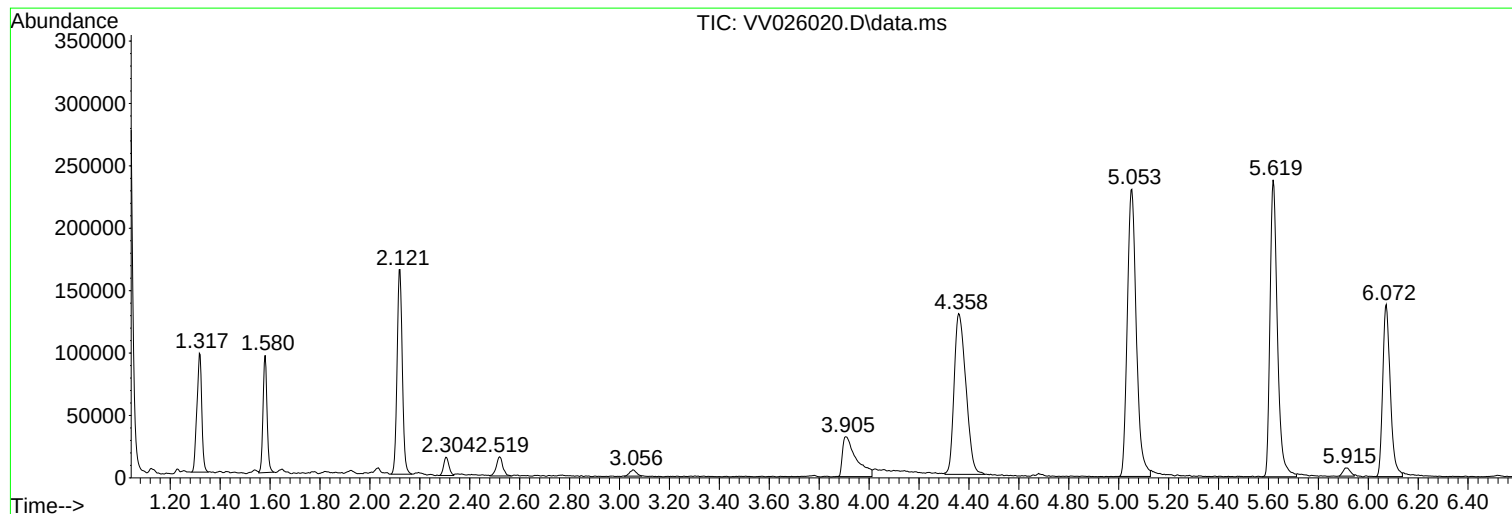

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026020.D
Acq On : 08 Jun 2022 15:01
Operator : SY/MD
Sample : N3256-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026020.D
Acq On : 08 Jun 2022 15:01
Operator : SY/MD
Sample : N3256-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc