

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
 Data File : VV026041.D
 Acq On : 08 Jun 2022 23:25
 Operator : SY/MD
 Sample : N3253-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	77	87	103	rVB	75183	89275	16.90%	1.991%
2	1.580	160	168	180	rVB	84467	94245	17.84%	2.102%
3	2.121	326	336	351	rVB	141237	204243	38.66%	4.556%
4	2.590	474	482	491	rBV3	3579	5600	1.06%	0.125%
5	2.966	589	599	616	rVB9	4696	10107	1.91%	0.225%
6	3.918	885	895	923	rBV2	27980	108363	20.51%	2.417%
7	4.362	1018	1033	1058	rVB2	102548	256064	48.47%	5.712%
8	5.056	1232	1249	1278	rBV2	206982	519696	98.37%	11.593%
9	5.625	1414	1426	1452	rBV	209226	430113	81.41%	9.595%
10	5.915	1506	1516	1535	rBV4	7403	16740	3.17%	0.373%
11	6.075	1553	1566	1591	rBV	129096	270673	51.23%	6.038%
12	6.307	1629	1638	1662	rBV5	6921	20948	3.97%	0.467%
13	6.992	1837	1851	1869	rBV	41775	82284	15.57%	1.836%
14	7.320	1943	1953	1969	rBV	216430	376691	71.30%	8.403%
15	7.397	1969	1977	1996	rVB	25794	48322	9.15%	1.078%
16	7.632	2040	2050	2071	rBV	23217	45128	8.54%	1.007%
17	8.095	2183	2194	2232	rBV2	172039	425128	80.47%	9.484%
18	8.249	2236	2242	2260	rVB9	7442	15877	3.01%	0.354%
19	8.853	2414	2430	2449	rBV	321622	528313	100.00%	11.785%
20	9.146	2510	2521	2535	rBV3	4855	8897	1.68%	0.198%
21	9.567	2642	2652	2664	rBV2	18851	32299	6.11%	0.721%
22	10.217	2843	2854	2870	rBV	77567	124870	23.64%	2.786%
23	10.381	2897	2905	2914	rBV4	3607	5798	1.10%	0.129%
24	11.249	3164	3175	3194	rBV	276021	428081	81.03%	9.549%
25	11.625	3280	3292	3310	rBV	202725	326353	61.77%	7.280%
26	12.349	3509	3517	3530	rVB6	5499	8703	1.65%	0.194%




Sum of corrected areas: 4482811

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026041.D
Acq On : 08 Jun 2022 23:25
Operator : SY/MD
Sample : N3253-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

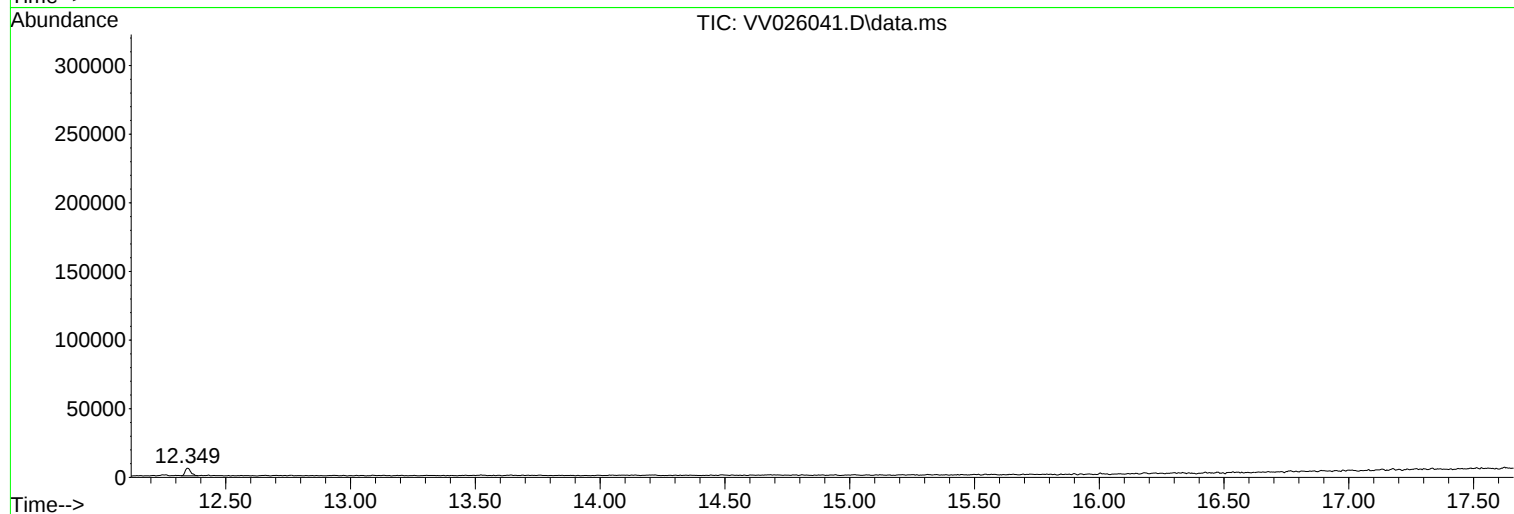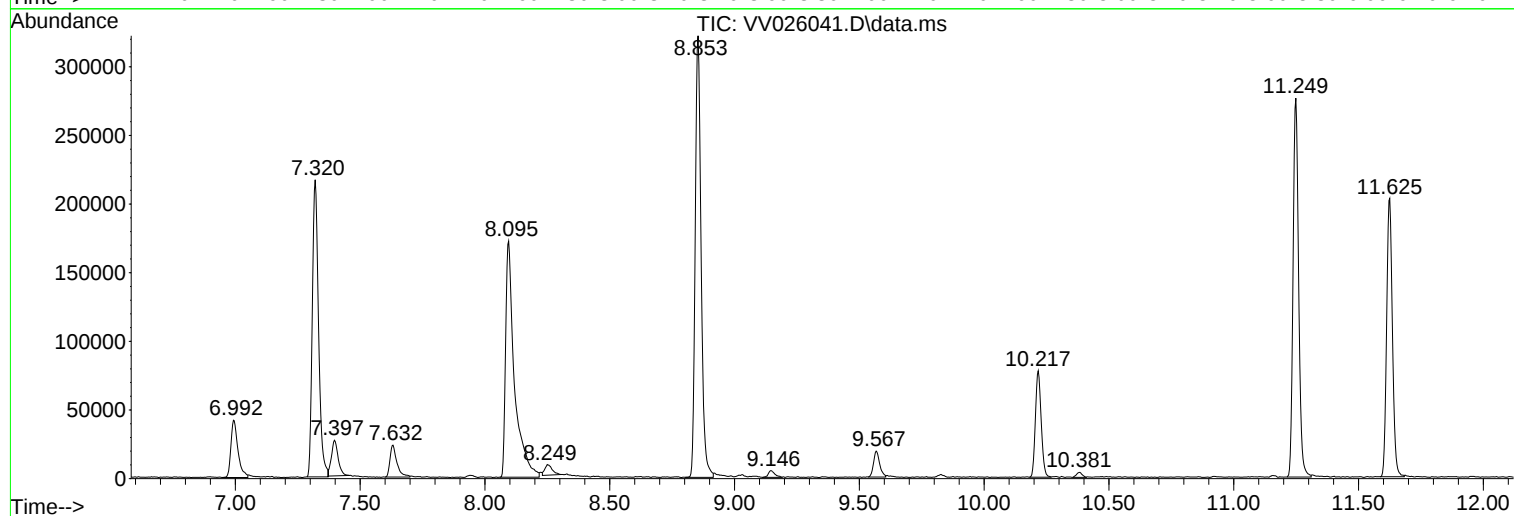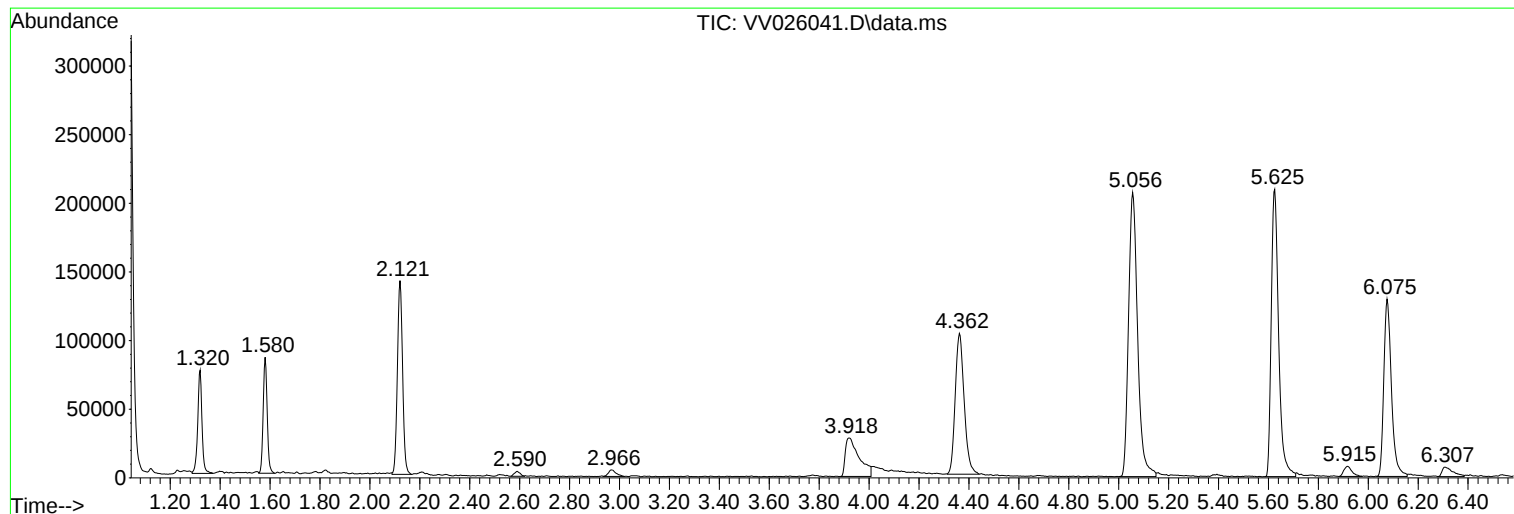

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026041.D
Acq On : 08 Jun 2022 23:25
Operator : SY/MD
Sample : N3253-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
Data File : VV026041.D
Acq On : 08 Jun 2022 23:25
Operator : SY/MD
Sample : N3253-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc