
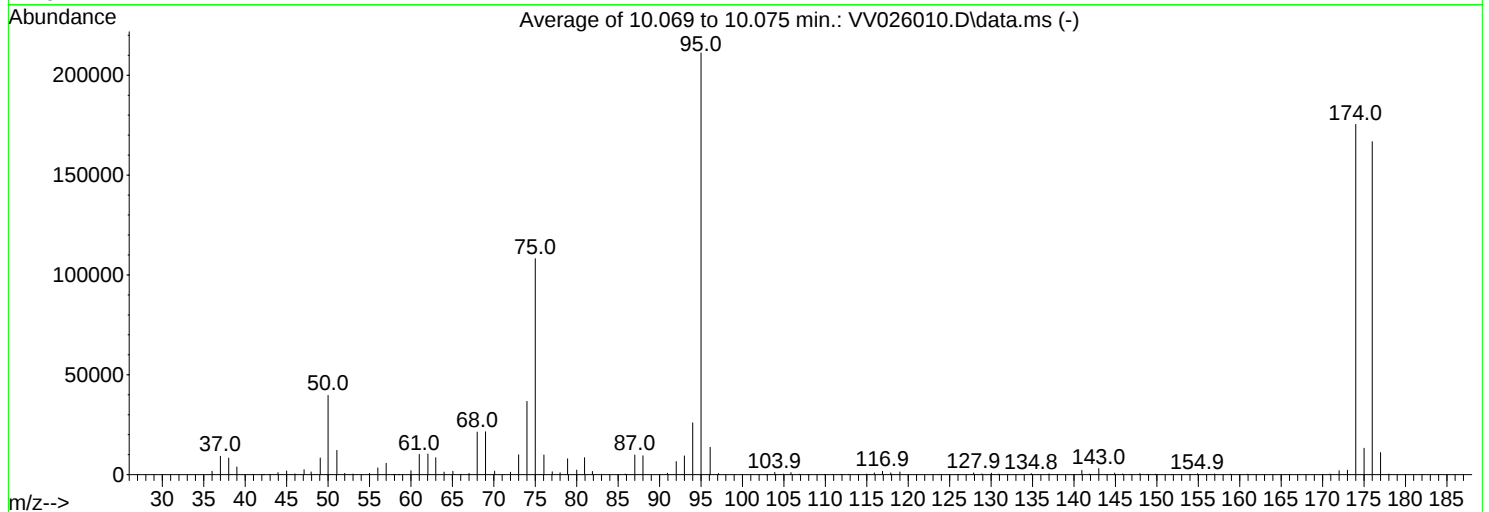


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060822\
 Data File : VV026010.D
 Acq On : 08 Jun 2022 08:50
 Operator : SY/MD
 Sample : BFB322
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB322

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jun 13 07:40:59 2022

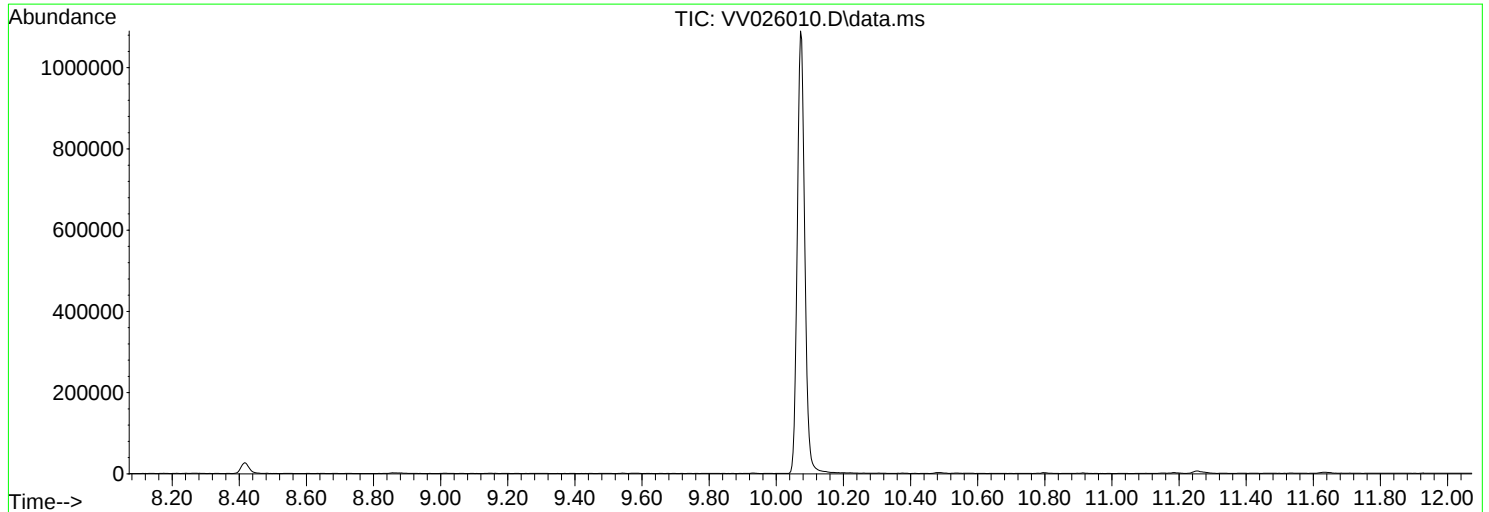

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	39677	PASS
75	95	30	80	51.2	108141	PASS
95	95	100	100	100.0	211221	PASS
96	95	5	9	6.5	13679	PASS
173	174	0.00	2	1.3	2286	PASS
174	95	50	120	83.0	175360	PASS
175	174	5	9	7.6	13242	PASS
176	174	95	105	95.1	166741	PASS
177	176	5	10	6.6	11067	PASS

m/z	Abundance
39.90	672.0
43.90	506.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322

m/z	Abundance
36.00	1558.0
37.00	8579.0
38.00	8178.0
39.00	3773.0
40.00	762.0
40.80	173.0
43.10	117.0
44.00	1533.0
45.00	1731.0
46.00	381.0
47.10	2339.0
48.00	1304.0
49.00	8332.0
50.00	38992.0
51.00	11882.0
52.00	571.0
53.00	268.0
55.00	613.0
56.00	3337.0
57.00	5318.0
57.90	217.0
58.50	107.0
60.00	2034.0
61.00	9719.0
62.00	10226.0
63.00	8212.0
64.00	1306.0
65.00	1662.0
66.00	269.0
67.00	597.0
68.00	20376.0
69.00	20624.0
70.10	1785.0
72.00	1222.0
73.00	9607.0
74.00	35008.0
75.00	103984.0
76.00	9501.0
77.00	1312.0
78.00	964.0
78.90	7662.0
80.00	2052.0
80.90	8288.0
81.90	1712.0
83.00	169.0
85.90	347.0
87.00	9590.0
88.00	9489.0
90.90	693.0
92.00	6312.0
93.00	8690.0
94.00	24424.0
95.00	199808.0
96.10	13618.0
97.10	485.0
103.90	1020.0
105.00	344.0
105.80	1014.0
106.90	246.0
110.00	116.0
111.00	159.0
111.90	171.0
112.80	171.0
115.00	272.0
115.90	933.0
116.90	1641.0
117.90	803.0
119.00	1267.0
123.70	155.0
127.90	843.0
128.90	358.0
130.10	647.0
131.00	254.0
134.80	481.0
137.00	400.0
140.10	144.0
141.00	2019.0
141.80	232.0
143.00	3039.0
143.90	198.0
144.90	960.0
145.90	400.0
146.80	116.0
148.00	478.0
148.80	172.0
149.80	255.0
151.80	122.0
153.90	170.0
154.90	441.0
156.90	436.0
158.80	162.0
160.90	233.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322

170.90	391.0
172.00	1940.0
173.00	2087.0
174.00	162624.0
175.00	12743.0
176.00	154176.0
177.00	10569.0
178.00	339.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322

m/z	Abundance
36.00	1783.0
37.00	9559.0
38.00	8664.0
39.00	4064.0
40.00	735.0
40.80	128.0
42.20	101.0
42.90	153.0
44.00	1595.0
45.00	1985.0
46.00	396.0
47.10	2575.0
47.90	1421.0
49.00	8566.0
50.00	41240.0
51.00	12559.0
52.00	672.0
53.00	308.0
54.10	122.0
55.00	699.0
56.00	3469.0
57.00	5993.0
57.90	195.0
60.00	2101.0
61.00	10475.0
62.00	10668.0
63.00	8698.0
64.00	1295.0
65.00	1713.0
66.10	276.0
67.00	658.0
68.00	22040.0
69.00	22352.0
70.10	1806.0
72.00	1238.0
73.00	10310.0
74.00	38064.0
75.00	112208.0
76.10	10255.0
77.10	1518.0
78.00	1020.0
78.90	8246.0
80.00	2467.0
81.00	8849.0
81.90	1673.0
83.00	211.0
85.90	372.0
87.00	10306.0
88.00	9814.0
90.90	788.0
92.00	6715.0
93.00	9710.0
94.00	26888.0
95.00	218624.0
96.10	14194.0
97.10	571.0
103.90	1183.0
105.00	340.0
105.90	1114.0
106.80	285.0
109.90	127.0
110.90	163.0
111.90	201.0
112.80	169.0
114.90	367.0
115.90	924.0
116.90	1716.0
117.90	934.0
119.00	1414.0
123.70	151.0
126.00	146.0
127.90	930.0
128.90	446.0
130.00	699.0
130.90	316.0
134.90	546.0
137.00	418.0
141.00	2225.0
141.90	361.0
143.00	3239.0
143.80	163.0
144.90	819.0
145.90	419.0
146.80	159.0
147.90	625.0
148.80	203.0
149.80	222.0
151.80	111.0
153.00	156.0
153.90	152.0
154.90	505.0
157.00	444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322

158.90	227.0
161.00	233.0
170.90	356.0
172.00	2048.0
173.00	2368.0
174.00	181568.0
175.00	13674.0
176.00	172608.0
177.00	11449.0
178.00	318.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322

m/z	Abundance
36.00	1733.0
37.00	9449.0
38.00	8279.0
39.00	3776.0
40.00	691.0
42.90	167.0
44.00	1507.0
45.00	1879.0
46.00	357.0
47.10	2443.0
47.90	1380.0
49.10	8080.0
50.00	38800.0
51.10	12047.0
52.00	612.0
53.00	294.0
54.10	133.0
55.00	648.0
56.00	3308.0
57.00	5819.0
58.10	219.0
60.00	1990.0
61.00	10256.0
62.10	10019.0
63.00	8487.0
64.00	1155.0
65.10	1600.0
66.10	242.0
67.00	625.0
68.00	21520.0
69.00	21576.0
70.10	1614.0
72.00	1137.0
73.00	9799.0
74.00	37040.0
75.00	108232.0
76.10	9829.0
77.10	1571.0
78.00	1010.0
78.90	8000.0
80.00	2543.0
81.00	8466.0
81.90	1547.0
83.00	245.0
85.80	331.0
87.00	9807.0
88.00	9205.0
91.00	807.0
92.00	6590.0
93.00	9799.0
94.00	26528.0
95.00	215232.0
96.10	13226.0
97.10	540.0
102.90	118.0
103.90	1142.0
104.90	305.0
105.90	1107.0
106.80	269.0
107.90	114.0
109.80	155.0
110.80	162.0
111.90	194.0
112.80	187.0
114.90	397.0
115.90	790.0
116.90	1622.0
117.90	979.0
119.00	1374.0
126.00	160.0
127.90	930.0
128.90	454.0
130.00	718.0
130.90	359.0
134.90	559.0
137.00	363.0
140.90	2240.0
141.90	432.0
143.00	2941.0
143.80	130.0
144.90	585.0
145.90	400.0
146.80	184.0
147.90	703.0
148.80	132.0
149.90	190.0
153.00	199.0
153.90	135.0
154.90	513.0
157.00	446.0
159.00	290.0
161.00	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322

170.90	335.0
172.00	2035.0
173.00	2402.0
174.00	181888.0
175.00	13310.0
176.00	173440.0
177.00	11182.0
178.00	291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB322