




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072724\
Data File : VV036731.D
Acq On : 26 Jul 2024 14:57
Operator : SY/MD
Sample : P3328-15
Misc : 7.32g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L8

Manual IntegrationsAPPROVED

Quant Time: Jul 27 04:17:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 04:14:21 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/10/2024
Supervised By :Semsettin Yesilyurt 08/10/2024

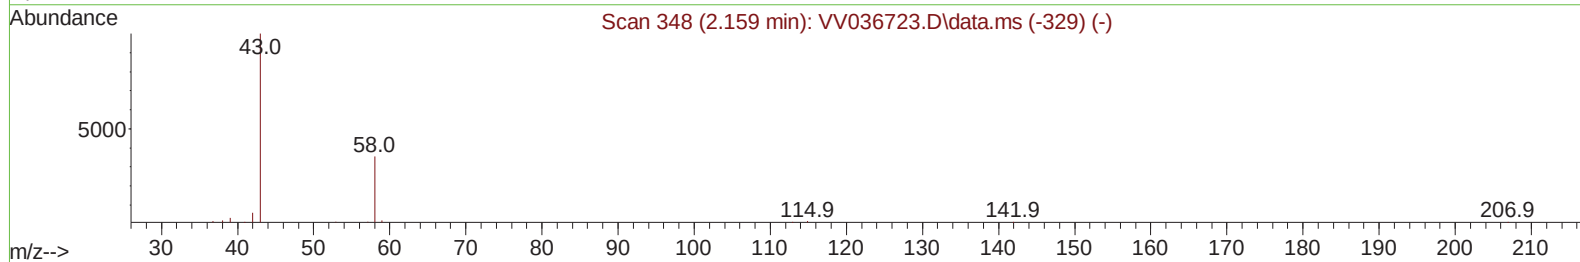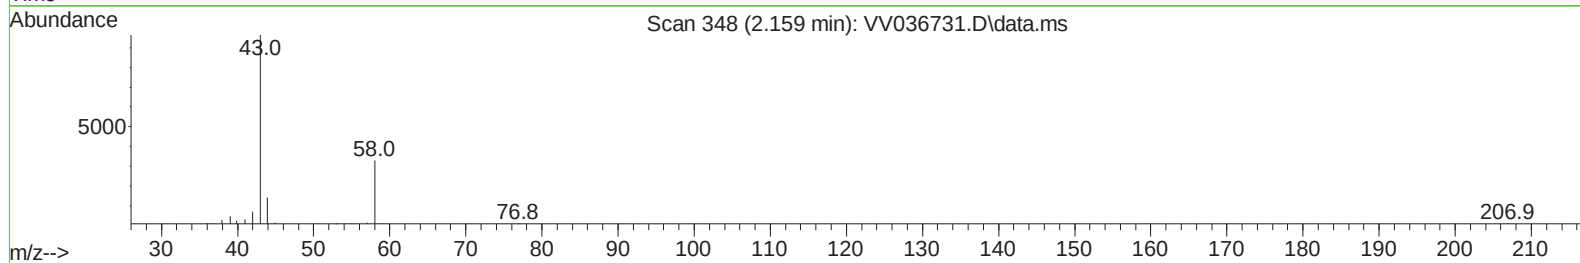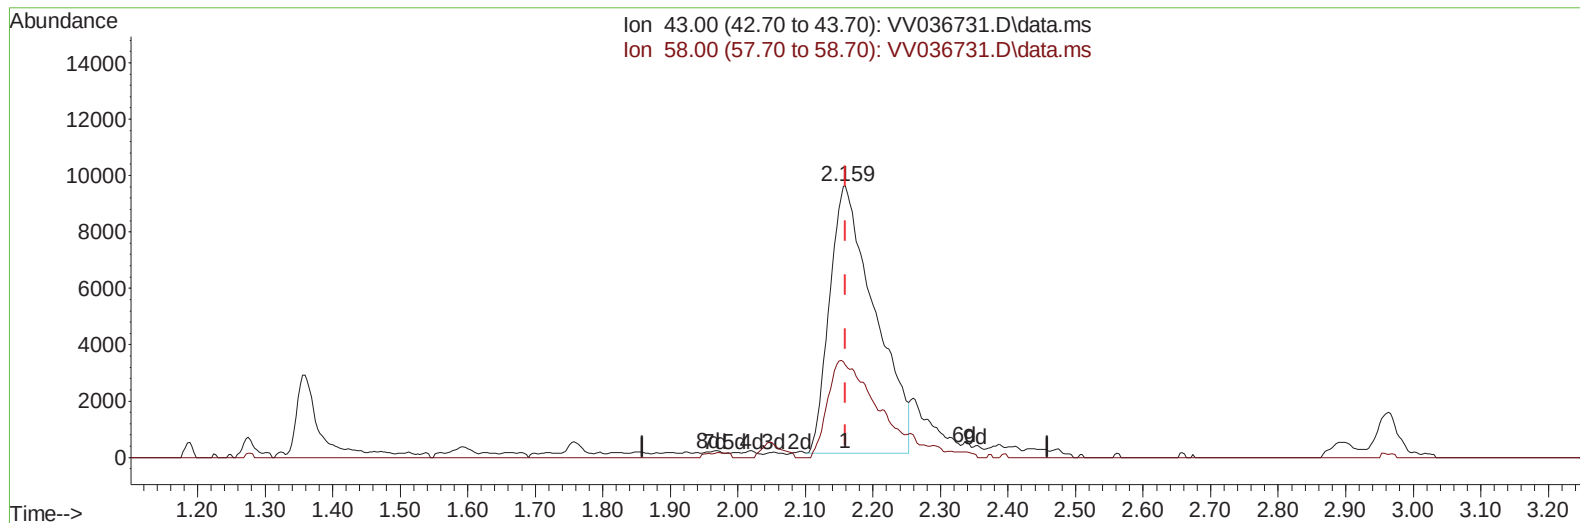

TIC: VV036731.D\data.ms

(13) Acetone (T)

2.159min (+ 0.000) 33.15 ug/L

response 43823

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.50	17.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072724\
Data File : VV036731.D
Acq On : 26 Jul 2024 14:57
Operator : SY/MD
Sample : P3328-15
Misc : 7.32g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L8

Manual IntegrationsAPPROVED

Quant Time: Jul 27 04:17:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 04:14:21 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/10/2024
Supervised By :Semsettin Yesilyurt 08/10/2024

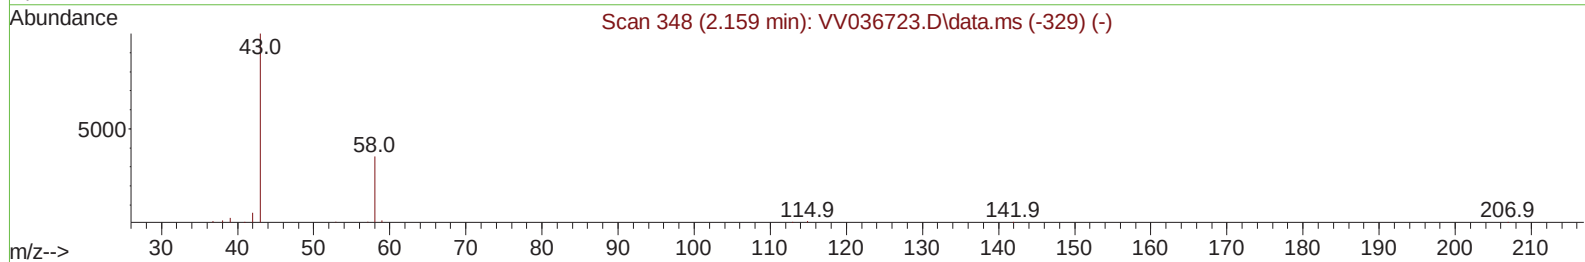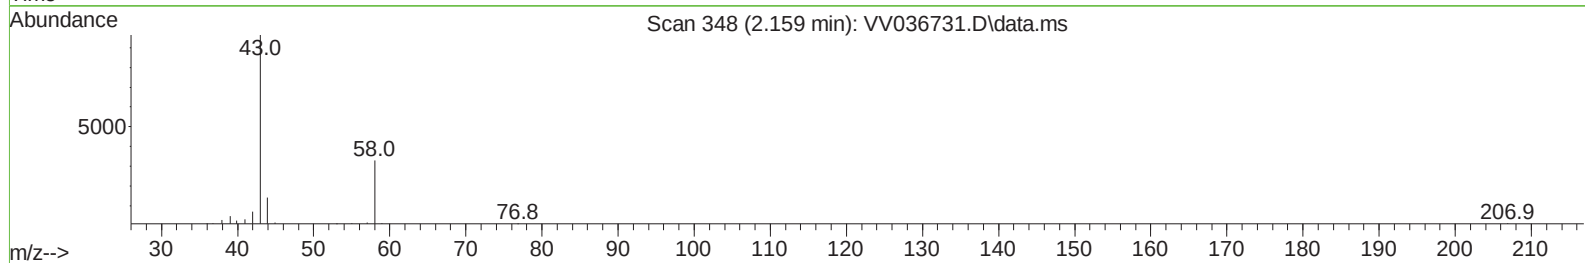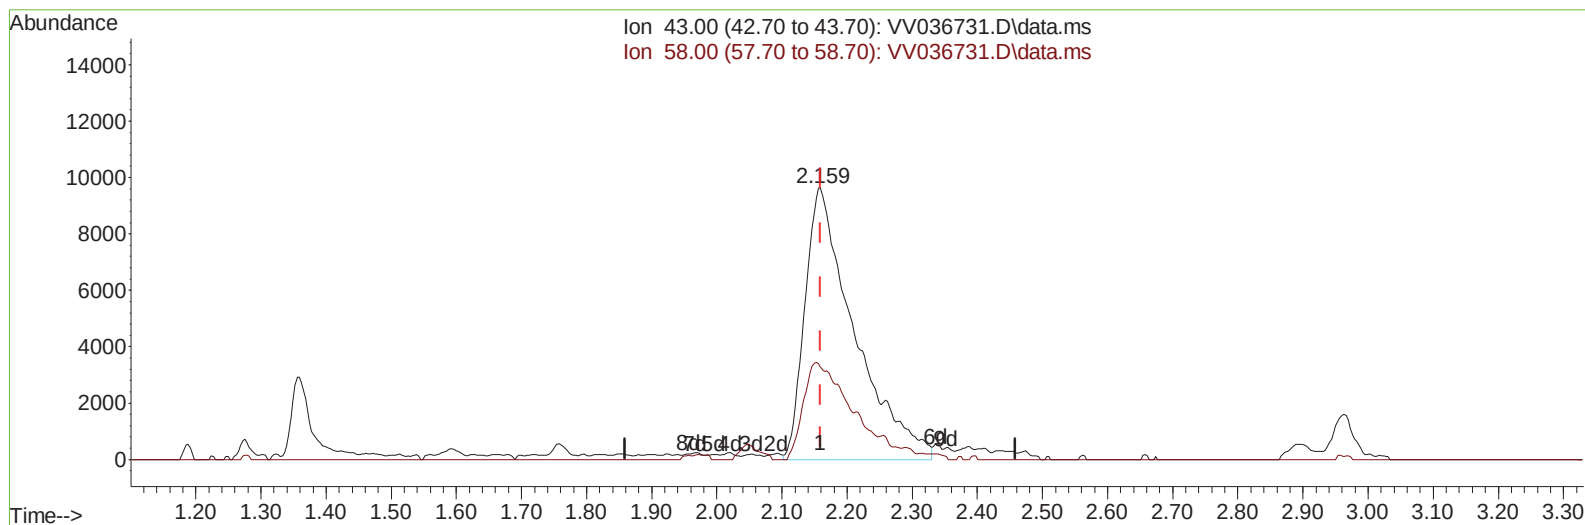

TIC: VV036731.D\data.ms

(13) Acetone (T)

2.159min (+ 0.000) 38.18 ug/L m

response 50474

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.50	15.04
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072724\
 Data File : VV036731.D
 Acq On : 26 Jul 2024 14:57
 Operator : SY/MD
 Sample : P3328-15
 Misc : 7.32g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L8

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/10/2024
 Supervised By :Semsettin Yesilyurt 08/10/2024

Quant Time: Jul 27 04:17:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 04:14:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	318357	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	323691	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	147508	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	40267	11.548	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	46.200%	
7) Chloroethane-d5	1.526	69	42993	13.652	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.600%	
11) 1,1-Dichloroethene-d2	2.050	65	18581	10.078	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	40.320%#	
21) 2-Butanone-d5	3.841	46	54230	66.643	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	133.280%	
24) Chloroform-d	4.246	84	141870	16.850	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	67.400%	
26) 1,2-Dichloroethane-d4	4.941	65	78624	18.928	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.720%	
32) Benzene-d6	4.957	84	195143	12.720	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	50.880%	
36) 1,2-Dichloropropane-d6	5.989	67	74363	17.012	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	68.040%#	
41) Toluene-d8	7.243	98	151100	10.321	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	41.280%	
43) trans-1,3-Dichloroprop...	7.558	79	28133	14.478	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	57.920%	
47) 2-Hexanone-d5	8.034	63	36774	63.215	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	126.420%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	117817	30.924	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	123.680%#	
66) 1,2-Dichlorobenzene-d4	11.558	152	107419	20.861	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	83.440%	
Target Compounds						
13) Acetone	2.159	43	50474m	38.184	ug/L	
16) Methylene chloride	2.442	84	47564	8.030	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072724\
Data File : VV036731.D
Acq On : 26 Jul 2024 14:57
Operator : SY/MD
Sample : P3328-15
Misc : 7.32g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L8

Manual IntegrationsAPPROVED

Quant Time: Jul 27 04:17:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 04:14:21 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/10/2024
Supervised By :Semsettin Yesilyurt 08/10/2024

