
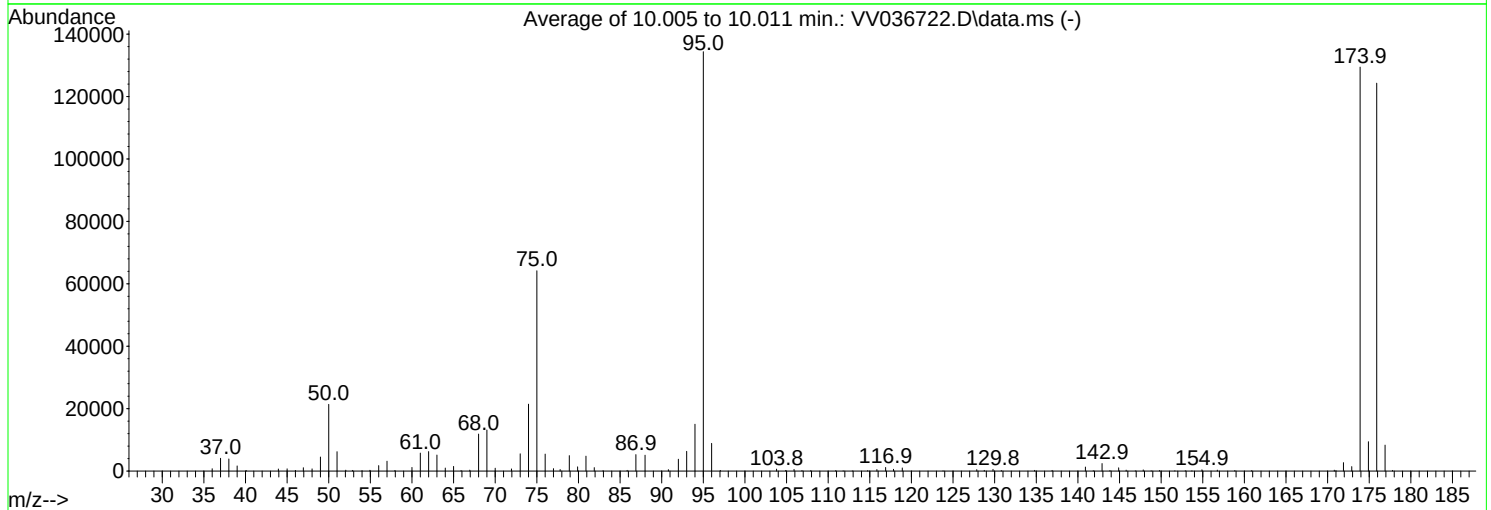


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072724\
Data File : VV036722.D
Acq On : 26 Jul 2024 10:11
Operator : SY/MD
Sample : BFB351
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB351

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Title : VOC Analysis
Last Update : Sat Jul 27 04:14:21 2024

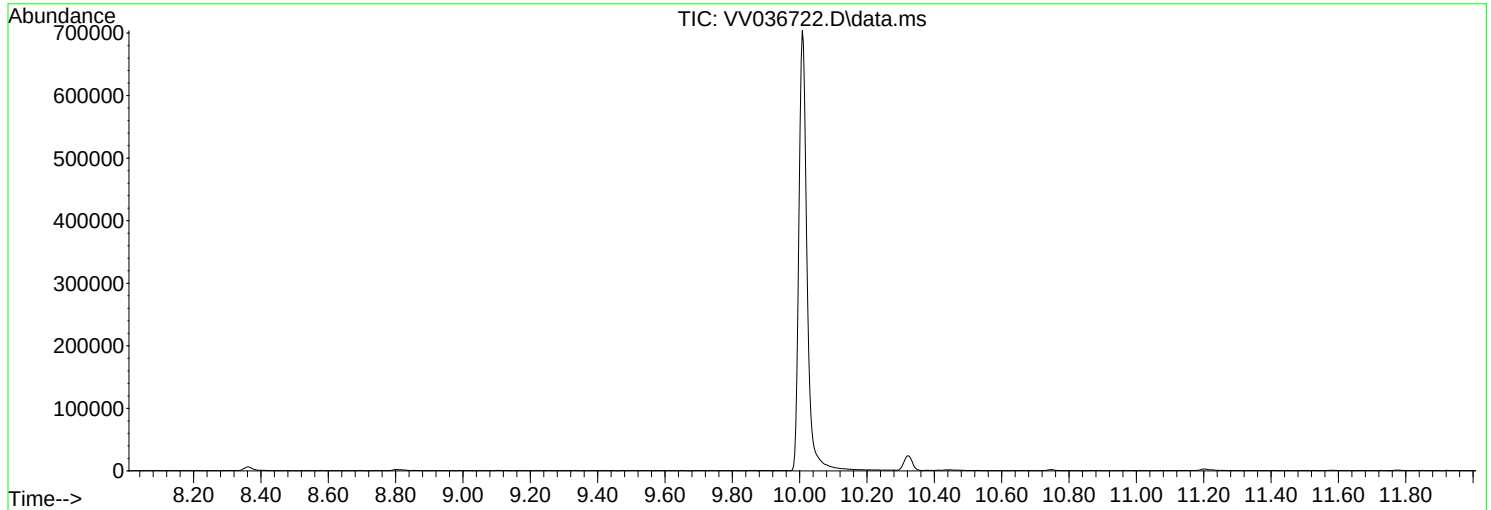

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	21381	PASS
75	95	30	80	47.8	64176	PASS
95	95	100	100	100.0	134368	PASS
96	95	5	9	6.6	8880	PASS
173	174	0.00	2	1.1	1424	PASS
174	95	50	120	96.3	129440	PASS
175	174	5	9	7.3	9415	PASS
176	174	95	101	96.0	124285	PASS
177	176	5	9	6.7	8329	PASS

m/z	Abundance
39.90	102.0
44.00	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	770.0
37.00	4063.0
38.00	3926.0
39.00	1639.0
39.90	190.0
43.90	956.0
45.00	731.0
46.00	264.0
47.00	1028.0
48.00	674.0
49.00	4504.0
50.00	20904.0
51.00	6269.0
52.00	290.0
52.80	237.0
54.00	118.0
55.00	272.0
56.00	1608.0
57.00	3156.0
57.90	183.0
60.00	1132.0
61.00	5396.0
62.00	5986.0
63.00	5185.0
64.00	947.0
65.00	1598.0
65.90	129.0
67.00	299.0
68.00	11554.0
69.00	13074.0
70.00	853.0
71.90	644.0
73.00	5417.0
74.00	20552.0
75.00	63096.0
76.00	5371.0
77.00	790.0
77.80	503.0
78.90	4919.0
79.90	1340.0
80.90	4635.0
81.90	1119.0
83.00	113.0
85.80	239.0
86.90	5141.0
88.00	4927.0
90.80	482.0
92.00	3781.0
93.00	6233.0
94.00	14448.0
95.00	130144.0
96.00	8879.0
97.10	202.0
103.80	603.0
104.90	210.0
105.90	515.0
106.80	160.0
107.90	117.0
110.90	106.0
114.70	149.0
115.90	518.0
116.90	1026.0
117.90	583.0
118.90	951.0
123.80	125.0
127.90	378.0
128.80	206.0
129.80	539.0
130.80	198.0
134.70	235.0
136.90	219.0
140.90	1308.0
141.90	151.0
142.90	2431.0
143.80	161.0
144.90	1072.0
145.80	270.0
147.90	351.0
148.80	150.0
149.80	217.0
151.60	112.0
152.90	116.0
154.90	411.0
156.70	290.0
158.90	168.0
160.80	147.0
170.80	449.0
171.90	2639.0
172.90	1327.0
173.90	122784.0
174.90	9157.0
175.90	116128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

176.90	8108.0
177.80	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	780.0
37.00	4243.0
38.00	3985.0
39.00	1676.0
40.10	223.0
44.00	983.0
45.00	740.0
46.00	231.0
46.90	1151.0
48.00	737.0
49.00	4649.0
50.00	22184.0
51.00	6365.0
52.10	299.0
52.90	224.0
54.00	113.0
55.00	269.0
56.00	1855.0
57.00	3260.0
57.90	221.0
60.00	1212.0
61.00	5986.0
62.00	6497.0
63.00	5328.0
64.00	991.0
65.00	1558.0
65.90	164.0
67.00	321.0
68.00	12204.0
69.00	13696.0
70.00	951.0
71.90	739.0
73.00	5692.0
74.00	22264.0
75.00	66016.0
76.00	5663.0
77.00	822.0
77.80	524.0
78.90	5132.0
79.90	1414.0
80.90	4934.0
81.90	1154.0
82.90	123.0
85.80	248.0
86.90	5467.0
88.00	5321.0
90.80	477.0
92.00	3952.0
93.00	6493.0
94.00	15421.0
95.00	138560.0
96.00	9171.0
97.10	224.0
103.80	661.0
104.90	223.0
105.90	543.0
106.90	193.0
107.90	145.0
110.90	142.0
111.80	103.0
114.70	170.0
115.90	520.0
116.90	1211.0
117.90	578.0
118.90	1040.0
123.80	103.0
127.80	476.0
128.70	227.0
129.80	591.0
130.80	193.0
134.80	217.0
136.90	236.0
140.90	1350.0
141.80	129.0
142.90	2509.0
143.90	199.0
144.90	1080.0
145.80	329.0
146.90	125.0
147.80	393.0
148.80	134.0
149.80	202.0
151.60	125.0
152.90	119.0
153.70	105.0
154.90	439.0
156.80	333.0
158.90	214.0
160.80	132.0
170.80	445.0
171.90	2804.0
172.90	1462.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

173.90	133568.0
174.90	9747.0
175.90	128592.0
176.90	8631.0
177.80	227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	732.0
37.00	3999.0
38.00	3737.0
39.00	1613.0
40.10	241.0
44.00	937.0
45.00	705.0
45.90	138.0
46.90	1053.0
48.00	717.0
49.00	4386.0
50.00	21056.0
51.00	5992.0
52.00	298.0
52.90	195.0
54.00	109.0
54.90	240.0
56.00	1837.0
57.00	3133.0
58.00	227.0
60.00	1171.0
61.00	5935.0
62.00	6278.0
63.00	4905.0
64.00	995.0
65.00	1352.0
65.90	189.0
66.90	310.0
68.00	11816.0
69.00	12727.0
70.00	975.0
72.00	708.0
73.00	5511.0
74.00	21504.0
75.00	63416.0
76.00	5312.0
77.00	778.0
77.80	437.0
78.90	4813.0
79.90	1344.0
80.90	4796.0
81.90	1068.0
82.90	116.0
85.90	218.0
86.90	5247.0
88.00	5049.0
90.80	453.0
92.00	3672.0
93.00	6242.0
94.00	15160.0
95.00	134400.0
96.00	8589.0
97.00	214.0
103.80	630.0
104.90	223.0
105.90	564.0
106.90	188.0
107.90	140.0
110.90	144.0
111.80	120.0
112.90	131.0
114.80	164.0
115.80	428.0
116.90	1228.0
117.80	553.0
118.90	1025.0
127.80	553.0
128.70	240.0
129.80	526.0
130.80	179.0
134.90	228.0
136.90	212.0
140.90	1250.0
141.80	126.0
142.90	2287.0
143.90	186.0
144.90	979.0
145.80	319.0
146.90	118.0
147.80	413.0
149.80	149.0
151.70	115.0
152.90	114.0
153.70	111.0
154.90	413.0
156.80	330.0
158.80	211.0
160.90	118.0
171.00	391.0
171.90	2694.0
172.90	1484.0
173.90	131968.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

174.90	9341.0
175.90	128136.0
176.90	8249.0
177.80	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351