

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027189.D
 Acq On : 03 Aug 2022 13:50
 Operator : SY/MD
 Sample : VV0803WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Quant Time: Aug 04 03:03:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 04 02:57:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	651406	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	638521	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	274108	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	248718	58.914	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	117.820%	
7) Chloroethane-d5	1.561	69	180871	57.253	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	114.500%	
11) 1,1-Dichloroethene-d2	2.101	63	305045	37.945	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.900%	
21) 2-Butanone-d5	3.873	46	243643	87.658	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	87.660%	
24) Chloroform-d	4.339	84	391563	45.886	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.780%	
26) 1,2-Dichloroethane-d4	5.024	65	236247	48.795	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.600%	
32) Benzene-d6	5.043	84	835359	49.441	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.880%	
36) 1,2-Dichloropropane-d6	6.063	67	258389	49.436	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.880%	
41) Toluene-d8	7.310	98	694055	45.565	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.120%	
43) trans-1,3-Dichloroprop...	7.616	79	104966	45.758	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.520%	
47) 2-Hexanone-d5	8.085	63	189799	94.059	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	94.060%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	352246	45.084	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.160%	
66) 1,2-Dichlorobenzene-d4	11.622	152	255031	52.940	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	105.880%	
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.246	75	30680	5.391	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027189.D
Acq On : 03 Aug 2022 13:50
Operator : SY/MD
Sample : VV0803WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Time: Aug 04 03:03:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 04 02:57:16 2022
Response via : Initial Calibration

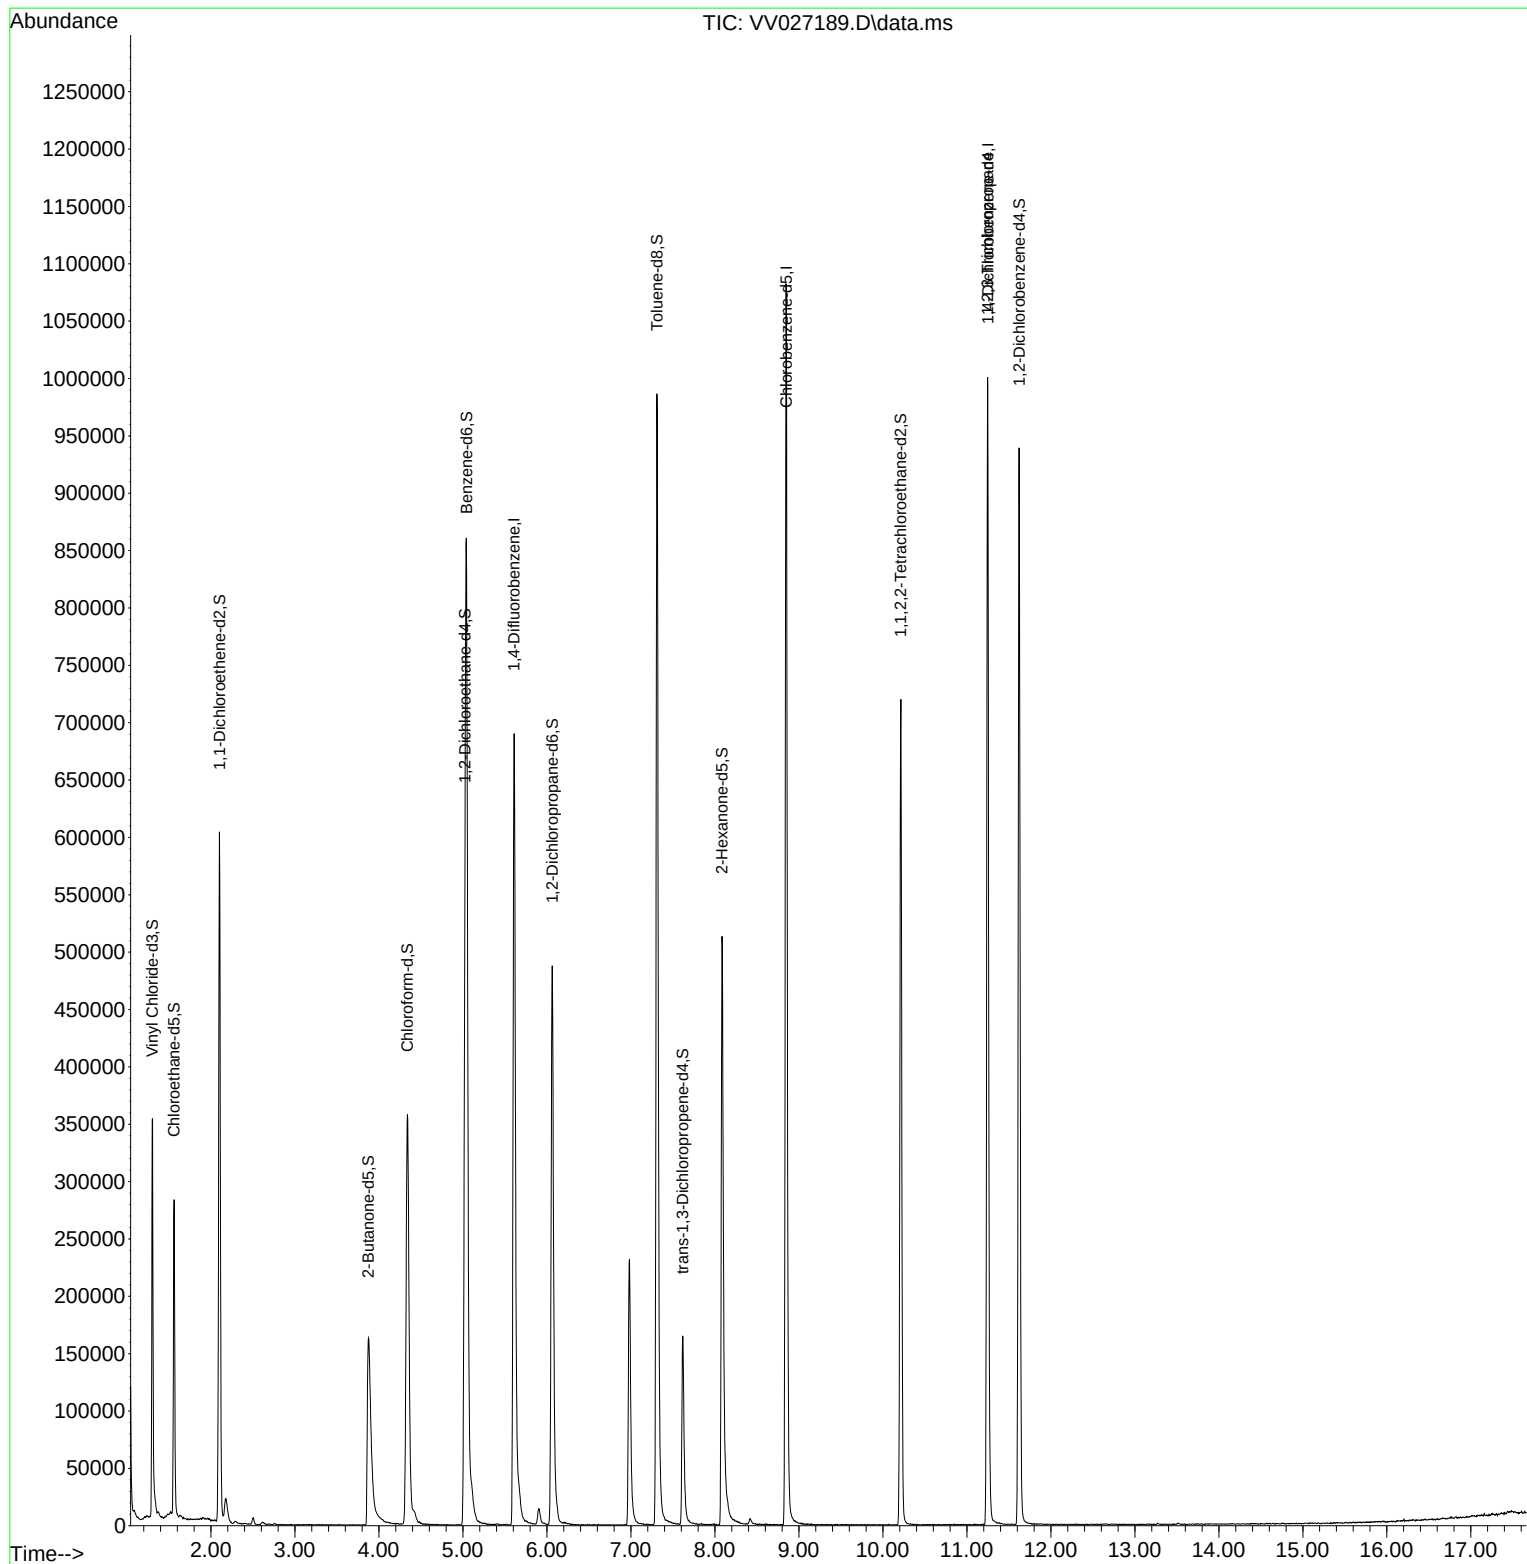

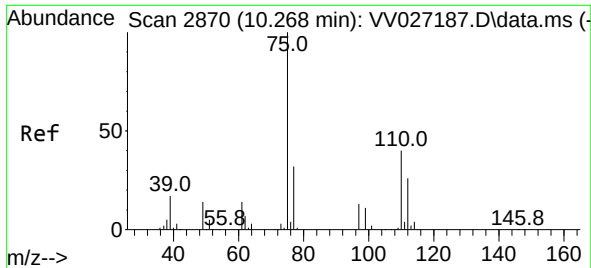

#61
 1,2,3-Trichloropropane
 Concen: 5.391 ug/L
 RT: 11.246 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV027189.D
 Acq: 03 Aug 2022 13:50

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Tgt Ion: 75	Resp:	30680
Ion Ratio	Lower	Upper
75	100	
77	31.2	25.8 38.8
110	2.7	32.8 49.2#

