




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027191.D
 Acq On : 03 Aug 2022 14:59
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Manual IntegrationsAPPROVED

Quant Time: Aug 04 03:03:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 04 02:57:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/04/2022
 Supervised By :Mahesh Dadoda 08/05/2022

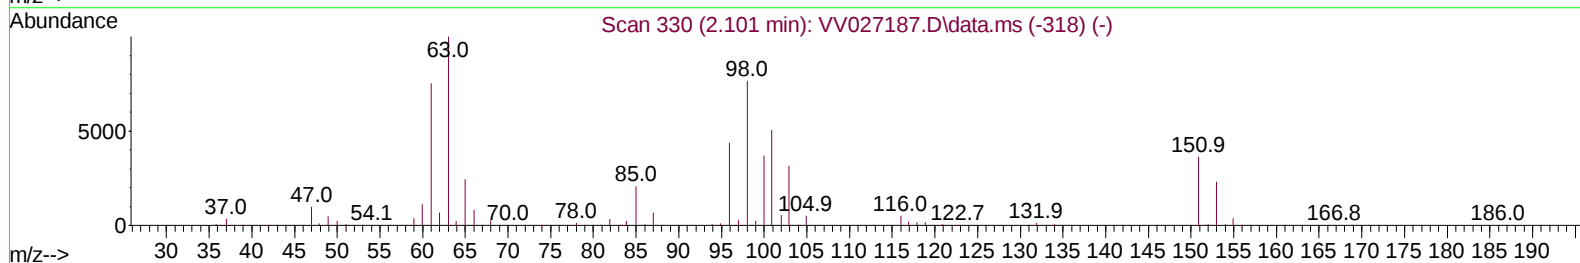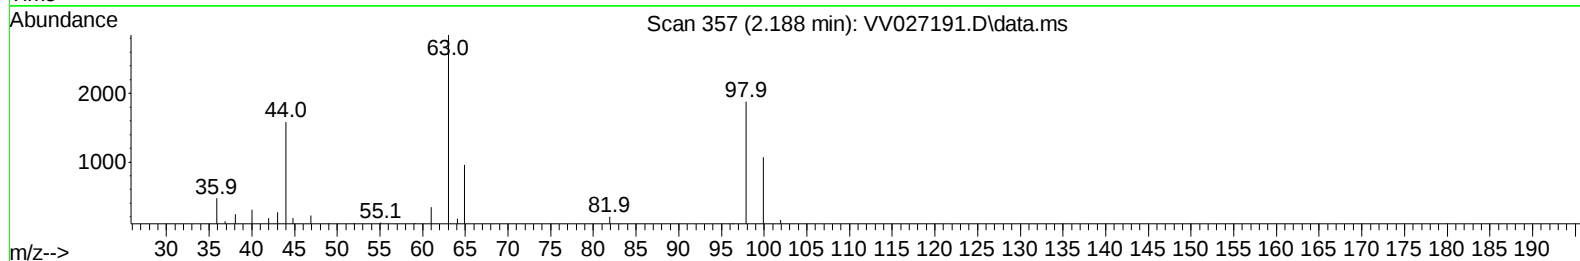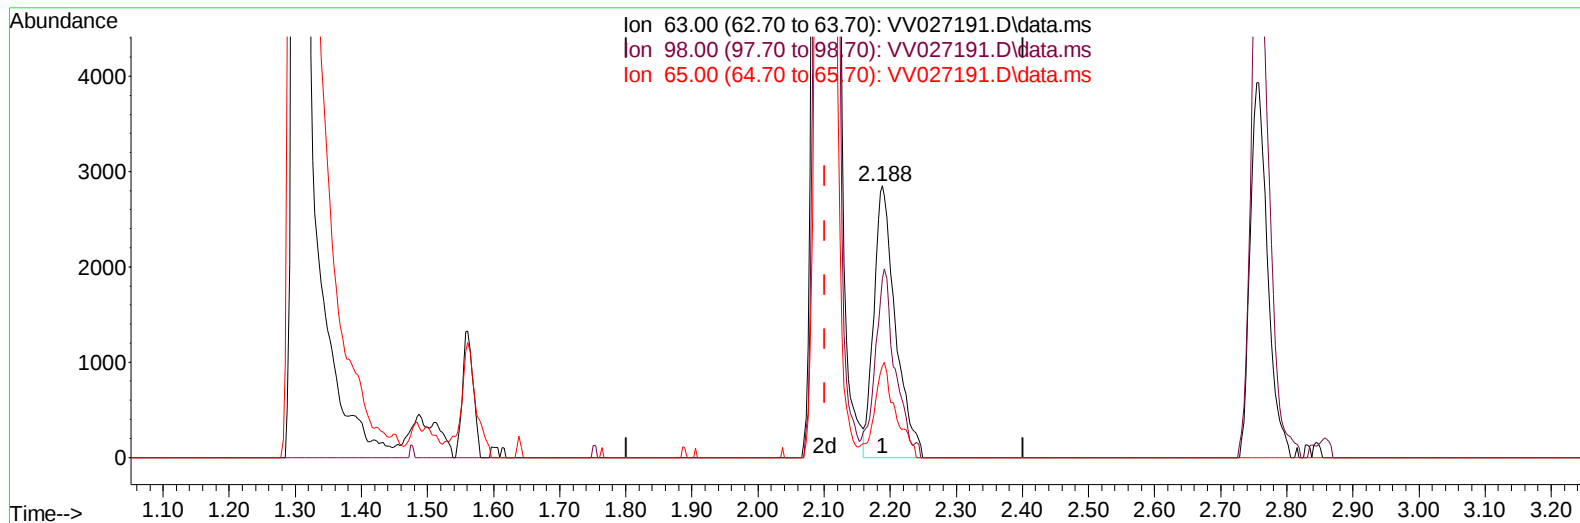

TIC: VV027191.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.188min (+ 0.087) 1.52 ug/L

response 6455

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	79.90	63.73
65.00	23.50	21.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027191.D
 Acq On : 03 Aug 2022 14:59
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Manual IntegrationsAPPROVED

Quant Time: Aug 04 03:03:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 04 02:57:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/04/2022
 Supervised By :Mahesh Dadoda 08/05/2022

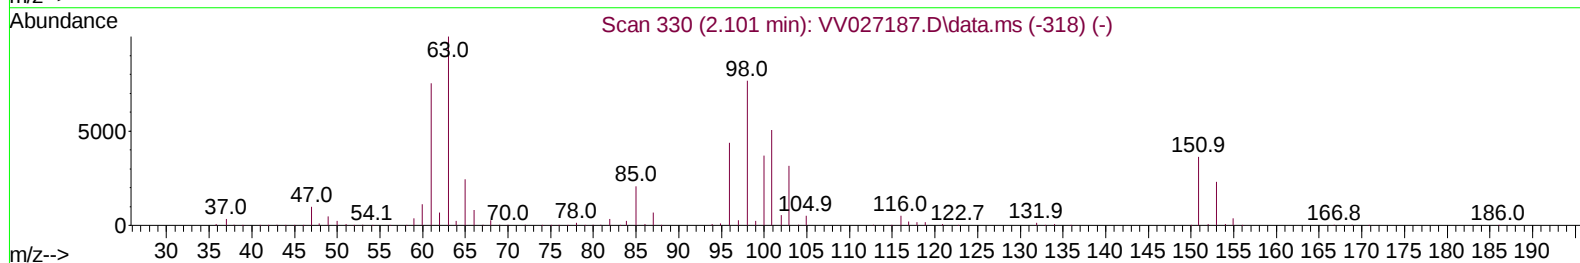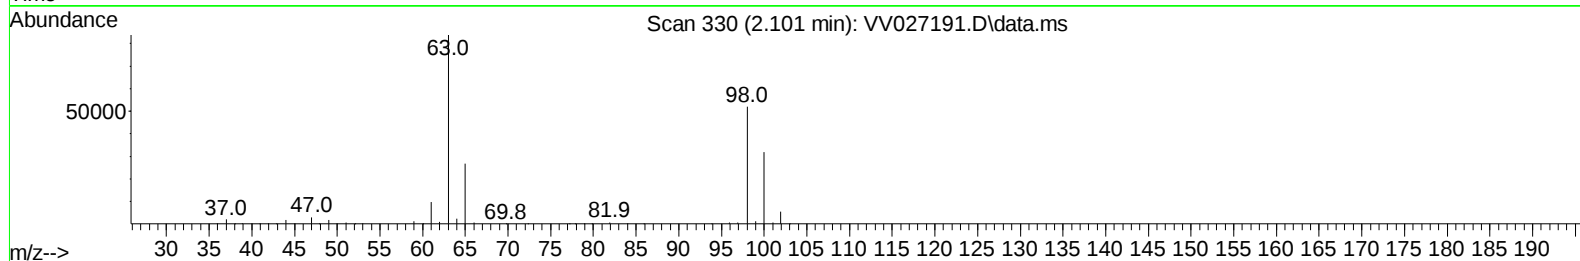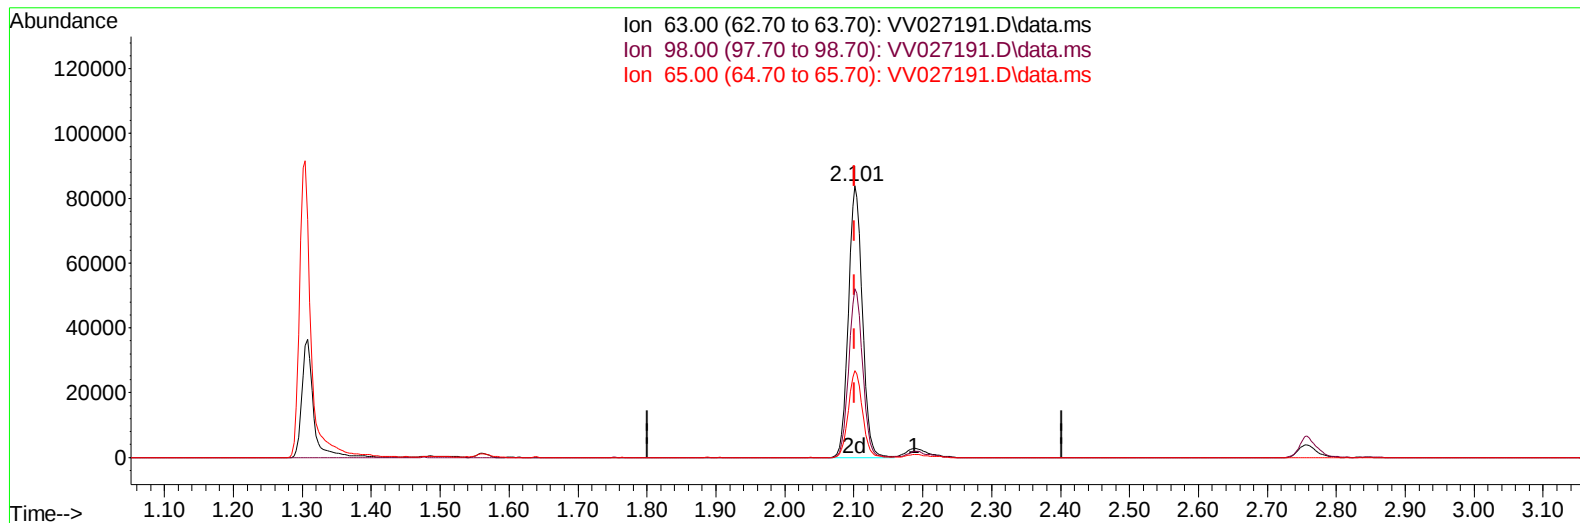

TIC: VV027191.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (+ 0.000) 27.95 ug/L m

response 118333

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	79.90	3.48#
65.00	23.50	1.17#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027191.D
 Acq On : 03 Aug 2022 14:59
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Manual IntegrationsAPPROVED

Quant Time: Aug 04 03:03:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 04 02:57:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/04/2022
 Supervised By :Mahesh Dadoda 08/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	343055	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	339030	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	135943	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	106414	47.863	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	95.720%	
7) Chloroethane-d5	1.561	69	91483	54.987	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	109.980%	
11) 1,1-Dichloroethene-d2	2.101	63	118333m	27.951	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	55.900%#	
21) 2-Butanone-d5	3.876	46	233680	159.643	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	159.640%#	
24) Chloroform-d	4.343	84	256046	56.974	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	113.940%	
26) 1,2-Dichloroethane-d4	5.027	65	156923	61.544	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	123.080%	
32) Benzene-d6	5.047	84	413056	46.042	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.080%	
36) 1,2-Dichloropropane-d6	6.066	67	158536	57.126	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	114.260%	
41) Toluene-d8	7.313	98	273700	33.841	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	67.680%#	
43) trans-1,3-Dichloroprop...	7.619	79	63741	52.333	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	104.660%	
47) 2-Hexanone-d5	8.088	63	157699	147.189	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	147.190%#	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	293719	70.803	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	141.600%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	159414	66.724	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	133.440%#	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.307	62	779147	240.475	ug/L	99
17) trans-1,2-Dichloroethene	2.757	96	16712	6.600	ug/L	95
20) cis-1,2-Dichloroethene	3.905	96	102574	38.163	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027191.D
Acq On : 03 Aug 2022 14:59
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Manual IntegrationsAPPROVED

Quant Time: Aug 04 03:03:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 04 02:57:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/04/2022
Supervised By :Mahesh Dadoda 08/05/2022

