

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027188.D
 Acq On : 03 Aug 2022 11:30
 Operator : SY/MD
 Sample : VV0803MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	100	rBV	204425	235634	12.21%	1.547%
2	1.555	154	160	177	rVB	126828	139027	7.20%	0.913%
3	2.095	319	328	342	rBV	445082	632907	32.79%	4.156%
4	2.552	467	470	471	rBV2	561	318	0.02%	0.002%
5	2.613	479	489	504	rBV	18301	37002	1.92%	0.243%
6	2.915	581	583	585	rVB	358	93	0.00%	0.001%
7	2.950	592	594	599	rBV2	422	185	0.01%	0.001%
8	3.031	616	619	621	rBV	328	246	0.01%	0.002%
9	3.230	678	681	686	rBV2	420	365	0.02%	0.002%
10	3.362	720	722	724	rBV	221	122	0.01%	0.001%
11	3.413	734	738	739	rBV	406	194	0.01%	0.001%
12	3.474	755	757	764	rVB3	458	387	0.02%	0.003%
13	3.507	764	767	771	rBV2	261	200	0.01%	0.001%
14	3.552	779	781	782	rBV	277	79	0.00%	0.001%
15	3.593	790	794	799	rVB3	512	496	0.03%	0.003%
16	3.619	799	802	807	rBV3	357	370	0.02%	0.002%
17	3.642	807	809	813	rBV2	166	135	0.01%	0.001%
18	3.728	832	836	837	rBV2	174	124	0.01%	0.001%
19	3.873	867	881	927	rBV2	153396	518263	26.85%	3.403%
20	4.336	1010	1025	1065	rBV	315160	792476	41.06%	5.203%
21	4.741	1149	1151	1153	rVB2	185	71	0.00%	0.000%
22	4.757	1153	1156	1158	rBV2	321	160	0.01%	0.001%
23	4.780	1162	1163	1164	rVB	276	53	0.00%	0.000%
24	4.806	1168	1171	1172	rBV	401	196	0.01%	0.001%
25	4.860	1185	1188	1189	rBV2	214	114	0.01%	0.001%
26	4.912	1201	1204	1205	rBV	241	108	0.01%	0.001%
27	4.928	1207	1209	1212	rVB	365	158	0.01%	0.001%
28	4.947	1212	1215	1216	rBV	202	118	0.01%	0.001%
29	4.979	1223	1225	1226	rBV	209	114	0.01%	0.001%
30	5.034	1226	1242	1289	rVV2	737845	1930274	100.00%	12.674%
31	5.397	1353	1355	1358	rBV3	714	499	0.03%	0.003%
32	5.461	1371	1375	1378	rBV5	340	326	0.02%	0.002%
33	5.529	1393	1396	1402	rVB4	613	566	0.03%	0.004%
34	5.564	1402	1407	1408	rBV3	536	461	0.02%	0.003%
35	5.606	1408	1420	1450	rBV	677580	1400267	72.54%	9.194%
36	5.899	1500	1511	1528	rBV5	15715	34905	1.81%	0.229%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027188.D
 Acq On : 03 Aug 2022 11:30
 Operator : SY/MD
 Sample : VV0803MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.059	1548	1561	1595	rBV	426601	886229	45.91%	5.819%
38	6.314	1635	1640	1648	rVB4	874	883	0.05%	0.006%
39	6.349	1648	1651	1654	rVB3	341	152	0.01%	0.001%
40	6.400	1665	1667	1669	rBV	181	78	0.00%	0.001%
41	6.461	1683	1686	1691	rVB	691	319	0.02%	0.002%
42	6.487	1691	1694	1696	rBV2	305	224	0.01%	0.001%
43	6.535	1706	1709	1711	rBV2	207	113	0.01%	0.001%
44	6.548	1711	1713	1716	rVB2	295	156	0.01%	0.001%
45	6.577	1716	1722	1727	rBV3	281	364	0.02%	0.002%
46	6.603	1729	1730	1732	rVB	155	33	0.00%	0.000%
47	6.616	1732	1734	1735	rBV2	570	253	0.01%	0.002%
48	6.632	1735	1739	1743	rBV5	1532	1766	0.09%	0.012%
49	6.780	1783	1785	1790	rVB2	264	156	0.01%	0.001%
50	6.805	1790	1793	1795	rBV	231	149	0.01%	0.001%
51	6.883	1815	1817	1819	rBV	144	67	0.00%	0.000%
52	6.899	1819	1822	1824	rVB2	331	168	0.01%	0.001%
53	6.912	1824	1826	1832	rVB2	195	112	0.01%	0.001%
54	6.940	1832	1835	1836	rBV	109	59	0.00%	0.000%
55	6.979	1836	1847	1872	rBV	207521	390172	20.21%	2.562%
56	7.310	1938	1950	1979	rBV	829976	1459169	75.59%	9.581%
57	7.616	2036	2045	2080	rVB	147297	265581	13.76%	1.744%
58	7.831	2109	2112	2113	rBV2	401	212	0.01%	0.001%
59	7.953	2148	2150	2152	rBV	297	122	0.01%	0.001%
60	7.973	2152	2156	2166	rVV5	1774	2378	0.12%	0.016%
61	8.011	2166	2168	2171	rVB2	207	61	0.00%	0.000%
62	8.050	2178	2180	2181	rBV2	213	93	0.00%	0.001%
63	8.085	2181	2191	2236	rVV	455597	877612	45.47%	5.762%
64	8.561	2337	2339	2341	rBV	261	127	0.01%	0.001%
65	8.773	2402	2405	2408	rVB2	435	253	0.01%	0.002%
66	8.847	2413	2428	2458	rBV	1031340	1686683	87.38%	11.075%
67	9.355	2584	2586	2589	rBV	408	243	0.01%	0.002%
68	9.426	2605	2608	2611	rBV2	239	168	0.01%	0.001%
69	9.465	2617	2620	2623	rBV	183	148	0.01%	0.001%
70	9.628	2670	2671	2672	rBV	229	78	0.00%	0.001%
71	9.767	2712	2714	2717	rBV	274	174	0.01%	0.001%
72	9.828	2730	2733	2736	rBV2	293	249	0.01%	0.002%
73	9.857	2739	2742	2745	rVV2	401	217	0.01%	0.001%
74	9.876	2745	2748	2750	rVB2	298	169	0.01%	0.001%
75	9.905	2755	2757	2759	rBV2	250	132	0.01%	0.001%
76	10.037	2794	2798	2802	rBV3	480	491	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027188.D
 Acq On : 03 Aug 2022 11:30
 Operator : SY/MD
 Sample : VV0803MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	10.130	2823	2827	2835	rVB2	470	653	0.03%	0.004%
78	10.165	2835	2838	2840	rBV	272	207	0.01%	0.001%
79	10.214	2840	2853	2878	rBV	645721	1034991	53.62%	6.796%
80	10.413	2913	2915	2917	rBV	261	135	0.01%	0.001%
81	10.429	2917	2920	2921	rBV	315	174	0.01%	0.001%
82	10.497	2938	2941	2942	rBV	234	124	0.01%	0.001%
83	10.542	2950	2955	2956	rBV3	706	538	0.03%	0.004%
84	10.580	2964	2967	2968	rBV2	587	314	0.02%	0.002%
85	10.831	3043	3045	3046	rBV2	220	79	0.00%	0.001%
86	10.915	3068	3071	3075	rBV3	940	964	0.05%	0.006%
87	10.960	3083	3085	3087	rBV	270	152	0.01%	0.001%
88	11.085	3120	3124	3128	rBV2	435	363	0.02%	0.002%
89	11.185	3149	3155	3163	rBV4	3711	5671	0.29%	0.037%
90	11.246	3163	3174	3204	rVV	944278	1460529	75.66%	9.590%
91	11.558	3267	3271	3273	rBV3	383	279	0.01%	0.002%
92	11.622	3278	3291	3317	rBV	847785	1330449	68.93%	8.736%
93	12.326	3507	3510	3512	rBV	620	308	0.02%	0.002%
94	12.648	3601	3610	3626	rBV4	6154	9411	0.49%	0.062%
95	12.966	3708	3709	3711	rBV2	379	104	0.01%	0.001%
96	13.152	3763	3767	3768	rBV	537	408	0.02%	0.003%
97	13.262	3794	3801	3814	rVB3	9313	14238	0.74%	0.093%
98	13.503	3868	3876	3894	rVB	29717	49191	2.55%	0.323%
99	13.744	3944	3951	3966	rVB3	11483	18149	0.94%	0.119%



Sum of corrected areas: 15230257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027188.D
Acq On : 03 Aug 2022 11:30
Operator : SY/MD
Sample : VV0803MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

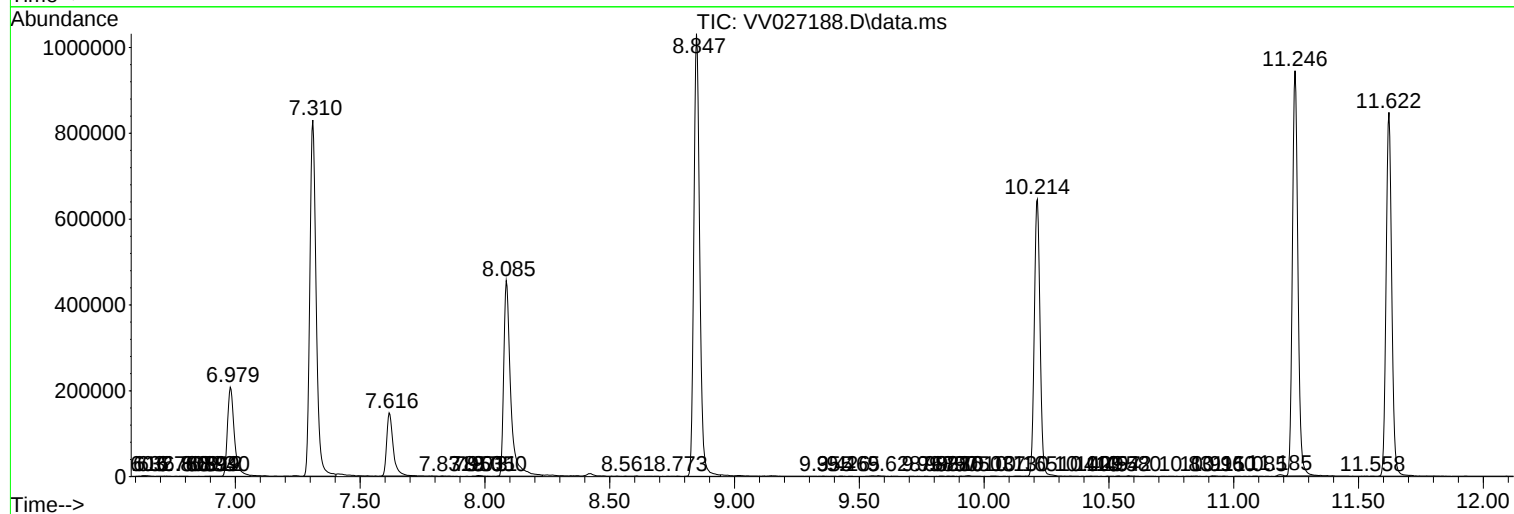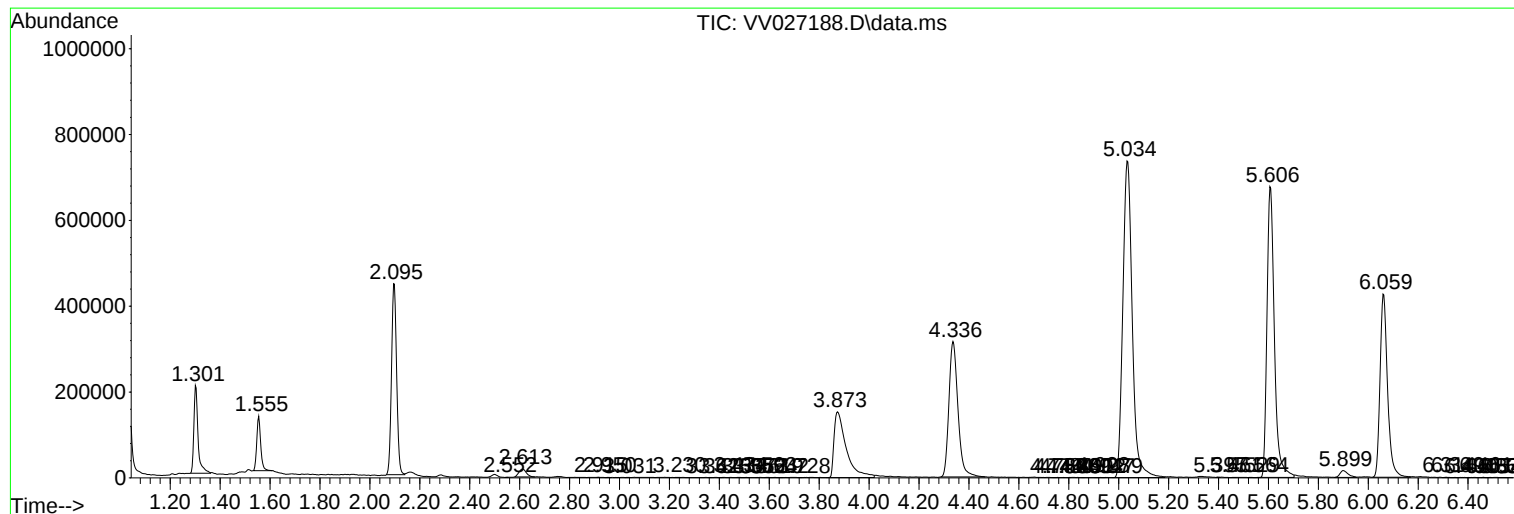

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027188.D
Acq On : 03 Aug 2022 11:30
Operator : SY/MD
Sample : VV0803MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027188.D
Acq On : 03 Aug 2022 11:30
Operator : SY/MD
Sample : VV0803MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc