

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027190.D
 Acq On : 03 Aug 2022 14:34
 Operator : SY/MD
 Sample : N4003-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

Signal : TIC: VV027190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	102	rBV2	827598	948194	47.01%	5.675%
2	1.561	154	162	177	rVB	209830	244567	12.13%	1.464%
3	2.101	319	330	342	rBV	373520	525836	26.07%	3.147%
4	2.288	381	388	398	rBV6	2442	4660	0.23%	0.028%
5	2.381	415	417	420	rBV2	503	339	0.02%	0.002%
6	2.500	445	454	465	rBV2	7297	11986	0.59%	0.072%
7	2.609	479	488	499	rBV3	3053	5752	0.29%	0.034%
8	2.754	523	533	552	rVB	37806	67642	3.35%	0.405%
9	2.944	589	592	597	rVB2	363	251	0.01%	0.002%
10	3.034	616	620	623	rBV2	414	305	0.02%	0.002%
11	3.050	623	625	631	rVB	428	411	0.02%	0.002%
12	3.098	637	640	646	rVB2	390	374	0.02%	0.002%
13	3.375	723	726	732	rVB2	253	233	0.01%	0.001%
14	3.481	757	759	765	rVB	257	233	0.01%	0.001%
15	3.580	788	790	794	rBV2	255	229	0.01%	0.001%
16	3.870	868	880	930	rBV2	237557	770435	38.20%	4.611%
17	4.339	1009	1026	1048	rBV	374289	933415	46.28%	5.586%
18	4.770	1155	1160	1162	rBV2	394	270	0.01%	0.002%
19	4.841	1179	1182	1186	rVB2	369	266	0.01%	0.002%
20	4.866	1186	1190	1193	rVB3	324	271	0.01%	0.002%
21	4.915	1202	1205	1209	rBV2	284	249	0.01%	0.001%
22	5.037	1225	1243	1288	rBV2	739571	2017013	100.00%	12.071%
23	5.239	1304	1306	1309	rVB4	684	385	0.02%	0.002%
24	5.294	1320	1323	1328	rVB4	620	489	0.02%	0.003%
25	5.333	1333	1335	1338	rBV2	312	230	0.01%	0.001%
26	5.410	1357	1359	1362	rVB	702	275	0.01%	0.002%
27	5.529	1390	1396	1401	rBV2	319	313	0.02%	0.002%
28	5.609	1408	1421	1459	rBV	522363	1107868	54.93%	6.630%
29	5.850	1493	1496	1499	rBV2	530	360	0.02%	0.002%
30	5.902	1501	1512	1525	rBV3	16319	36849	1.83%	0.221%
31	6.063	1547	1562	1592	rBV	476432	995683	49.36%	5.959%
32	6.275	1627	1628	1631	rVB3	589	324	0.02%	0.002%
33	6.294	1631	1634	1637	rBV3	630	400	0.02%	0.002%
34	6.365	1652	1656	1657	rVV3	398	251	0.01%	0.002%
35	6.397	1663	1666	1670	rVV2	501	391	0.02%	0.002%
36	6.487	1690	1694	1697	rVB2	329	270	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027190.D
 Acq On : 03 Aug 2022 14:34
 Operator : SY/MD
 Sample : N4003-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.506	1697	1700	1704	rBV	316	273	0.01%	0.002%
38	6.558	1713	1716	1721	rVB	377	284	0.01%	0.002%
39	6.767	1779	1781	1787	rVB2	361	302	0.01%	0.002%
40	6.841	1799	1804	1807	rBV3	317	337	0.02%	0.002%
41	6.979	1836	1847	1875	rBV	226186	438883	21.76%	2.627%
42	7.111	1886	1888	1894	rVB2	860	645	0.03%	0.004%
43	7.159	1898	1903	1904	rBV2	666	560	0.03%	0.003%
44	7.185	1909	1911	1914	rVB3	524	237	0.01%	0.001%
45	7.310	1938	1950	1980	rBV	643110	1179807	58.49%	7.061%
46	7.616	2035	2045	2072	rBV	167883	310192	15.38%	1.856%
47	7.860	2116	2121	2123	rBV3	358	291	0.01%	0.002%
48	7.943	2142	2147	2149	rBV4	607	509	0.03%	0.003%
49	8.085	2180	2191	2234	rBV	749982	1410422	69.93%	8.441%
50	8.423	2286	2296	2305	rBV7	3454	6968	0.35%	0.042%
51	8.513	2320	2324	2328	rBV4	494	479	0.02%	0.003%
52	8.606	2346	2353	2358	rBV4	332	438	0.02%	0.003%
53	8.702	2381	2383	2391	rVB4	554	605	0.03%	0.004%
54	8.741	2391	2395	2396	rBV	409	307	0.02%	0.002%
55	8.751	2396	2398	2402	rVV3	434	354	0.02%	0.002%
56	8.850	2416	2429	2455	rBV	816639	1361679	67.51%	8.149%
57	9.149	2520	2522	2525	rVB	402	232	0.01%	0.001%
58	9.169	2525	2528	2530	rBV3	560	285	0.01%	0.002%
59	9.214	2538	2542	2545	rBV2	362	345	0.02%	0.002%
60	9.265	2556	2558	2562	rVB2	362	239	0.01%	0.001%
61	9.284	2562	2564	2568	rBV3	333	236	0.01%	0.001%
62	9.310	2568	2572	2575	rBV2	315	310	0.02%	0.002%
63	9.596	2658	2661	2665	rVB2	406	267	0.01%	0.002%
64	9.696	2688	2692	2696	rVB2	282	244	0.01%	0.001%
65	9.799	2718	2724	2726	rBV2	349	317	0.02%	0.002%
66	10.210	2840	2852	2881	rVV	937002	1487641	73.75%	8.903%
67	10.496	2937	2941	2948	rBV2	343	447	0.02%	0.003%
68	10.680	2995	2998	3005	rVB3	406	512	0.03%	0.003%
69	10.857	3046	3053	3058	rVB4	979	1116	0.06%	0.007%
70	11.191	3153	3157	3162	rVB3	865	796	0.04%	0.005%
71	11.246	3162	3174	3198	rBV	746567	1160201	57.52%	6.943%
72	11.432	3229	3232	3238	rVV3	610	541	0.03%	0.003%
73	11.477	3242	3246	3251	rBV3	589	496	0.02%	0.003%
74	11.551	3266	3269	3271	rBV3	502	308	0.02%	0.002%
75	11.622	3278	3291	3315	rBV	1072374	1654496	82.03%	9.902%
76	11.895	3374	3376	3380	rBV2	491	455	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027190.D
 Acq On : 03 Aug 2022 14:34
 Operator : SY/MD
 Sample : N4003-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.194	3467	3469	3474	rBV2	536	310	0.02%	0.002%
78	12.278	3491	3495	3497	rBV2	426	262	0.01%	0.002%
79	12.532	3571	3574	3577	rBV2	385	290	0.01%	0.002%
80	12.647	3607	3610	3614	rBV2	507	460	0.02%	0.003%
81	12.670	3615	3617	3620	rVB3	485	246	0.01%	0.001%
82	12.709	3626	3629	3630	rBV	423	228	0.01%	0.001%
83	12.837	3666	3669	3672	rBV2	374	304	0.02%	0.002%
84	12.914	3691	3693	3699	rVB3	531	395	0.02%	0.002%
85	12.953	3700	3705	3707	rVB3	298	296	0.01%	0.002%
86	13.252	3795	3798	3799	rBV	444	250	0.01%	0.001%
87	13.332	3820	3823	3826	rBV3	307	253	0.01%	0.002%
88	13.352	3826	3829	3837	rVB2	521	523	0.03%	0.003%
89	13.410	3843	3847	3850	rBV2	357	283	0.01%	0.002%
90	13.606	3906	3908	3913	rVB3	816	641	0.03%	0.004%
91	13.747	3948	3952	3956	rBV2	731	691	0.03%	0.004%
92	13.850	3980	3984	3988	rVB3	471	411	0.02%	0.002%
93	13.869	3988	3990	3992	rBV3	360	235	0.01%	0.001%
94	13.937	4008	4011	4013	rBV3	383	254	0.01%	0.002%
95	14.046	4042	4045	4047	rBV2	426	248	0.01%	0.001%
96	14.220	4095	4099	4103	rBV2	482	429	0.02%	0.003%
97	14.409	4155	4158	4159	rBV3	383	227	0.01%	0.001%
98	14.644	4229	4231	4236	rVB4	684	385	0.02%	0.002%
99	15.316	4438	4440	4443	rBV2	966	641	0.03%	0.004%
100	16.001	4649	4653	4655	rBV4	1108	985	0.05%	0.006%




Sum of corrected areas: 16709322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027190.D
Acq On : 03 Aug 2022 14:34
Operator : SY/MD
Sample : N4003-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

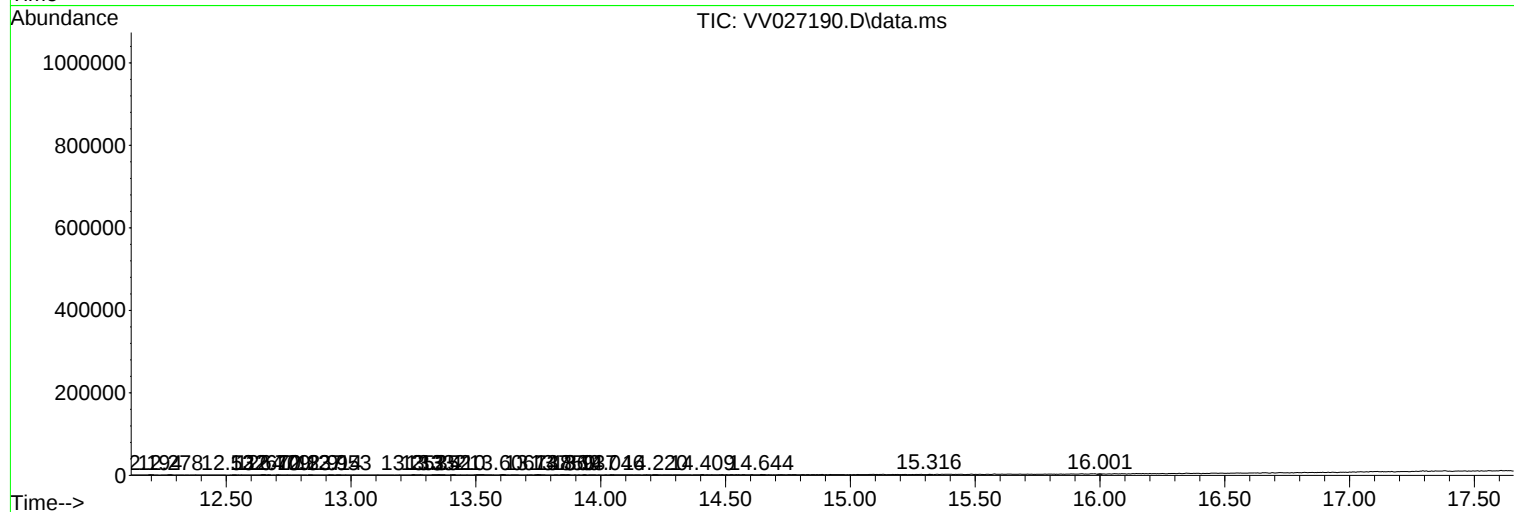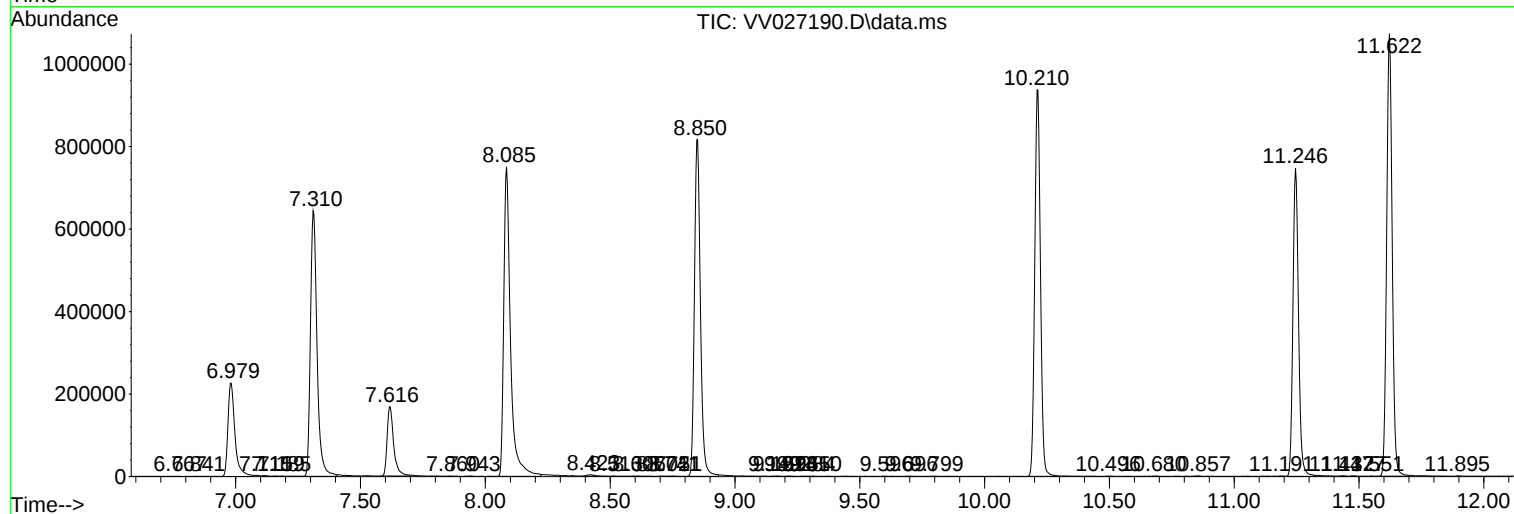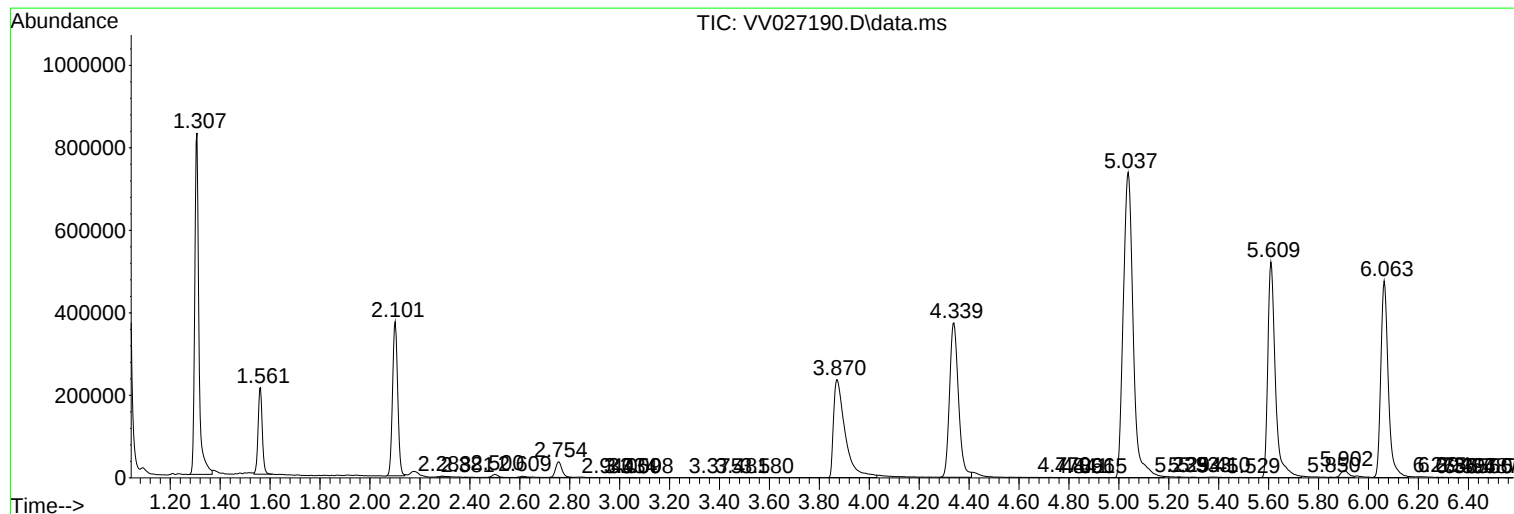

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027190.D
Acq On : 03 Aug 2022 14:34
Operator : SY/MD
Sample : N4003-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027190.D
Acq On : 03 Aug 2022 14:34
Operator : SY/MD
Sample : N4003-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc