

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027191.D
 Acq On : 03 Aug 2022 14:59
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	105	rBV2	1252734	1400318	100.00%	11.894%
2	1.561	155	162	176	rVB	138501	161574	11.54%	1.372%
3	2.101	320	330	345	rBV	229503	328610	23.47%	2.791%
4	2.294	381	390	398	rBV8	2333	5323	0.38%	0.045%
5	2.503	447	455	468	rVB	6073	9660	0.69%	0.082%
6	2.616	482	490	496	rBV3	1858	3437	0.25%	0.029%
7	2.757	523	534	555	rVV	41628	73513	5.25%	0.624%
8	2.847	558	562	565	rBV3	802	478	0.03%	0.004%
9	2.999	605	609	613	rBV2	482	446	0.03%	0.004%
10	3.044	620	623	629	rVB2	558	444	0.03%	0.004%
11	3.163	657	660	663	rBV2	314	241	0.02%	0.002%
12	3.278	692	696	699	rBV3	267	294	0.02%	0.002%
13	3.426	736	742	747	rVB2	354	386	0.03%	0.003%
14	3.581	785	790	794	rVV	489	412	0.03%	0.003%
15	3.609	794	799	803	rVV2	243	308	0.02%	0.003%
16	3.680	816	821	825	rVB3	408	399	0.03%	0.003%
17	3.735	832	838	842	rBV2	471	492	0.04%	0.004%
18	3.838	865	870	872	rBV3	409	411	0.03%	0.003%
19	3.899	872	889	914	rBV3	258540	927552	66.24%	7.878%
20	4.343	1007	1027	1049	rBV	234458	587331	41.94%	4.989%
21	4.597	1103	1106	1111	rVB5	531	425	0.03%	0.004%
22	4.629	1113	1116	1119	rBV3	388	292	0.02%	0.002%
23	4.896	1194	1199	1201	rBV2	484	311	0.02%	0.003%
24	5.040	1227	1244	1264	rBV2	455323	1207195	86.21%	10.254%
25	5.259	1310	1312	1316	rVB3	536	294	0.02%	0.002%
26	5.413	1355	1360	1368	rVB3	530	772	0.06%	0.007%
27	5.613	1411	1422	1468	rBV	358364	774640	55.32%	6.580%
28	5.789	1474	1477	1482	rVB6	971	763	0.05%	0.006%
29	5.905	1502	1513	1530	rBV3	11712	26962	1.93%	0.229%
30	6.066	1547	1563	1596	rBV	297236	625712	44.68%	5.315%
31	6.339	1644	1648	1652	rBV3	522	495	0.04%	0.004%
32	6.381	1657	1661	1664	rBV2	368	317	0.02%	0.003%
33	6.410	1668	1670	1673	rVB	515	256	0.02%	0.002%
34	6.503	1692	1699	1703	rBV3	221	242	0.02%	0.002%
35	6.532	1703	1708	1712	rBV2	381	346	0.02%	0.003%
36	6.854	1806	1808	1811	rBV	451	251	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027191.D
 Acq On : 03 Aug 2022 14:59
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.986	1838	1849	1875	rBV	134128	263486	18.82%	2.238%
38	7.150	1898	1900	1905	rVB4	487	286	0.02%	0.002%
39	7.313	1939	1951	1977	rBV	372948	694941	49.63%	5.903%
40	7.545	2018	2023	2027	rBV4	512	619	0.04%	0.005%
41	7.622	2037	2047	2071	rBV	98266	183330	13.09%	1.557%
42	7.834	2110	2113	2115	rVB2	585	336	0.02%	0.003%
43	7.854	2115	2119	2120	rBV	625	443	0.03%	0.004%
44	7.892	2128	2131	2133	rBV2	286	254	0.02%	0.002%
45	7.979	2155	2158	2162	rVB4	651	633	0.05%	0.005%
46	8.021	2169	2171	2175	rBV2	280	268	0.02%	0.002%
47	8.088	2181	2192	2227	rBV	432431	861441	61.52%	7.317%
48	8.413	2287	2293	2294	rBV3	3644	2611	0.19%	0.022%
49	8.561	2337	2339	2345	rVB3	482	357	0.03%	0.003%
50	8.693	2377	2380	2382	rBV2	400	247	0.02%	0.002%
51	8.741	2392	2395	2399	rVB	437	340	0.02%	0.003%
52	8.770	2399	2404	2407	rBV3	270	306	0.02%	0.003%
53	8.850	2415	2429	2459	rBV	562818	950068	67.85%	8.070%
54	9.069	2494	2497	2501	rVB4	438	364	0.03%	0.003%
55	9.143	2516	2520	2522	rBV3	303	282	0.02%	0.002%
56	9.239	2547	2550	2554	rBV3	328	307	0.02%	0.003%
57	9.339	2580	2581	2587	rVB	292	261	0.02%	0.002%
58	9.368	2587	2590	2594	rVB3	503	374	0.03%	0.003%
59	9.394	2594	2598	2600	rBV2	401	303	0.02%	0.003%
60	9.413	2600	2604	2607	rBV3	332	263	0.02%	0.002%
61	9.529	2634	2640	2641	rBV2	363	309	0.02%	0.003%
62	9.744	2700	2707	2713	rBV3	304	441	0.03%	0.004%
63	9.834	2730	2735	2737	rBV2	489	333	0.02%	0.003%
64	10.214	2840	2853	2874	rBV	588439	939894	67.12%	7.983%
65	10.487	2934	2938	2941	rBV4	295	246	0.02%	0.002%
66	10.632	2979	2983	2985	rBV2	343	253	0.02%	0.002%
67	10.799	3029	3035	3036	rBV2	425	390	0.03%	0.003%
68	10.850	3049	3051	3055	rVB2	384	241	0.02%	0.002%
69	10.966	3083	3087	3092	rVV	15272	8707	0.62%	0.074%
70	10.998	3092	3097	3099	rBV3	341	246	0.02%	0.002%
71	11.018	3099	3103	3107	rVB3	402	320	0.02%	0.003%
72	11.046	3110	3112	3118	rVB2	434	372	0.03%	0.003%
73	11.143	3137	3142	3143	rBV2	534	391	0.03%	0.003%
74	11.191	3150	3157	3162	rBV2	813	900	0.06%	0.008%
75	11.249	3163	3175	3201	rBV	485609	769945	54.98%	6.540%
76	11.468	3240	3243	3246	rVV2	552	358	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027191.D
 Acq On : 03 Aug 2022 14:59
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.487	3246	3249	3253	rVB2	484	397	0.03%	0.003%
78	11.506	3253	3255	3257	rBV	419	244	0.02%	0.002%
79	11.519	3257	3259	3263	rVB2	659	367	0.03%	0.003%
80	11.551	3264	3269	3271	rBV3	442	420	0.03%	0.004%
81	11.622	3279	3291	3311	rBV	600228	935833	66.83%	7.949%
82	12.339	3510	3514	3518	rBV2	353	360	0.03%	0.003%
83	12.992	3713	3717	3721	rVB2	300	251	0.02%	0.002%
84	13.034	3726	3730	3735	rBV3	398	478	0.03%	0.004%
85	13.275	3801	3805	3811	rBV5	673	703	0.05%	0.006%
86	13.394	3840	3842	3844	rBV2	501	307	0.02%	0.003%
87	13.519	3875	3881	3888	rBV4	988	1503	0.11%	0.013%
88	13.567	3893	3896	3897	rBV	442	272	0.02%	0.002%
89	13.680	3925	3931	3934	rBV3	386	474	0.03%	0.004%
90	13.770	3956	3959	3967	rVB4	606	666	0.05%	0.006%
91	13.853	3981	3985	3988	rBV4	530	481	0.03%	0.004%
92	13.937	4008	4011	4014	rBV2	516	332	0.02%	0.003%
93	14.239	4100	4105	4107	rBV2	335	344	0.02%	0.003%
94	14.304	4122	4125	4127	rBV2	441	327	0.02%	0.003%
95	14.667	4234	4238	4239	rBV2	491	351	0.03%	0.003%
96	14.693	4244	4246	4249	rBV3	468	308	0.02%	0.003%
97	14.802	4278	4280	4286	rVB2	667	565	0.04%	0.005%
98	14.834	4286	4290	4291	rBV2	672	556	0.04%	0.005%
99	14.863	4296	4299	4300	rBV	619	345	0.02%	0.003%
100	15.143	4379	4386	4390	rBV5	770	1112	0.08%	0.009%




Sum of corrected areas: 11773364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027191.D
Acq On : 03 Aug 2022 14:59
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

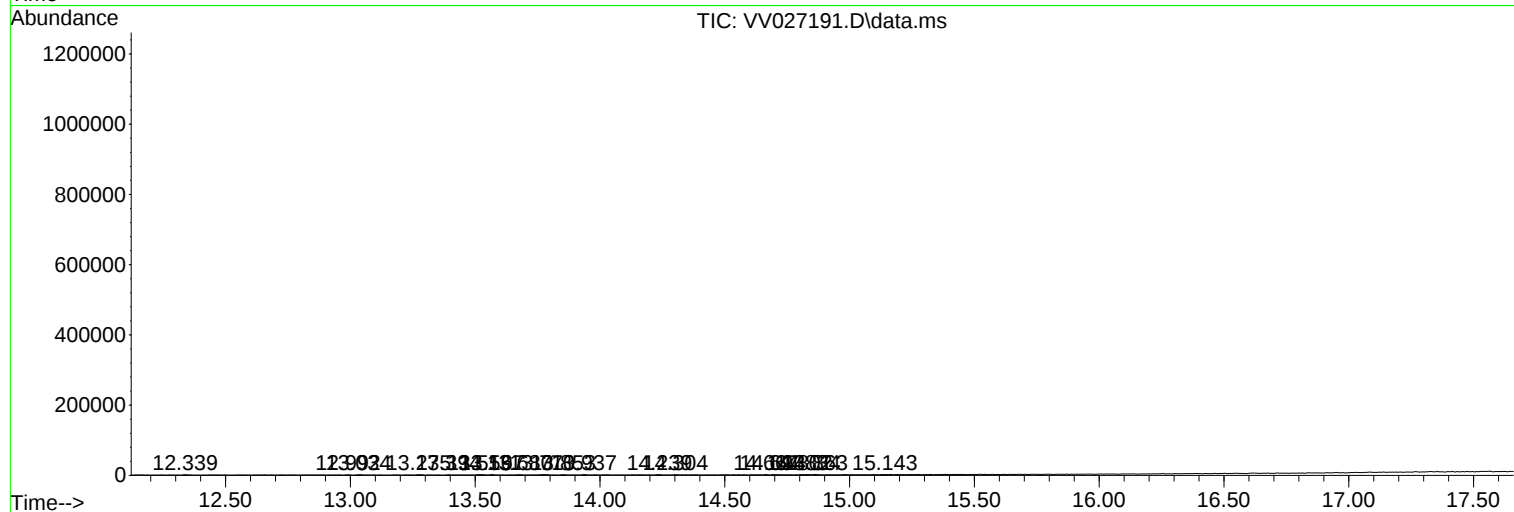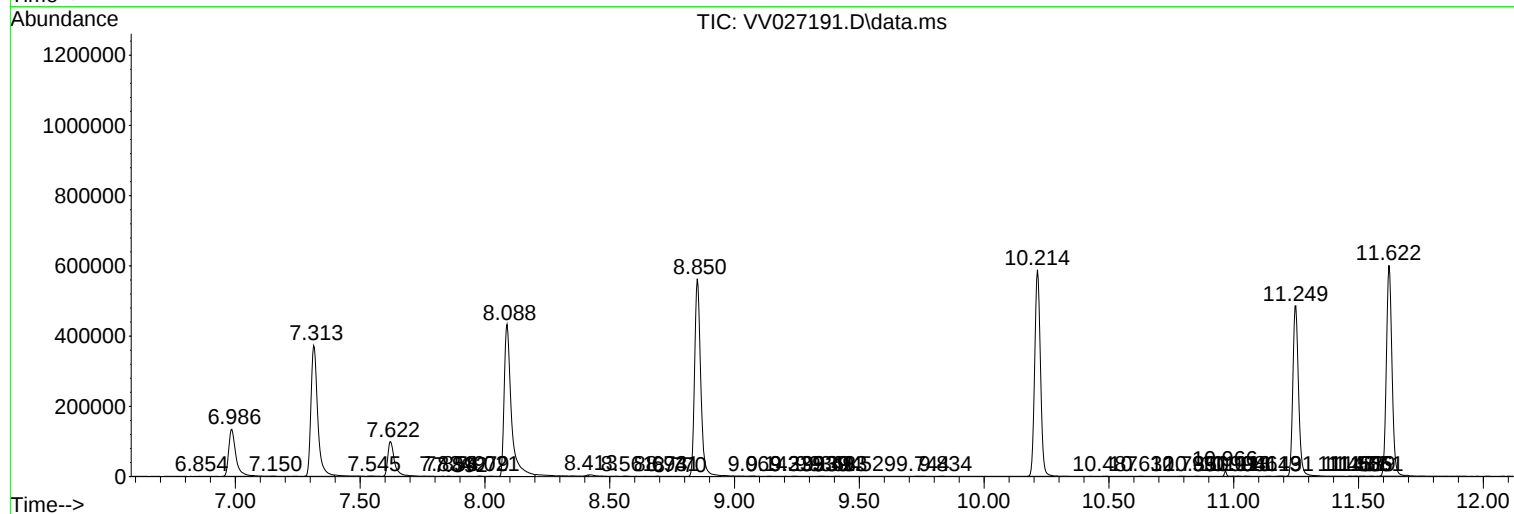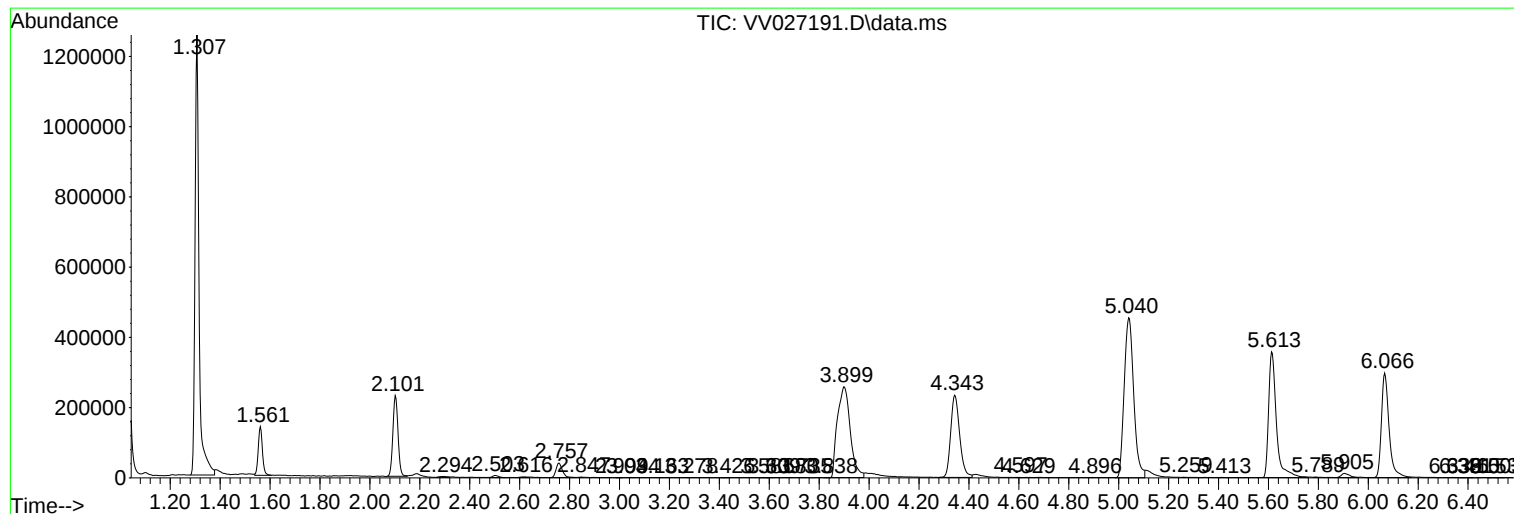

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027191.D
Acq On : 03 Aug 2022 14:59
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027191.D
Acq On : 03 Aug 2022 14:59
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------