

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027193.D
 Acq On : 03 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4005-03DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

Signal : TIC: VV027193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	140804	155163	8.70%	1.060%
2	1.561	155	162	175	rVB	144733	164194	9.21%	1.121%
3	2.101	320	330	342	rBV	242046	340589	19.10%	2.326%
4	2.294	381	390	392	rBV4	3451	4277	0.24%	0.029%
5	2.500	445	454	468	rVB3	6508	11272	0.63%	0.077%
6	2.616	484	490	497	rBV4	1691	2564	0.14%	0.018%
7	2.693	511	514	520	rBV4	529	432	0.02%	0.003%
8	2.754	520	533	552	rBV	1044177	1782914	100.00%	12.178%
9	2.851	555	563	584	rVB2	24471	63376	3.55%	0.433%
10	3.027	614	618	622	rBV3	506	499	0.03%	0.003%
11	3.214	673	676	681	rBV2	369	259	0.01%	0.002%
12	3.291	696	700	703	rBV3	241	261	0.01%	0.002%
13	3.326	709	711	716	rVB2	544	433	0.02%	0.003%
14	3.355	716	720	721	rBV2	502	317	0.02%	0.002%
15	3.397	728	733	736	rBV3	229	272	0.02%	0.002%
16	3.433	741	744	752	rBV2	485	672	0.04%	0.005%
17	3.609	791	799	807	rBV2	496	796	0.04%	0.005%
18	3.664	807	816	819	rBV3	431	594	0.03%	0.004%
19	3.680	819	821	828	rVB3	350	330	0.02%	0.002%
20	3.744	836	841	843	rBV2	329	303	0.02%	0.002%
21	3.902	870	890	914	rBV3	428130	1373880	77.06%	9.384%
22	4.278	1005	1007	1010	rBV2	549	337	0.02%	0.002%
23	4.342	1011	1027	1048	rBV	248719	614934	34.49%	4.200%
24	4.654	1121	1124	1128	rVB3	433	337	0.02%	0.002%
25	4.674	1128	1130	1135	rBV2	416	392	0.02%	0.003%
26	4.719	1141	1144	1150	rVB2	469	476	0.03%	0.003%
27	4.744	1150	1152	1157	rBV2	486	424	0.02%	0.003%
28	4.802	1166	1170	1173	rBV2	582	405	0.02%	0.003%
29	4.918	1202	1206	1208	rBV	376	280	0.02%	0.002%
30	5.040	1228	1244	1293	rBV2	491146	1337702	75.03%	9.137%
31	5.400	1353	1356	1358	rBV2	431	289	0.02%	0.002%
32	5.474	1375	1379	1384	rBV3	583	673	0.04%	0.005%
33	5.526	1392	1395	1399	rBV2	388	296	0.02%	0.002%
34	5.613	1409	1422	1469	rBV	542075	1168697	65.55%	7.982%
35	5.834	1489	1491	1495	rBV4	481	351	0.02%	0.002%
36	5.915	1502	1516	1543	rBV3	55604	134481	7.54%	0.919%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027193.D
 Acq On : 03 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4005-03DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.066	1550	1563	1600	rBV2	318215	674718	37.84%	4.608%
38	6.252	1618	1621	1628	rVB5	967	967	0.05%	0.007%
39	6.320	1639	1642	1645	rVB2	501	339	0.02%	0.002%
40	6.339	1645	1648	1652	rBV2	358	316	0.02%	0.002%
41	6.387	1660	1663	1666	rVB3	372	256	0.01%	0.002%
42	6.423	1671	1674	1680	rVB4	319	278	0.02%	0.002%
43	6.452	1680	1683	1686	rBV2	335	247	0.01%	0.002%
44	6.510	1697	1701	1705	rVV2	403	462	0.03%	0.003%
45	6.529	1705	1707	1711	rVV3	433	341	0.02%	0.002%
46	6.696	1755	1759	1766	rVB3	315	409	0.02%	0.003%
47	6.844	1799	1805	1806	rBV2	432	349	0.02%	0.002%
48	6.924	1828	1830	1834	rVB3	368	245	0.01%	0.002%
49	6.985	1838	1849	1871	rBV	144749	280015	15.71%	1.913%
50	7.313	1940	1951	1977	rBV	407849	745168	41.79%	5.090%
51	7.622	2036	2047	2078	rBV2	106179	200136	11.23%	1.367%
52	7.799	2097	2102	2106	rVB3	672	642	0.04%	0.004%
53	7.973	2152	2156	2157	rBV2	413	259	0.01%	0.002%
54	8.088	2176	2192	2231	rBV	486469	947866	53.16%	6.474%
55	8.336	2266	2269	2277	rVB7	663	678	0.04%	0.005%
56	8.423	2291	2296	2299	rVB3	842	680	0.04%	0.005%
57	8.468	2307	2310	2312	rBV	642	342	0.02%	0.002%
58	8.551	2332	2336	2339	rBV	535	385	0.02%	0.003%
59	8.622	2352	2358	2363	rBV4	586	750	0.04%	0.005%
60	8.728	2388	2391	2396	rVB2	456	361	0.02%	0.002%
61	8.805	2411	2415	2417	rBV3	478	390	0.02%	0.003%
62	8.850	2417	2429	2463	rBV	864820	1430482	80.23%	9.770%
63	9.146	2517	2521	2524	rBV3	545	462	0.03%	0.003%
64	9.191	2529	2535	2536	rBV3	439	382	0.02%	0.003%
65	9.281	2560	2563	2565	rVV2	358	278	0.02%	0.002%
66	9.516	2632	2636	2639	rBV2	516	411	0.02%	0.003%
67	9.654	2675	2679	2686	rBV3	381	480	0.03%	0.003%
68	9.818	2728	2730	2735	rVB3	396	272	0.02%	0.002%
69	9.963	2771	2775	2778	rVV3	353	298	0.02%	0.002%
70	10.124	2820	2825	2827	rBV	375	294	0.02%	0.002%
71	10.214	2840	2853	2876	rBV	633574	1006254	56.44%	6.873%
72	10.532	2950	2952	2956	rVV	393	336	0.02%	0.002%
73	10.751	3016	3020	3023	rBV2	388	287	0.02%	0.002%
74	10.850	3048	3051	3054	rBV	612	357	0.02%	0.002%
75	10.931	3069	3076	3081	rVB3	562	803	0.05%	0.005%
76	10.972	3081	3089	3092	rBV3	478	695	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027193.D
 Acq On : 03 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4005-03DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.188	3153	3156	3160	rVB2	524	441	0.02%	0.003%
78	11.249	3163	3175	3203	rBV	737115	1157002	64.89%	7.902%
79	11.538	3261	3265	3267	rBV4	701	570	0.03%	0.004%
80	11.622	3278	3291	3315	rBV	638609	1011297	56.72%	6.907%
81	11.924	3383	3385	3388	rBV3	340	264	0.01%	0.002%
82	12.072	3429	3431	3434	rBV2	554	343	0.02%	0.002%
83	12.197	3465	3470	3479	rBV3	450	633	0.04%	0.004%
84	12.477	3554	3557	3560	rBV2	272	257	0.01%	0.002%
85	12.625	3600	3603	3607	rVB2	349	268	0.02%	0.002%
86	12.657	3607	3613	3618	rVB5	609	747	0.04%	0.005%
87	12.744	3637	3640	3644	rBV2	306	295	0.02%	0.002%
88	13.030	3727	3729	3735	rVB3	425	330	0.02%	0.002%
89	13.304	3811	3814	3817	rBV	540	377	0.02%	0.003%
90	13.342	3821	3826	3829	rBV3	435	486	0.03%	0.003%
91	13.644	3915	3920	3922	rBV2	555	564	0.03%	0.004%
92	13.709	3938	3940	3942	rBV2	441	261	0.01%	0.002%
93	13.992	4025	4028	4031	rBV2	514	340	0.02%	0.002%
94	14.541	4197	4199	4202	rBV3	403	286	0.02%	0.002%
95	14.766	4264	4269	4271	rBV3	587	546	0.03%	0.004%
96	14.863	4296	4299	4302	rVB3	751	480	0.03%	0.003%
97	14.879	4302	4304	4311	rBV4	884	1016	0.06%	0.007%
98	15.030	4349	4351	4355	rVB2	907	560	0.03%	0.004%
99	15.381	4456	4460	4462	rBV2	936	835	0.05%	0.006%
100	15.471	4485	4488	4491	rBV4	730	629	0.04%	0.004%




Sum of corrected areas: 14640988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027193.D
Acq On : 03 Aug 2022 15:48
Operator : SY/MD
Sample : N4005-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

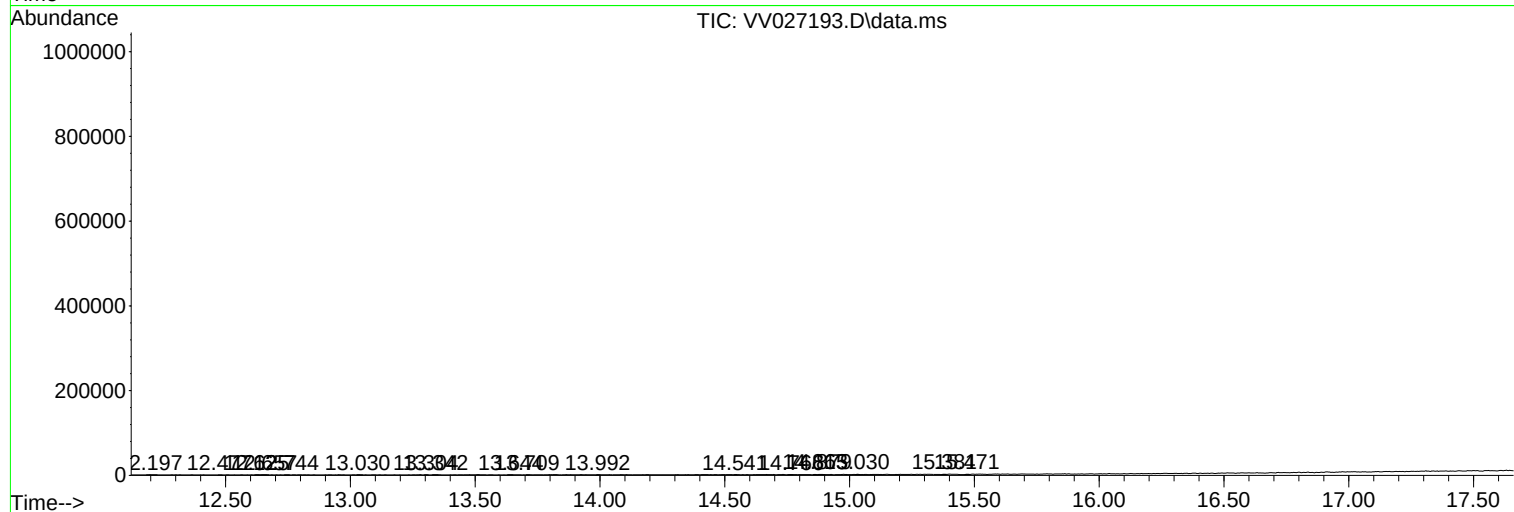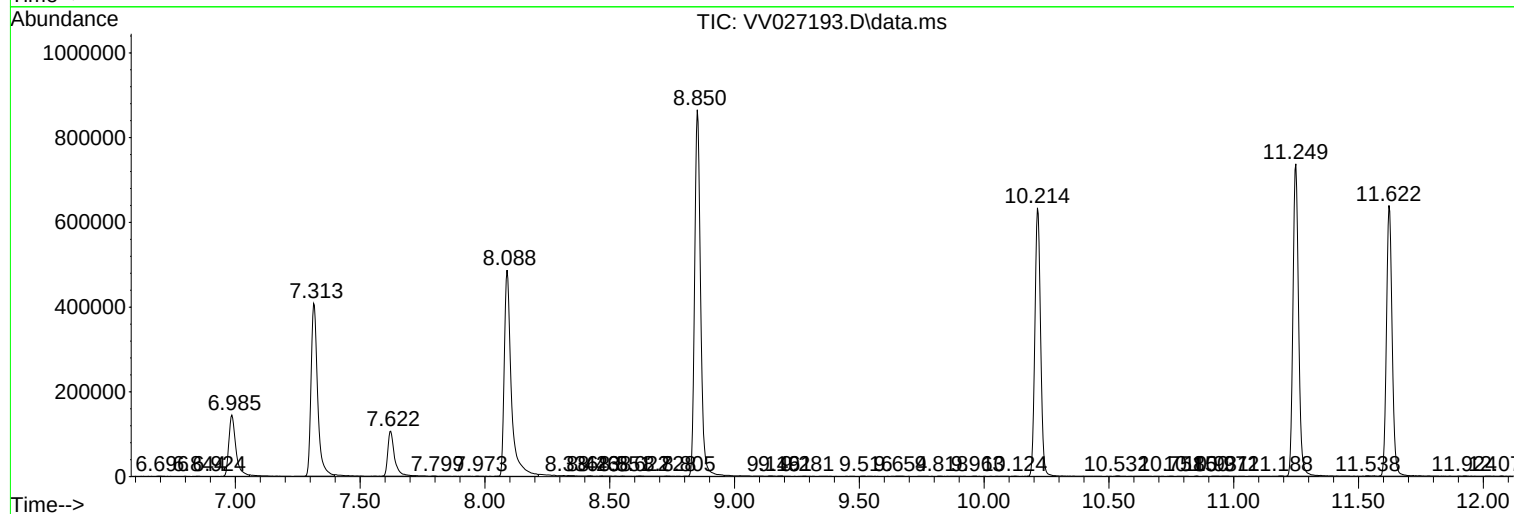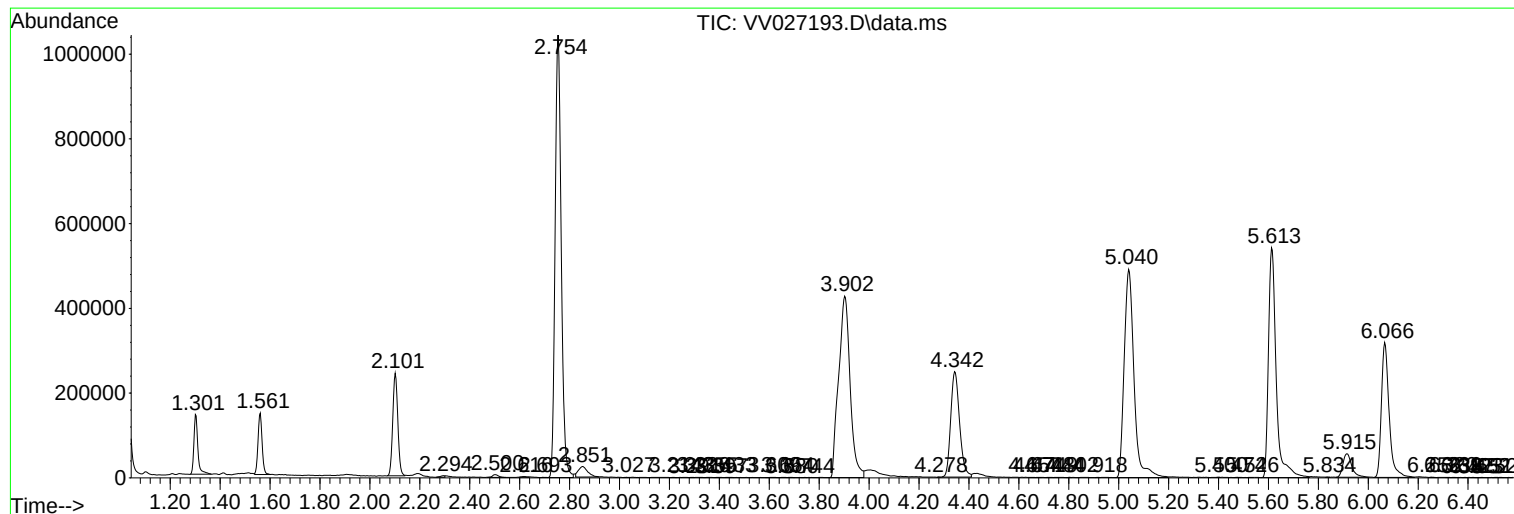

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027193.D
Acq On : 03 Aug 2022 15:48
Operator : SY/MD
Sample : N4005-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027193.D
Acq On : 03 Aug 2022 15:48
Operator : SY/MD
Sample : N4005-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc