

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027194.D
 Acq On : 03 Aug 2022 16:13
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

Signal : TIC: VV027194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	170877	181485	11.95%	1.247%
2	1.558	154	161	172	rVB	164359	188522	12.41%	1.295%
3	2.101	320	330	347	rBV	281750	395205	26.02%	2.715%
4	2.294	381	390	392	rBV5	2330	3088	0.20%	0.021%
5	2.503	446	455	464	rVB	7787	11517	0.76%	0.079%
6	2.616	480	490	491	rBV3	2127	2683	0.18%	0.018%
7	2.754	521	533	555	rBV	778593	1338781	88.15%	9.196%
8	2.857	556	565	589	rVB3	19897	51455	3.39%	0.353%
9	2.979	599	603	607	rVB3	405	360	0.02%	0.002%
10	3.024	613	617	620	rBV3	413	346	0.02%	0.002%
11	3.047	620	624	627	rVB4	645	530	0.03%	0.004%
12	3.259	685	690	697	rVV2	398	564	0.04%	0.004%
13	3.465	748	754	760	rVB3	354	505	0.03%	0.003%
14	3.902	870	890	915	rBV3	461538	1518774	100.00%	10.432%
15	4.342	1010	1027	1048	rBV	293887	724133	47.68%	4.974%
16	4.574	1097	1099	1103	rVB2	548	307	0.02%	0.002%
17	4.664	1124	1127	1131	rBV3	408	383	0.03%	0.003%
18	4.802	1167	1170	1172	rVV2	552	329	0.02%	0.002%
19	4.902	1196	1201	1205	rBV3	545	533	0.04%	0.004%
20	5.040	1227	1244	1262	rBV2	578883	1510177	99.43%	10.373%
21	5.413	1358	1360	1364	rVB4	642	403	0.03%	0.003%
22	5.436	1365	1367	1372	rVB4	605	345	0.02%	0.002%
23	5.522	1392	1394	1402	rVB3	295	351	0.02%	0.002%
24	5.612	1409	1422	1470	rBV	385042	837424	55.14%	5.752%
25	5.818	1484	1486	1489	rBV3	484	290	0.02%	0.002%
26	5.908	1503	1514	1536	rVB7	14852	36630	2.41%	0.252%
27	6.066	1550	1563	1596	rBV	373142	792407	52.17%	5.443%
28	6.204	1603	1606	1610	rBV4	1287	1040	0.07%	0.007%
29	6.288	1629	1632	1635	rVB3	465	326	0.02%	0.002%
30	6.349	1648	1651	1655	rBV2	342	324	0.02%	0.002%
31	6.371	1655	1658	1662	rVB	552	389	0.03%	0.003%
32	6.538	1707	1710	1714	rBV4	370	364	0.02%	0.003%
33	6.702	1756	1761	1764	rVB3	365	350	0.02%	0.002%
34	6.892	1816	1820	1824	rBV3	510	368	0.02%	0.003%
35	6.985	1838	1849	1883	rBV	173533	337945	22.25%	2.321%
36	7.313	1939	1951	1983	rBV	494482	911462	60.01%	6.261%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027194.D
 Acq On : 03 Aug 2022 16:13
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	7.619	2037	2046	2072	rBV	128040	236195	15.55%	1.622%
38	7.786	2096	2098	2104	rVB2	324	290	0.02%	0.002%
39	7.979	2155	2158	2160	rBV2	576	396	0.03%	0.003%
40	8.027	2172	2173	2178	rVB2	635	326	0.02%	0.002%
41	8.088	2181	2192	2223	rBV	615383	1168744	76.95%	8.028%
42	8.538	2327	2332	2334	rBV2	405	379	0.02%	0.003%
43	8.583	2344	2346	2351	rVB4	626	448	0.03%	0.003%
44	8.622	2356	2358	2364	rVB4	702	655	0.04%	0.004%
45	8.654	2364	2368	2371	rBV4	425	386	0.03%	0.003%
46	8.799	2407	2413	2414	rBV2	448	360	0.02%	0.002%
47	8.850	2418	2429	2452	rBV	613257	1019820	67.15%	7.005%
48	9.075	2496	2499	2507	rVB5	586	714	0.05%	0.005%
49	9.217	2541	2543	2546	rVB2	529	297	0.02%	0.002%
50	9.320	2571	2575	2577	rBV3	416	311	0.02%	0.002%
51	9.416	2603	2605	2610	rVB2	508	349	0.02%	0.002%
52	9.558	2647	2649	2652	rVV3	630	358	0.02%	0.002%
53	9.892	2748	2753	2757	rBV3	448	545	0.04%	0.004%
54	9.937	2761	2767	2773	rVB4	486	510	0.03%	0.004%
55	9.992	2779	2784	2786	rBV2	394	378	0.02%	0.003%
56	10.214	2841	2853	2881	rVV	762414	1203070	79.21%	8.264%
57	10.574	2963	2965	2972	rVB2	462	371	0.02%	0.003%
58	10.625	2977	2981	2989	rVB3	415	538	0.04%	0.004%
59	10.728	3008	3013	3015	rBV	510	439	0.03%	0.003%
60	10.886	3057	3062	3067	rVB3	328	356	0.02%	0.002%
61	10.931	3073	3076	3079	rBV3	414	297	0.02%	0.002%
62	10.988	3090	3094	3097	rBV3	439	437	0.03%	0.003%
63	11.062	3113	3117	3119	rBV	727	500	0.03%	0.003%
64	11.249	3163	3175	3201	rBV	530605	823271	54.21%	5.655%
65	11.361	3208	3210	3214	rVB3	644	363	0.02%	0.002%
66	11.458	3238	3240	3245	rVB2	607	429	0.03%	0.003%
67	11.496	3245	3252	3254	rBV3	518	577	0.04%	0.004%
68	11.529	3256	3262	3264	rBV4	1175	1056	0.07%	0.007%
69	11.622	3279	3291	3310	rBV	753913	1182693	77.87%	8.124%
70	11.956	3393	3395	3400	rVB2	434	301	0.02%	0.002%
71	12.107	3438	3442	3443	rBV2	928	585	0.04%	0.004%
72	12.146	3451	3454	3461	rVB4	506	431	0.03%	0.003%
73	12.365	3515	3522	3532	rVV3	5904	8373	0.55%	0.058%
74	12.413	3532	3537	3546	rVB4	2101	2355	0.16%	0.016%
75	12.467	3546	3554	3559	rBV4	2931	4272	0.28%	0.029%
76	12.512	3565	3568	3574	rBV5	1597	1763	0.12%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027194.D
 Acq On : 03 Aug 2022 16:13
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.638	3603	3607	3611	rBV3	664	561	0.04%	0.004%
78	12.725	3631	3634	3640	rVB4	759	563	0.04%	0.004%
79	12.776	3644	3650	3652	rBV3	388	423	0.03%	0.003%
80	12.882	3674	3683	3689	rBV7	2933	4102	0.27%	0.028%
81	12.950	3697	3704	3715	rVB5	4922	7638	0.50%	0.052%
82	13.004	3715	3721	3722	rBV	410	371	0.02%	0.003%
83	13.056	3728	3737	3749	rVB4	7237	12735	0.84%	0.087%
84	13.111	3749	3754	3758	rBV2	596	680	0.04%	0.005%
85	13.146	3763	3765	3769	rVB2	586	406	0.03%	0.003%
86	13.271	3801	3804	3809	rVB4	581	536	0.04%	0.004%
87	13.361	3828	3832	3835	rBV3	642	600	0.04%	0.004%
88	13.503	3866	3876	3877	rBV4	3565	4486	0.30%	0.031%
89	13.596	3899	3905	3907	rBV3	1114	1243	0.08%	0.009%
90	13.676	3924	3930	3933	rBV6	1454	1419	0.09%	0.010%
91	13.712	3938	3941	3951	rVB6	1366	1786	0.12%	0.012%
92	13.901	3997	4000	4003	rBV2	575	411	0.03%	0.003%
93	13.940	4008	4012	4014	rBV2	823	657	0.04%	0.005%
94	14.297	4117	4123	4129	rVB5	813	898	0.06%	0.006%
95	14.493	4181	4184	4187	rBV3	835	587	0.04%	0.004%
96	14.577	4206	4210	4217	rBV6	796	1194	0.08%	0.008%
97	14.818	4281	4285	4287	rBV4	1465	1064	0.07%	0.007%
98	14.901	4306	4311	4312	rBV2	884	678	0.04%	0.005%
99	15.297	4432	4434	4438	rVB3	1126	681	0.04%	0.005%
100	15.528	4503	4506	4508	rBV2	708	514	0.03%	0.004%




Sum of corrected areas: 14558266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027194.D
Acq On : 03 Aug 2022 16:13
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

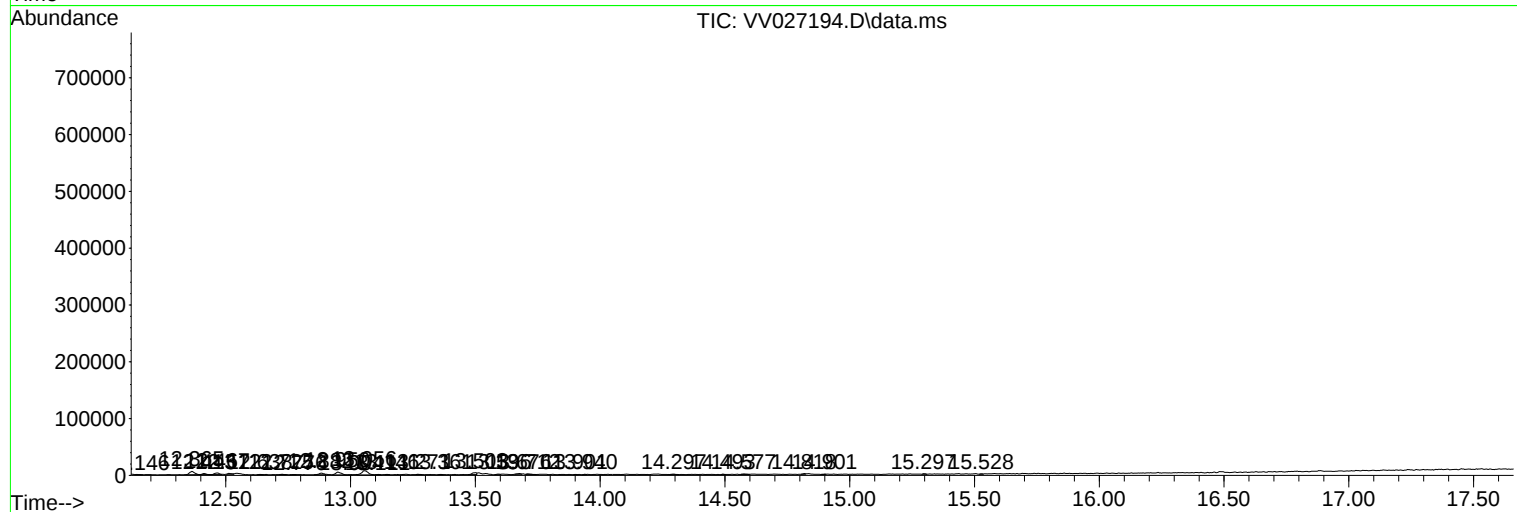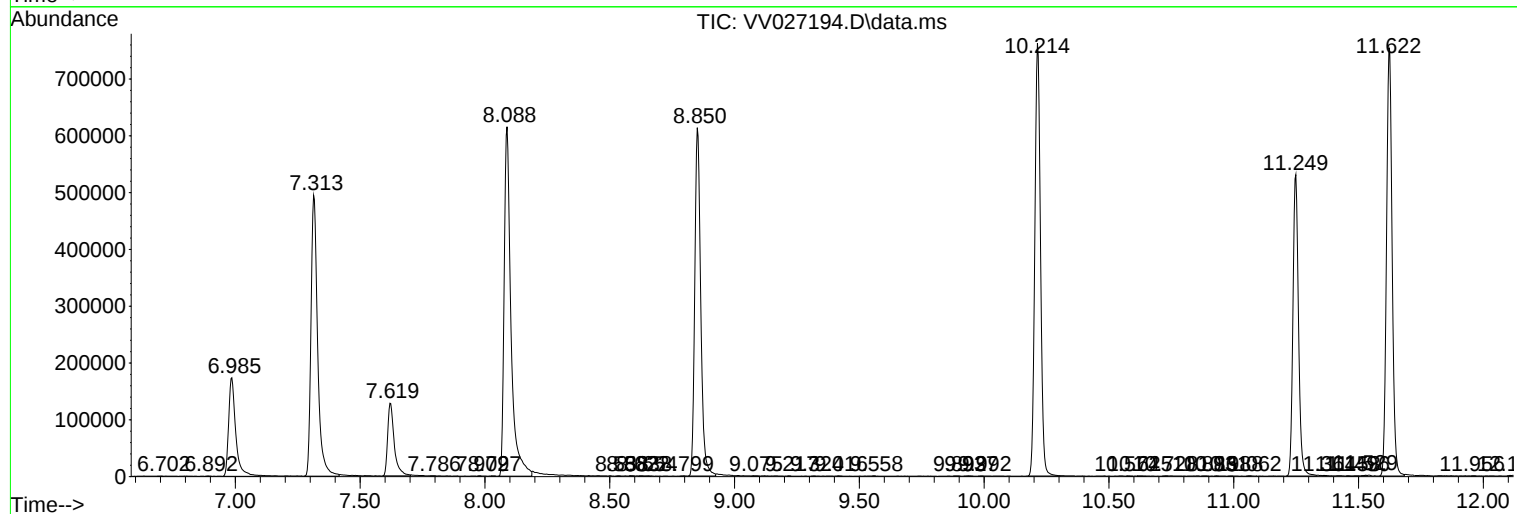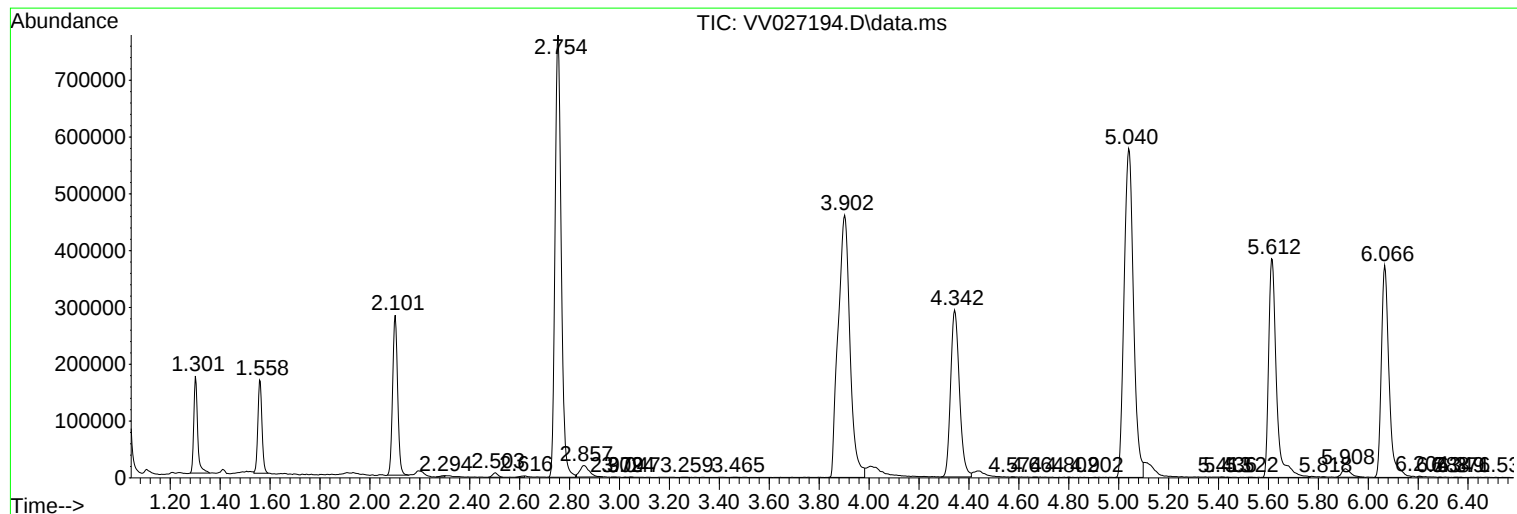

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027194.D
Acq On : 03 Aug 2022 16:13
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027194.D
Acq On : 03 Aug 2022 16:13
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc