

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027195.D
 Acq On : 03 Aug 2022 16:37
 Operator : SY/MD
 Sample : N4005-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

Signal : TIC: VV027195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	102	rVB	142034	153741	8.49%	1.215%
2	1.558	155	161	173	rVB	132128	152733	8.44%	1.207%
3	2.101	321	330	344	rVB	219633	309778	17.11%	2.448%
4	2.500	447	454	464	rVB3	6498	9641	0.53%	0.076%
5	2.712	518	520	522	rBV2	440	239	0.01%	0.002%
6	2.754	522	533	553	rVV	150005	262253	14.48%	2.072%
7	2.979	600	603	605	rBV2	323	245	0.01%	0.002%
8	3.040	620	622	627	rVB2	635	520	0.03%	0.004%
9	3.117	644	646	650	rBV2	332	260	0.01%	0.002%
10	3.182	661	666	667	rBV2	102	76	0.00%	0.001%
11	3.275	693	695	697	rBV	341	172	0.01%	0.001%
12	3.346	713	717	718	rBV2	336	225	0.01%	0.002%
13	3.375	723	726	727	rBV	194	116	0.01%	0.001%
14	3.416	734	739	741	rBV	380	278	0.02%	0.002%
15	3.564	783	785	787	rVB	337	141	0.01%	0.001%
16	3.658	811	814	817	rBV2	248	195	0.01%	0.002%
17	3.716	828	832	836	rBV2	331	261	0.01%	0.002%
18	3.741	836	840	844	rBV2	375	327	0.02%	0.003%
19	3.825	863	866	868	rBV	174	89	0.00%	0.001%
20	3.838	868	870	871	rBV	109	48	0.00%	0.000%
21	3.902	871	890	917	rBV3	616145	1810541	100.00%	14.305%
22	4.342	1013	1027	1050	rBV	229841	564603	31.18%	4.461%
23	4.738	1149	1150	1151	rBV	463	106	0.01%	0.001%
24	4.757	1151	1156	1159	rVV4	580	588	0.03%	0.005%
25	4.783	1163	1164	1165	rBV4	287	85	0.00%	0.001%
26	4.912	1200	1204	1208	rBV4	443	365	0.02%	0.003%
27	5.040	1227	1244	1266	rBV2	458312	1220269	67.40%	9.641%
28	5.471	1374	1378	1379	rBV3	319	219	0.01%	0.002%
29	5.532	1396	1397	1398	rVB	357	69	0.00%	0.001%
30	5.568	1402	1408	1410	rBV3	544	545	0.03%	0.004%
31	5.613	1410	1422	1439	rBV	514825	1049298	57.95%	8.290%
32	5.912	1503	1515	1530	rBV6	18761	46387	2.56%	0.367%
33	6.066	1550	1563	1601	rBV	293628	630399	34.82%	4.981%
34	6.387	1660	1663	1665	rBV2	397	236	0.01%	0.002%
35	6.407	1667	1669	1675	rVV2	506	384	0.02%	0.003%
36	6.436	1675	1678	1680	rVB	513	230	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027195.D
 Acq On : 03 Aug 2022 16:37
 Operator : SY/MD
 Sample : N4005-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.477	1689	1691	1695	rBV2	242	168	0.01%	0.001%
38	6.600	1726	1729	1730	rBV	310	154	0.01%	0.001%
39	6.645	1739	1743	1745	rBV2	246	197	0.01%	0.002%
40	6.712	1760	1764	1767	rBV2	271	273	0.02%	0.002%
41	6.764	1775	1780	1784	rBV3	327	285	0.02%	0.002%
42	6.793	1784	1789	1793	rVB2	425	523	0.03%	0.004%
43	6.831	1797	1801	1803	rBV2	282	269	0.01%	0.002%
44	6.879	1813	1816	1820	rVB	197	128	0.01%	0.001%
45	6.905	1820	1824	1826	rBV	223	163	0.01%	0.001%
46	6.915	1826	1827	1828	rVB	195	38	0.00%	0.000%
47	6.937	1828	1834	1838	rVB3	285	335	0.02%	0.003%
48	6.985	1838	1849	1883	rBV	137189	269020	14.86%	2.126%
49	7.313	1940	1951	1979	rBV	375857	701890	38.77%	5.546%
50	7.622	2037	2047	2071	rBV	96447	181820	10.04%	1.437%
51	7.841	2112	2115	2119	rBV2	471	257	0.01%	0.002%
52	7.905	2129	2135	2142	rBV4	554	810	0.04%	0.006%
53	7.937	2142	2145	2151	rVB3	449	418	0.02%	0.003%
54	8.002	2163	2165	2167	rBV	201	117	0.01%	0.001%
55	8.088	2182	2192	2230	rBV	448248	899109	49.66%	7.104%
56	8.484	2313	2315	2318	rBV3	568	298	0.02%	0.002%
57	8.577	2341	2344	2346	rBV3	411	254	0.01%	0.002%
58	8.715	2383	2387	2392	rVB	338	247	0.01%	0.002%
59	8.741	2392	2395	2397	rBV2	198	117	0.01%	0.001%
60	8.850	2417	2429	2453	rBV	826911	1361038	75.17%	10.754%
61	9.156	2521	2524	2532	rVB6	1060	1091	0.06%	0.009%
62	9.188	2532	2534	2535	rBV2	314	107	0.01%	0.001%
63	9.223	2541	2545	2548	rBV3	453	410	0.02%	0.003%
64	9.252	2552	2554	2556	rVB	424	243	0.01%	0.002%
65	9.374	2587	2592	2594	rBV2	262	263	0.01%	0.002%
66	9.403	2599	2601	2603	rBV	296	136	0.01%	0.001%
67	9.548	2639	2646	2654	rBV3	1528	2275	0.13%	0.018%
68	9.654	2678	2679	2682	rBV	250	99	0.01%	0.001%
69	9.670	2682	2684	2687	rVV2	214	110	0.01%	0.001%
70	9.731	2700	2703	2706	rBV2	376	232	0.01%	0.002%
71	9.796	2721	2723	2726	rBV	207	101	0.01%	0.001%
72	9.886	2748	2751	2754	rBV	351	237	0.01%	0.002%
73	9.947	2764	2770	2774	rVB4	518	626	0.03%	0.005%
74	9.969	2774	2777	2778	rBV2	420	245	0.01%	0.002%
75	10.136	2827	2829	2833	rBV2	443	323	0.02%	0.003%
76	10.214	2841	2853	2879	rBV	611216	955314	52.76%	7.548%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027195.D
 Acq On : 03 Aug 2022 16:37
 Operator : SY/MD
 Sample : N4005-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

77	10.419	2915	2917	2919	rBV	377	246	0.01%	0.002%
78	10.690	2999	3001	3004	rBV2	232	111	0.01%	0.001%
79	10.815	3037	3040	3042	rBV2	410	291	0.02%	0.002%
80	11.249	3163	3175	3198	rBV	705152	1104850	61.02%	8.729%
81	11.622	3280	3291	3316	rBV	592353	943833	52.13%	7.457%
82	12.648	3607	3610	3613	rBV4	563	441	0.02%	0.003%
83	13.513	3869	3879	3887	rBV4	6420	11243	0.62%	0.089%
84	13.850	3982	3984	3987	rVB2	487	257	0.01%	0.002%




Sum of corrected areas: 12656674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027195.D
Acq On : 03 Aug 2022 16:37
Operator : SY/MD
Sample : N4005-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

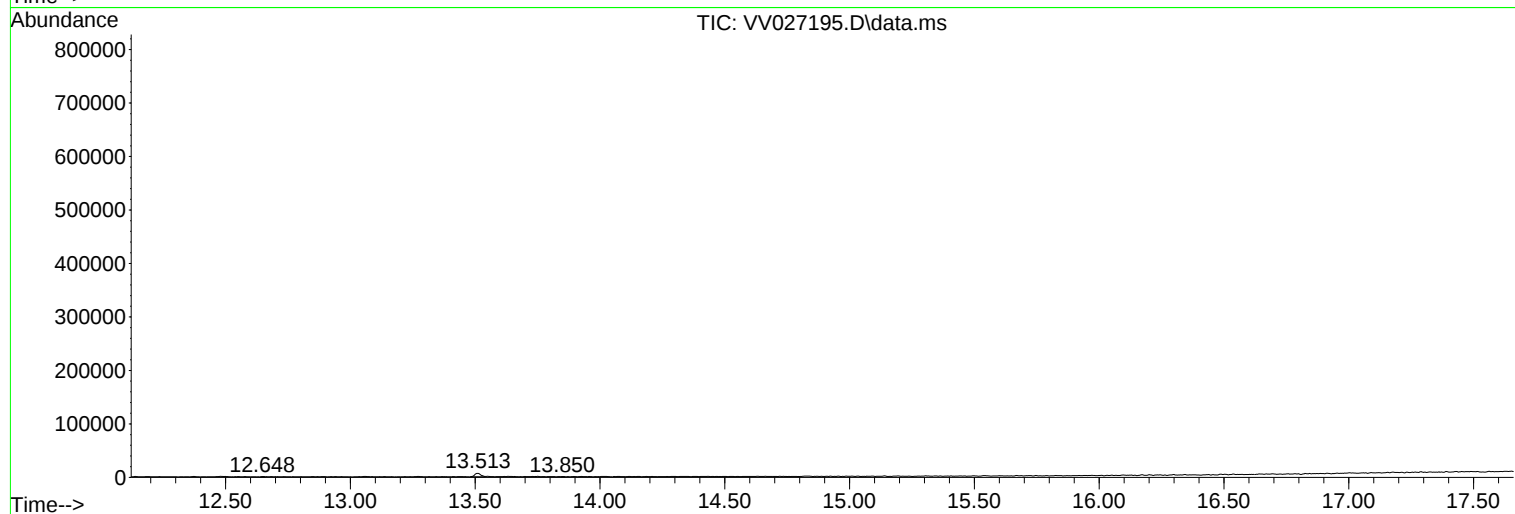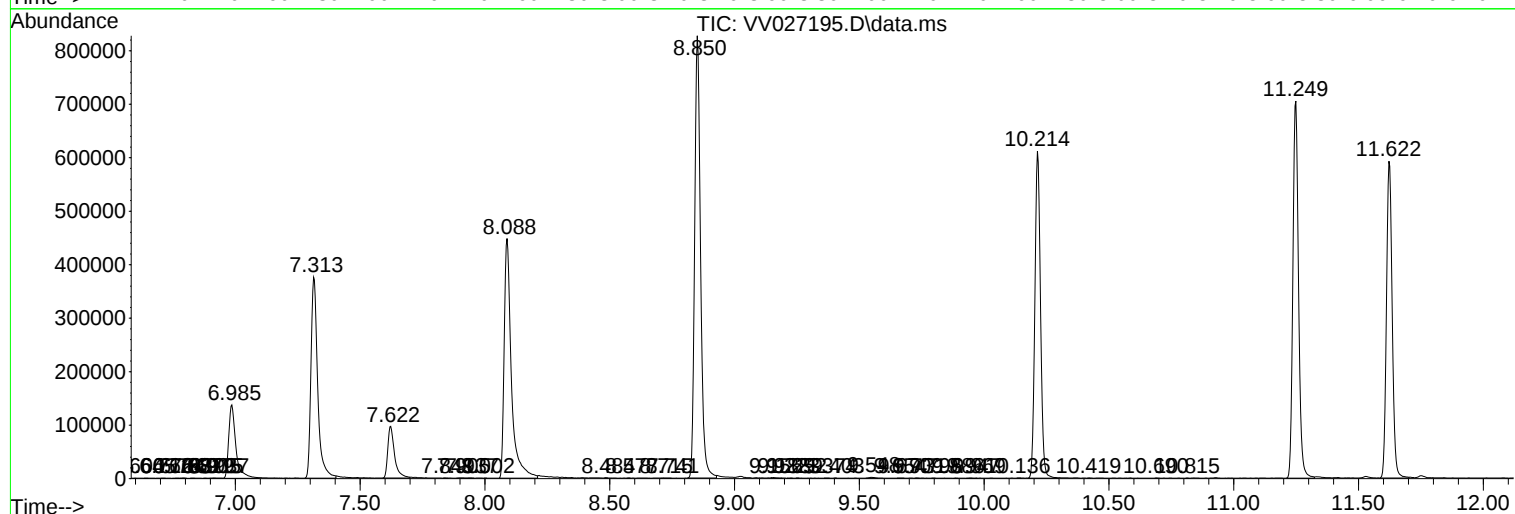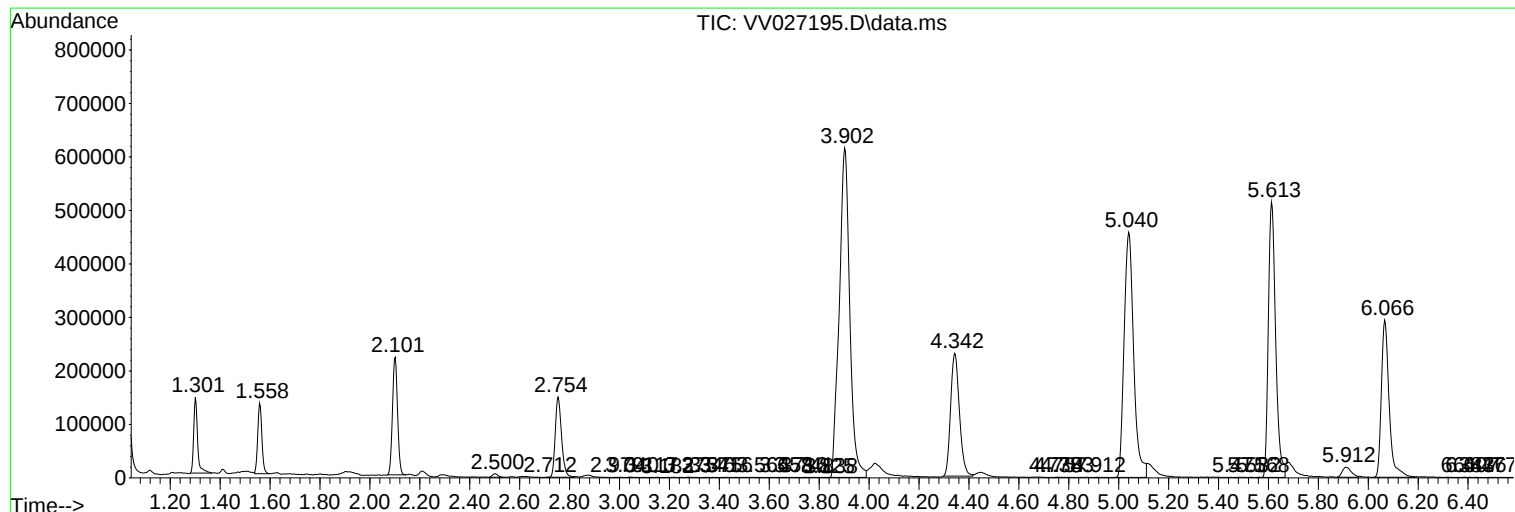

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027195.D
Acq On : 03 Aug 2022 16:37
Operator : SY/MD
Sample : N4005-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027195.D
Acq On : 03 Aug 2022 16:37
Operator : SY/MD
Sample : N4005-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc