

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027197.D
 Acq On : 03 Aug 2022 17:27
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

Signal : TIC: VV027197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	110	rBV2	1204790	1433427	65.39%	7.848%
2	1.561	154	162	175	rVB	280343	322905	14.73%	1.768%
3	2.101	319	330	347	rBV	586524	828563	37.80%	4.536%
4	2.214	357	365	383	rVB2	26967	53044	2.42%	0.290%
5	2.281	384	386	389	rBV2	796	456	0.02%	0.002%
6	2.355	406	409	412	rVB2	460	365	0.02%	0.002%
7	2.503	445	455	469	rVB	19968	33457	1.53%	0.183%
8	2.616	486	490	492	rBV2	638	452	0.02%	0.002%
9	2.757	524	534	553	rBV2	35464	64062	2.92%	0.351%
10	2.880	562	572	582	rBV4	901	2161	0.10%	0.012%
11	2.995	605	608	613	rVB2	376	355	0.02%	0.002%
12	3.031	616	619	622	rBV3	328	270	0.01%	0.001%
13	3.047	622	624	629	rVB2	633	391	0.02%	0.002%
14	3.076	629	633	635	rBV2	354	307	0.01%	0.002%
15	3.137	648	652	659	rVB3	459	652	0.03%	0.004%
16	3.198	667	671	673	rBV2	378	272	0.01%	0.001%
17	3.407	732	736	742	rVB2	286	345	0.02%	0.002%
18	3.539	775	777	780	rBV	609	296	0.01%	0.002%
19	3.625	799	804	807	rVB2	350	302	0.01%	0.002%
20	3.670	813	818	822	rBV	304	340	0.02%	0.002%
21	3.902	872	890	920	rBV3	212446	835659	38.12%	4.575%
22	4.236	991	994	997	rVB3	481	318	0.01%	0.002%
23	4.342	1010	1027	1050	rBV	364331	898800	41.00%	4.921%
24	4.625	1111	1115	1120	rVB4	415	322	0.01%	0.002%
25	4.728	1144	1147	1149	rBV3	441	284	0.01%	0.002%
26	4.863	1186	1189	1192	rBV2	427	332	0.02%	0.002%
27	5.043	1227	1245	1264	rBV2	864622	2192039	100.00%	12.001%
28	5.375	1346	1348	1351	rVB3	773	401	0.02%	0.002%
29	5.490	1381	1384	1391	rBV3	512	565	0.03%	0.003%
30	5.542	1395	1400	1402	rBV3	593	505	0.02%	0.003%
31	5.613	1410	1422	1439	rBV	645619	1295006	59.08%	7.090%
32	5.908	1502	1514	1528	rBV3	14671	31045	1.42%	0.170%
33	6.008	1543	1545	1548	rVB2	442	260	0.01%	0.001%
34	6.066	1549	1563	1603	rBV	489140	1042216	47.55%	5.706%
35	6.317	1639	1641	1644	rVB3	544	272	0.01%	0.001%
36	6.391	1660	1664	1665	rBV2	342	261	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027197.D
 Acq On : 03 Aug 2022 17:27
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.436	1672	1678	1681	rVB3	298	304	0.01%	0.002%
38	6.465	1685	1687	1691	rVB3	461	340	0.02%	0.002%
39	6.558	1711	1716	1719	rBV3	248	261	0.01%	0.001%
40	6.744	1771	1774	1777	rBV2	446	319	0.01%	0.002%
41	6.982	1837	1848	1884	rBV	230290	447323	20.41%	2.449%
42	7.313	1938	1951	1989	rBV	963200	1726107	78.74%	9.450%
43	7.619	2035	2046	2075	rBV	164943	303902	13.86%	1.664%
44	7.792	2095	2100	2104	rBV6	779	801	0.04%	0.004%
45	7.883	2124	2128	2130	rBV3	438	327	0.01%	0.002%
46	7.947	2145	2148	2155	rVB3	553	648	0.03%	0.004%
47	7.979	2155	2158	2161	rBV2	1147	720	0.03%	0.004%
48	8.088	2180	2192	2239	rBV	559687	1090323	49.74%	5.969%
49	8.616	2353	2356	2357	rBV2	520	281	0.01%	0.002%
50	8.635	2360	2362	2366	rVB2	518	316	0.01%	0.002%
51	8.693	2378	2380	2384	rVB2	511	335	0.02%	0.002%
52	8.728	2389	2391	2396	rVB3	484	349	0.02%	0.002%
53	8.850	2416	2429	2458	rBV	1026199	1670090	76.19%	9.143%
54	9.169	2525	2528	2535	rVB4	766	717	0.03%	0.004%
55	9.201	2535	2538	2540	rBV2	679	331	0.02%	0.002%
56	9.259	2552	2556	2557	rBV3	725	479	0.02%	0.003%
57	9.339	2579	2581	2589	rVV3	791	722	0.03%	0.004%
58	9.397	2597	2599	2605	rVB	303	279	0.01%	0.002%
59	9.532	2636	2641	2646	rBV2	320	419	0.02%	0.002%
60	9.554	2646	2648	2656	rVB4	405	433	0.02%	0.002%
61	9.645	2672	2676	2679	rBV3	381	353	0.02%	0.002%
62	9.683	2682	2688	2690	rVV	598	565	0.03%	0.003%
63	9.702	2692	2694	2697	rVV2	450	266	0.01%	0.001%
64	9.725	2697	2701	2704	rVV2	353	328	0.01%	0.002%
65	9.741	2704	2706	2713	rVB2	337	303	0.01%	0.002%
66	9.908	2754	2758	2764	rVB2	452	493	0.02%	0.003%
67	9.940	2764	2768	2770	rBV2	377	294	0.01%	0.002%
68	10.001	2784	2787	2788	rBV	426	249	0.01%	0.001%
69	10.024	2791	2794	2797	rVB2	468	259	0.01%	0.001%
70	10.149	2831	2833	2841	rVB2	313	313	0.01%	0.002%
71	10.214	2841	2853	2880	rBV	736233	1159722	52.91%	6.349%
72	10.513	2943	2946	2950	rBV3	328	278	0.01%	0.002%
73	10.754	3019	3021	3026	rVV2	402	378	0.02%	0.002%
74	10.789	3030	3032	3038	rVV2	439	341	0.02%	0.002%
75	10.857	3046	3053	3058	rBV4	545	738	0.03%	0.004%
76	10.924	3072	3074	3080	rVB	388	279	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027197.D
 Acq On : 03 Aug 2022 17:27
 Operator : SY/MD
 Sample : N4003-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.149	3140	3144	3146	rBV2	537	363	0.02%	0.002%
78	11.249	3163	3175	3202	rBV	885836	1382160	63.05%	7.567%
79	11.439	3232	3234	3239	rBV4	550	365	0.02%	0.002%
80	11.622	3279	3291	3311	rBV	915953	1423320	64.93%	7.792%
81	11.908	3377	3380	3382	rBV2	449	264	0.01%	0.001%
82	11.963	3393	3397	3400	rVB	508	338	0.02%	0.002%
83	12.117	3442	3445	3450	rVB2	472	420	0.02%	0.002%
84	12.451	3545	3549	3551	rBV3	525	446	0.02%	0.002%
85	12.496	3560	3563	3565	rBV	449	267	0.01%	0.001%
86	12.587	3588	3591	3595	rBV	343	276	0.01%	0.002%
87	12.773	3646	3649	3654	rBV3	574	482	0.02%	0.003%
88	12.802	3654	3658	3660	rBV2	393	274	0.01%	0.002%
89	13.156	3765	3768	3771	rBV2	493	453	0.02%	0.002%
90	13.246	3793	3796	3797	rBV2	443	245	0.01%	0.001%
91	13.413	3845	3848	3851	rBV2	473	329	0.02%	0.002%
92	13.516	3875	3880	3884	rBV3	580	773	0.04%	0.004%
93	13.664	3923	3926	3930	rBV2	353	376	0.02%	0.002%
94	13.747	3949	3952	3957	rBV	546	398	0.02%	0.002%
95	13.911	4001	4003	4008	rVB3	449	249	0.01%	0.001%
96	14.104	4059	4063	4065	rVB	558	342	0.02%	0.002%
97	14.313	4126	4128	4132	rBV3	595	391	0.02%	0.002%
98	14.676	4238	4241	4243	rBV3	671	402	0.02%	0.002%
99	15.120	4377	4379	4382	rBV3	642	333	0.02%	0.002%
100	15.374	4455	4458	4460	rBV3	745	588	0.03%	0.003%


Sum of corrected areas: 18265846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027197.D
Acq On : 03 Aug 2022 17:27
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

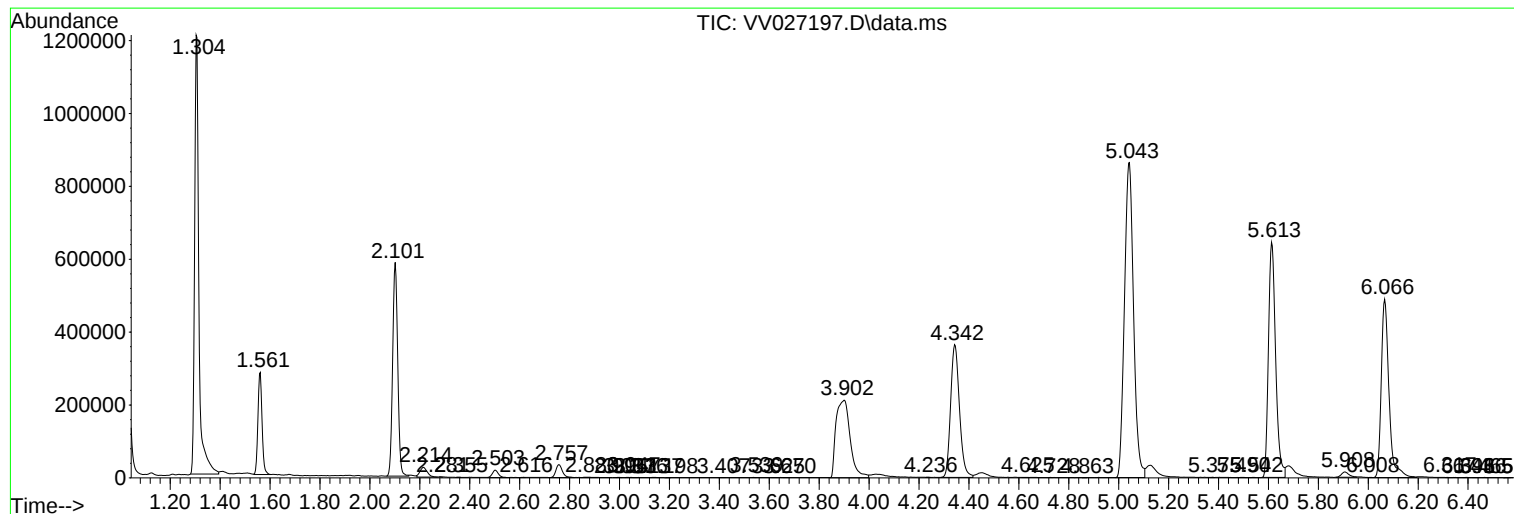

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027197.D
Acq On : 03 Aug 2022 17:27
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027197.D
Acq On : 03 Aug 2022 17:27
Operator : SY/MD
Sample : N4003-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------