

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V080322\
 Data File : VV027200.D
 Acq On : 03 Aug 2022 18:41
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	315883	352409	17.40%	2.006%
2	1.561	154	162	179	rVB	257915	303627	14.99%	1.729%
3	2.101	320	330	345	rBV	545168	767476	37.90%	4.370%
4	2.201	353	361	381	rVB3	18444	43368	2.14%	0.247%
5	2.291	383	389	401	rVB6	2460	4775	0.24%	0.027%
6	2.394	417	421	423	rBV2	437	326	0.02%	0.002%
7	2.503	444	455	466	rVB2	14284	23208	1.15%	0.132%
8	2.619	479	491	496	rBV4	2115	4563	0.23%	0.026%
9	2.696	511	515	516	rBV	485	312	0.02%	0.002%
10	2.754	520	533	554	rVV	746486	1268295	62.63%	7.221%
11	2.854	558	564	584	rVB3	12532	31402	1.55%	0.179%
12	3.310	700	706	710	rBV3	226	298	0.01%	0.002%
13	3.400	728	734	737	rVB	357	326	0.02%	0.002%
14	3.513	765	769	777	rVV3	375	567	0.03%	0.003%
15	3.596	792	795	800	rVB3	339	324	0.02%	0.002%
16	3.674	813	819	823	rBV2	488	675	0.03%	0.004%
17	3.905	871	891	916	rBV3	421500	1358398	67.08%	7.734%
18	4.342	1010	1027	1048	rBV	336569	826856	40.83%	4.708%
19	4.584	1099	1102	1106	rBV3	380	300	0.01%	0.002%
20	4.725	1142	1146	1151	rVB5	444	318	0.02%	0.002%
21	4.783	1159	1164	1168	rBV	477	459	0.02%	0.003%
22	4.931	1206	1210	1213	rBV2	404	313	0.02%	0.002%
23	5.043	1225	1245	1264	rBV2	793344	2025050	100.00%	11.530%
24	5.397	1351	1355	1357	rVV3	589	386	0.02%	0.002%
25	5.413	1358	1360	1363	rVB2	784	367	0.02%	0.002%
26	5.558	1402	1405	1408	rVB3	469	298	0.01%	0.002%
27	5.612	1408	1422	1457	rBV	567758	1207712	59.64%	6.876%
28	5.908	1503	1514	1529	rBV3	14182	32270	1.59%	0.184%
29	6.066	1549	1563	1594	rBV	449173	944481	46.64%	5.377%
30	6.413	1667	1671	1676	rBV2	500	413	0.02%	0.002%
31	6.477	1686	1691	1695	rBV3	378	442	0.02%	0.003%
32	6.513	1700	1702	1708	rVB	499	379	0.02%	0.002%
33	6.587	1723	1725	1731	rVB3	339	296	0.01%	0.002%
34	6.654	1743	1746	1750	rBV2	345	323	0.02%	0.002%
35	6.722	1763	1767	1772	rVB2	307	360	0.02%	0.002%
36	6.754	1772	1777	1783	rVB2	546	560	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027200.D
 Acq On : 03 Aug 2022 18:41
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.911	1820	1826	1831	rVB2	328	364	0.02%	0.002%
38	6.985	1836	1849	1884	rBV	208835	400472	19.78%	2.280%
39	7.220	1918	1922	1926	rVB2	722	539	0.03%	0.003%
40	7.246	1926	1930	1931	rBV2	537	413	0.02%	0.002%
41	7.313	1938	1951	1981	rBV	863553	1555812	76.83%	8.858%
42	7.619	2035	2046	2070	rBV	150434	272947	13.48%	1.554%
43	7.905	2132	2135	2141	rBV4	353	366	0.02%	0.002%
44	7.982	2155	2159	2163	rVB5	358	307	0.02%	0.002%
45	8.011	2163	2168	2170	rBV2	529	407	0.02%	0.002%
46	8.088	2182	2192	2223	rBV	507802	974540	48.12%	5.549%
47	8.850	2417	2429	2462	rBV	902589	1490824	73.62%	8.488%
48	9.075	2495	2499	2504	rVB3	461	328	0.02%	0.002%
49	9.291	2562	2566	2569	rBV2	462	435	0.02%	0.002%
50	9.445	2610	2614	2618	rBV2	263	295	0.01%	0.002%
51	9.487	2624	2627	2632	rVB3	461	376	0.02%	0.002%
52	9.757	2706	2711	2714	rVV2	344	358	0.02%	0.002%
53	9.805	2719	2726	2732	rBV3	447	567	0.03%	0.003%
54	10.027	2789	2795	2798	rVB3	279	333	0.02%	0.002%
55	10.082	2808	2812	2816	rBV3	401	318	0.02%	0.002%
56	10.127	2823	2826	2830	rBV2	312	303	0.01%	0.002%
57	10.214	2839	2853	2883	rBV	688805	1071346	52.90%	6.100%
58	10.400	2905	2911	2914	rBV3	445	458	0.02%	0.003%
59	10.471	2930	2933	2936	rBV2	498	377	0.02%	0.002%
60	10.587	2965	2969	2974	rVB2	331	313	0.02%	0.002%
61	10.667	2987	2994	2997	rVV2	515	546	0.03%	0.003%
62	10.747	3010	3019	3023	rBV3	548	826	0.04%	0.005%
63	10.850	3048	3051	3054	rVB3	1033	632	0.03%	0.004%
64	10.927	3070	3075	3078	rVB2	353	408	0.02%	0.002%
65	10.960	3078	3085	3087	rBV	368	363	0.02%	0.002%
66	11.181	3150	3154	3158	rBV3	371	378	0.02%	0.002%
67	11.249	3163	3175	3200	rBV	780357	1214416	59.97%	6.914%
68	11.532	3256	3263	3270	rBV5	1545	2186	0.11%	0.012%
69	11.622	3279	3291	3313	rBV	822806	1304017	64.39%	7.424%
70	11.808	3347	3349	3353	rVB2	673	451	0.02%	0.003%
71	11.831	3353	3356	3358	rBV2	674	393	0.02%	0.002%
72	12.117	3439	3445	3455	rVB6	1682	2633	0.13%	0.015%
73	12.201	3466	3471	3473	rBV2	353	324	0.02%	0.002%
74	12.365	3515	3522	3532	rBV4	6052	8944	0.44%	0.051%
75	12.413	3532	3537	3544	rVB6	1625	2097	0.10%	0.012%
76	12.468	3547	3554	3560	rBV6	2849	3504	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027200.D
 Acq On : 03 Aug 2022 18:41
 Operator : SY/MD
 Sample : N4005-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY157DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.516	3566	3569	3570	rBV2	1382	842	0.04%	0.005%
78	12.728	3629	3635	3638	rBV5	989	897	0.04%	0.005%
79	12.847	3669	3672	3677	rBV2	441	488	0.02%	0.003%
80	12.885	3677	3684	3692	rVB5	3033	4671	0.23%	0.027%
81	12.950	3693	3704	3710	rBV8	4417	7105	0.35%	0.040%
82	13.056	3729	3737	3752	rVB3	8496	13525	0.67%	0.077%
83	13.162	3766	3770	3773	rBV2	426	301	0.01%	0.002%
84	13.197	3778	3781	3783	rVV3	746	522	0.03%	0.003%
85	13.217	3783	3787	3794	rVV6	1011	1324	0.07%	0.008%
86	13.275	3802	3805	3809	rVV3	775	631	0.03%	0.004%
87	13.435	3848	3855	3859	rBV4	544	835	0.04%	0.005%
88	13.503	3867	3876	3884	rBV8	3091	6368	0.31%	0.036%
89	13.603	3902	3907	3911	rBV4	821	932	0.05%	0.005%
90	13.670	3922	3928	3929	rBV3	1800	1598	0.08%	0.009%
91	13.766	3952	3958	3961	rBV4	1254	1424	0.07%	0.008%
92	14.098	4058	4061	4069	rVB7	1060	1227	0.06%	0.007%
93	14.146	4072	4076	4077	rBV3	413	304	0.02%	0.002%
94	14.683	4240	4243	4248	rBV2	564	592	0.03%	0.003%
95	14.811	4278	4283	4284	rBV3	959	630	0.03%	0.004%
96	14.828	4285	4288	4289	rVV2	898	530	0.03%	0.003%
97	15.252	4417	4420	4423	rBV2	646	374	0.02%	0.002%
98	15.413	4467	4470	4473	rBV3	1153	755	0.04%	0.004%
99	15.519	4499	4503	4504	rBV	563	417	0.02%	0.002%
100	16.091	4679	4681	4685	rBV4	1050	798	0.04%	0.005%




Sum of corrected areas: 17563938

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027200.D
Acq On : 03 Aug 2022 18:41
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

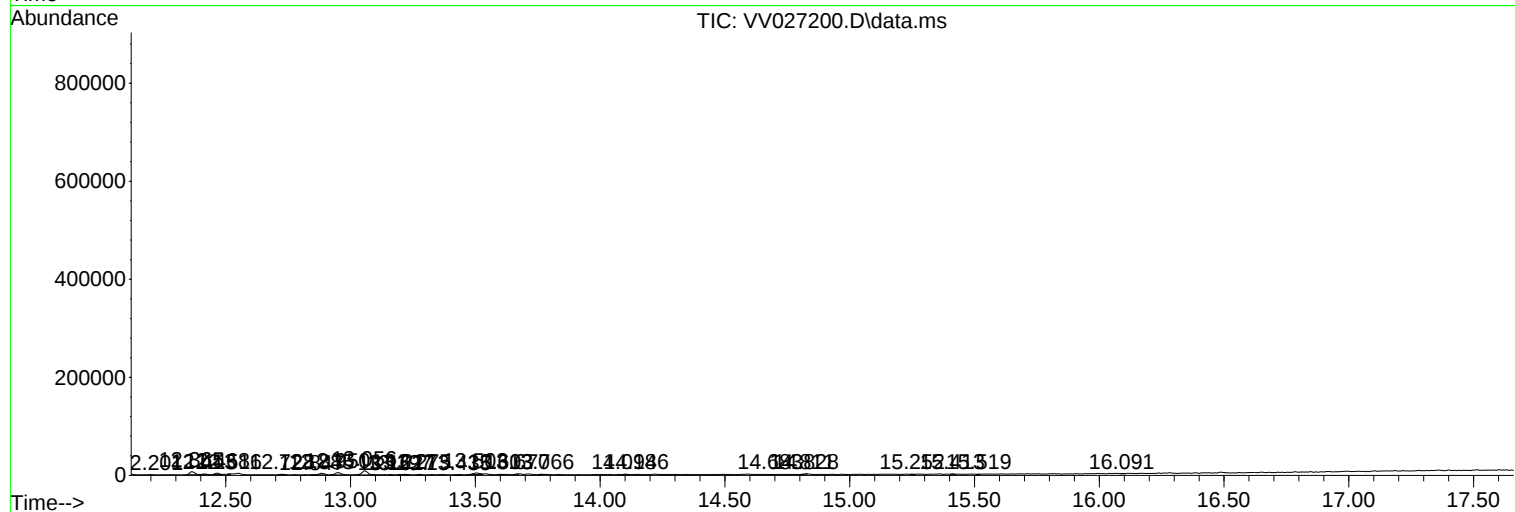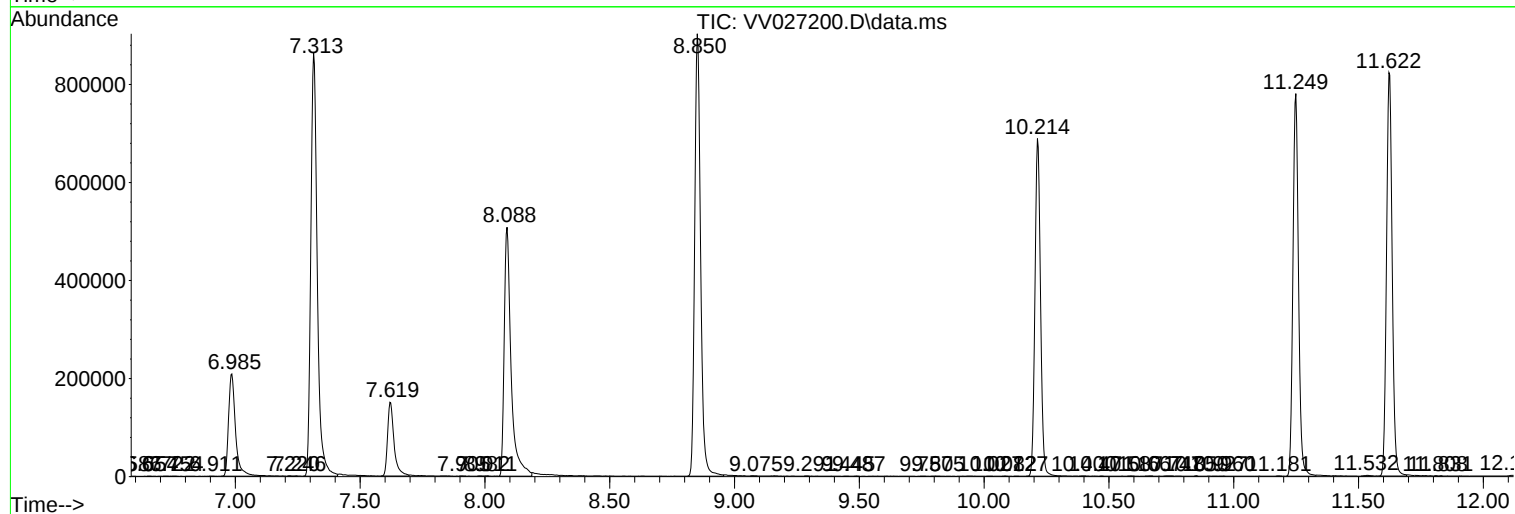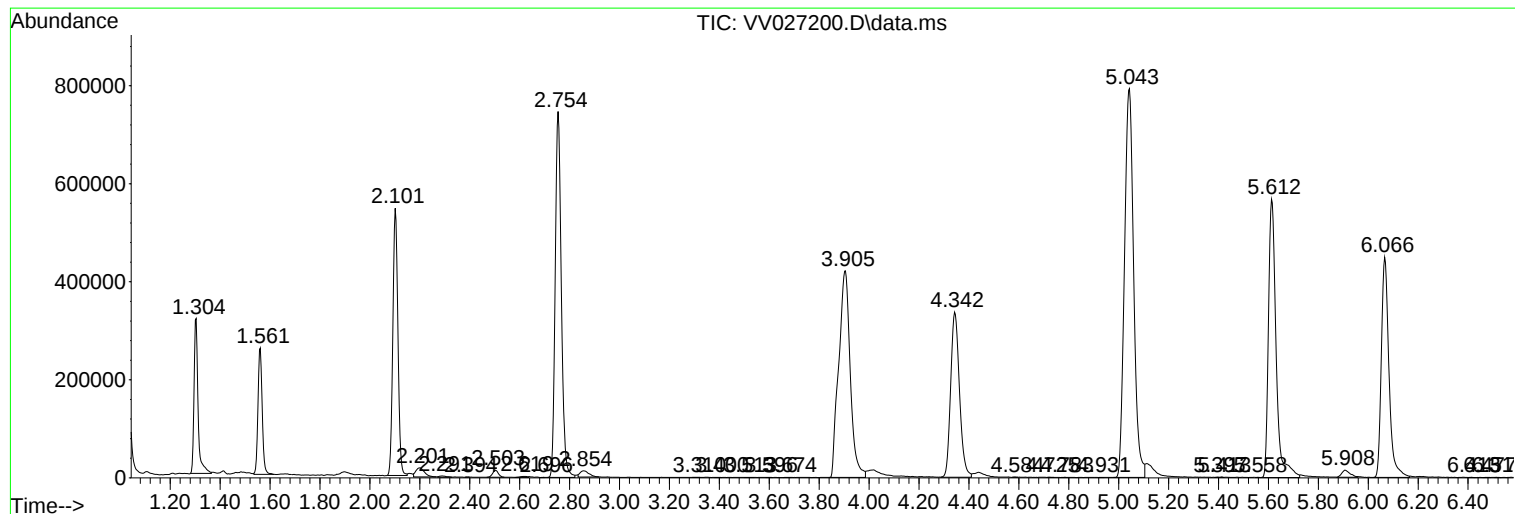

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027200.D
Acq On : 03 Aug 2022 18:41
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027200.D
Acq On : 03 Aug 2022 18:41
Operator : SY/MD
Sample : N4005-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY157DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc