

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027201.D
 Acq On : 03 Aug 2022 19:06
 Operator : SY/MD
 Sample : N4005-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	101	rBV2	352526	401345	6.53%	1.801%
2	1.561	154	162	173	rBV	249244	286292	4.66%	1.285%
3	2.101	320	330	346	rBV	533785	749502	12.19%	3.363%
4	2.191	353	358	379	rVB2	20597	42093	0.68%	0.189%
5	2.285	382	387	400	rVB4	3378	5822	0.09%	0.026%
6	2.503	441	455	466	rBV9	2474	5283	0.09%	0.024%
7	2.571	466	476	485	rBV6	4320	7226	0.12%	0.032%
8	2.638	493	497	498	rBV2	524	309	0.01%	0.001%
9	2.683	508	511	514	rBV2	445	337	0.01%	0.002%
10	2.754	519	533	553	rBV	642669	1097767	17.86%	4.926%
11	2.850	556	563	587	rVB	15446	38041	0.62%	0.171%
12	3.175	658	664	669	rBV3	333	418	0.01%	0.002%
13	3.288	695	699	707	rVB3	645	826	0.01%	0.004%
14	3.413	735	738	739	rBV	370	246	0.00%	0.001%
15	3.616	797	801	804	rBV2	318	246	0.00%	0.001%
16	3.821	862	865	871	rBV2	364	399	0.01%	0.002%
17	3.902	871	890	912	rBV2	2483656	6146343	100.00%	27.582%
18	4.342	1011	1027	1048	rBV	332456	813119	13.23%	3.649%
19	4.532	1084	1086	1089	rBV3	546	344	0.01%	0.002%
20	4.674	1123	1130	1132	rBV5	1492	2052	0.03%	0.009%
21	4.735	1143	1149	1151	rBV3	596	495	0.01%	0.002%
22	4.757	1154	1156	1160	rVV3	483	291	0.00%	0.001%
23	4.780	1160	1163	1167	rVB2	630	407	0.01%	0.002%
24	4.928	1206	1209	1211	rBV2	373	286	0.00%	0.001%
25	5.043	1226	1245	1260	rBV2	778719	2012310	32.74%	9.030%
26	5.362	1340	1344	1355	rBV6	1882	3604	0.06%	0.016%
27	5.400	1355	1356	1360	rVB2	945	307	0.00%	0.001%
28	5.558	1401	1405	1409	rBV4	550	464	0.01%	0.002%
29	5.612	1410	1422	1460	rBV	560745	1198459	19.50%	5.378%
30	5.915	1503	1516	1541	rVB3	51817	122807	2.00%	0.551%
31	6.066	1549	1563	1596	rBV	443188	936005	15.23%	4.200%
32	6.300	1634	1636	1639	rBV2	501	245	0.00%	0.001%
33	6.442	1673	1680	1682	rBV4	384	384	0.01%	0.002%
34	6.471	1686	1689	1692	rVV3	514	374	0.01%	0.002%
35	6.587	1720	1725	1727	rBV	469	344	0.01%	0.002%
36	6.802	1785	1792	1796	rBV4	362	495	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027201.D
 Acq On : 03 Aug 2022 19:06
 Operator : SY/MD
 Sample : N4005-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.985	1835	1849	1871	rBV	203402	388154	6.32%	1.742%
38	7.243	1927	1929	1933	rVB2	417	253	0.00%	0.001%
39	7.313	1939	1951	1992	rBV	844985	1547558	25.18%	6.945%
40	7.619	2036	2046	2076	rBV	146230	270504	4.40%	1.214%
41	7.818	2105	2108	2112	rVB2	446	325	0.01%	0.001%
42	7.979	2152	2158	2162	rBV5	920	799	0.01%	0.004%
43	8.088	2182	2192	2226	rBV	485007	939061	15.28%	4.214%
44	8.326	2264	2266	2271	rVB4	756	587	0.01%	0.003%
45	8.471	2308	2311	2315	rBV4	380	340	0.01%	0.002%
46	8.564	2336	2340	2342	rBV4	462	274	0.00%	0.001%
47	8.616	2352	2356	2360	rBV3	591	491	0.01%	0.002%
48	8.638	2360	2363	2368	rVB3	370	361	0.01%	0.002%
49	8.706	2380	2384	2388	rVB3	382	354	0.01%	0.002%
50	8.850	2417	2429	2458	rBV	895659	1468889	23.90%	6.592%
51	9.017	2473	2481	2495	rVB2	12432	20605	0.34%	0.092%
52	9.149	2514	2522	2535	rVB4	3898	6979	0.11%	0.031%
53	9.259	2552	2556	2558	rBV2	498	300	0.00%	0.001%
54	9.316	2572	2574	2578	rBV2	580	384	0.01%	0.002%
55	9.464	2617	2620	2624	rBV2	390	270	0.00%	0.001%
56	9.551	2635	2647	2658	rBV2	9197	15376	0.25%	0.069%
57	9.664	2679	2682	2687	rVB2	340	277	0.00%	0.001%
58	9.702	2690	2694	2701	rVV2	302	400	0.01%	0.002%
59	9.744	2704	2707	2715	rBV2	284	376	0.01%	0.002%
60	9.918	2755	2761	2763	rBV2	479	439	0.01%	0.002%
61	9.988	2782	2783	2788	rVB	386	258	0.00%	0.001%
62	10.021	2788	2793	2798	rBV3	328	380	0.01%	0.002%
63	10.120	2820	2824	2826	rBV2	350	256	0.00%	0.001%
64	10.214	2841	2853	2875	rBV	673763	1070733	17.42%	4.805%
65	10.387	2905	2907	2911	rVB4	563	369	0.01%	0.002%
66	10.606	2970	2975	2977	rBV2	405	375	0.01%	0.002%
67	10.683	2997	2999	3002	rVB	526	283	0.00%	0.001%
68	10.741	3010	3017	3019	rBV2	792	879	0.01%	0.004%
69	10.921	3065	3073	3081	rBV4	4111	6346	0.10%	0.028%
70	11.188	3149	3156	3162	rVB6	1201	1415	0.02%	0.006%
71	11.249	3162	3175	3197	rBV	785965	1214570	19.76%	5.450%
72	11.529	3253	3262	3278	rBV3	13065	23513	0.38%	0.106%
73	11.622	3278	3291	3312	rBV	845412	1313244	21.37%	5.893%
74	11.747	3322	3330	3345	rVB	17461	28606	0.47%	0.128%
75	11.879	3369	3371	3376	rVB2	464	250	0.00%	0.001%
76	11.921	3381	3384	3386	rBV2	420	261	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027201.D
 Acq On : 03 Aug 2022 19:06
 Operator : SY/MD
 Sample : N4005-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.021	3412	3415	3420	rVB4	668	611	0.01%	0.003%
78	12.117	3442	3445	3446	rBV2	568	313	0.01%	0.001%
79	12.294	3497	3500	3502	rBV	339	248	0.00%	0.001%
80	12.365	3516	3522	3532	rVB4	2493	3649	0.06%	0.016%
81	12.406	3532	3535	3538	rBV2	634	511	0.01%	0.002%
82	12.474	3546	3556	3565	rBV3	4629	8284	0.13%	0.037%
83	12.545	3575	3578	3580	rBV2	805	391	0.01%	0.002%
84	12.657	3611	3613	3617	rBV3	336	278	0.00%	0.001%
85	12.889	3678	3685	3689	rVB3	1389	1373	0.02%	0.006%
86	12.956	3700	3706	3713	rBV5	1394	1772	0.03%	0.008%
87	13.056	3730	3737	3747	rVV5	2150	3739	0.06%	0.017%
88	13.207	3779	3784	3786	rBV2	530	527	0.01%	0.002%
89	13.268	3799	3803	3806	rBV3	394	403	0.01%	0.002%
90	13.438	3853	3856	3861	rVB2	479	403	0.01%	0.002%
91	13.506	3868	3877	3892	rBV	28390	44201	0.72%	0.198%
92	13.606	3905	3908	3909	rBV2	776	415	0.01%	0.002%
93	13.625	3909	3914	3925	rVV2	4507	6622	0.11%	0.030%
94	13.686	3929	3933	3935	rBV2	714	487	0.01%	0.002%
95	13.828	3975	3977	3985	rVB4	565	504	0.01%	0.002%
96	14.332	4130	4134	4138	rBV3	451	518	0.01%	0.002%
97	14.824	4277	4287	4295	rBV6	3131	5885	0.10%	0.026%
98	15.104	4371	4374	4378	rBV4	889	736	0.01%	0.003%
99	15.364	4453	4455	4458	rBV3	628	384	0.01%	0.002%
100	15.734	4565	4570	4573	rBV4	1080	1124	0.02%	0.005%




Sum of corrected areas: 22283759

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027201.D
Acq On : 03 Aug 2022 19:06
Operator : SY/MD
Sample : N4005-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

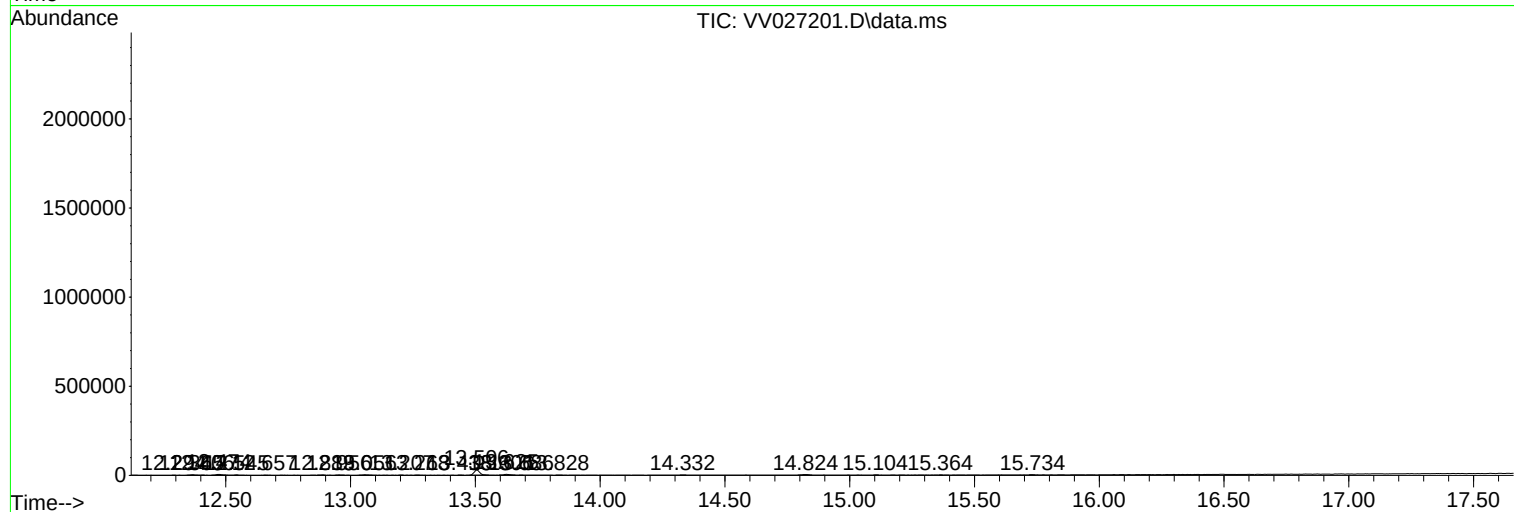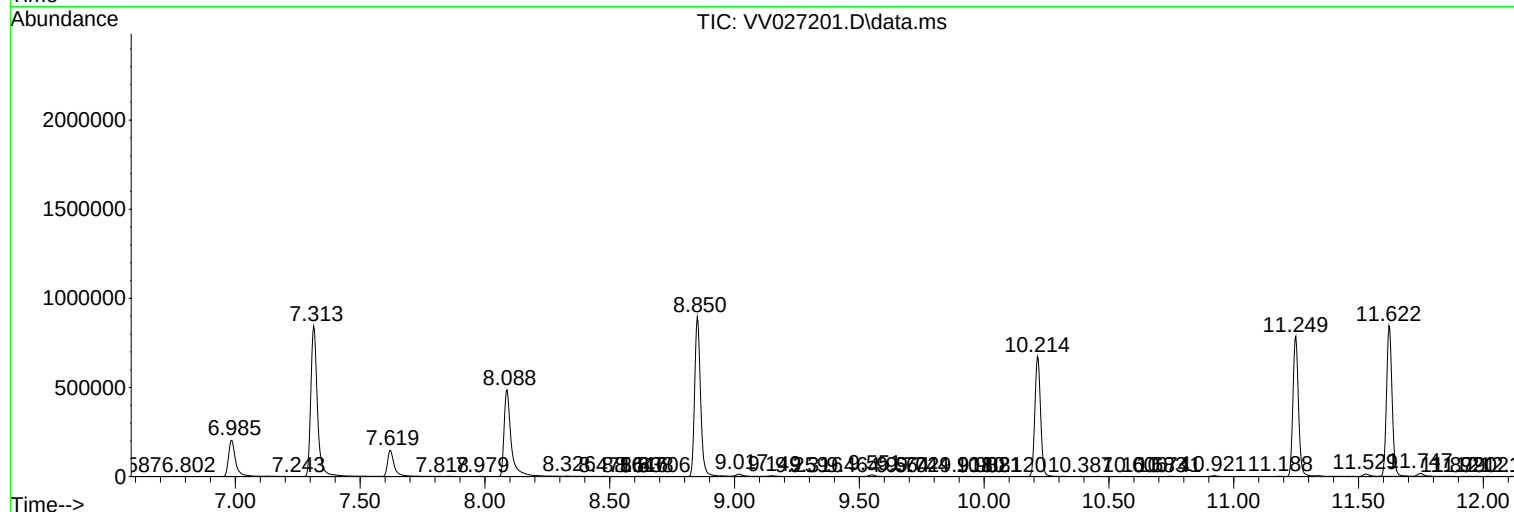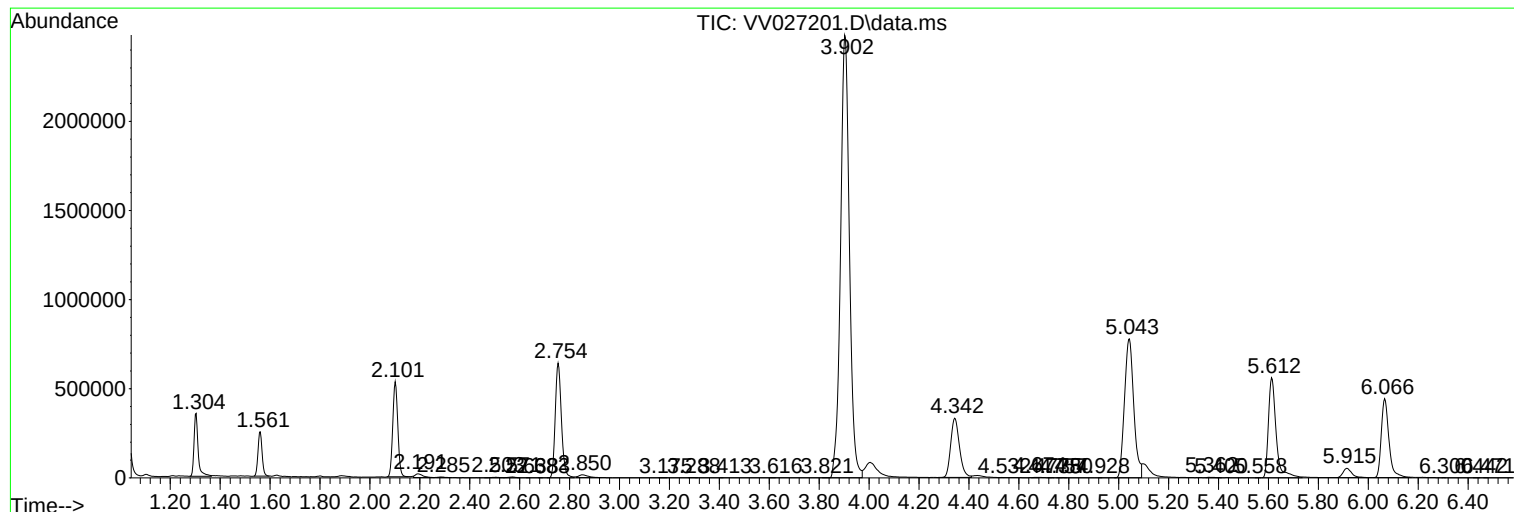

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027201.D
Acq On : 03 Aug 2022 19:06
Operator : SY/MD
Sample : N4005-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027201.D
Acq On : 03 Aug 2022 19:06
Operator : SY/MD
Sample : N4005-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc