

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027202.D
 Acq On : 03 Aug 2022 19:30
 Operator : SY/MD
 Sample : VIBLK270
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	104	rBV	299426	336727	16.33%	2.247%
2	1.561	154	162	176	rVB	256192	295298	14.32%	1.971%
3	2.101	319	330	346	rBV	524639	745357	36.14%	4.975%
4	2.503	444	455	467	rVB2	7421	11840	0.57%	0.079%
5	2.622	481	492	497	rBV6	2637	5017	0.24%	0.033%
6	2.760	527	535	545	rBV4	4502	7304	0.35%	0.049%
7	2.934	585	589	592	rBV2	295	256	0.01%	0.002%
8	3.114	643	645	650	rVB2	328	224	0.01%	0.001%
9	3.278	689	696	702	rBV3	390	563	0.03%	0.004%
10	3.320	706	709	714	rBV3	287	272	0.01%	0.002%
11	3.455	748	751	755	rBV2	381	379	0.02%	0.003%
12	3.506	763	767	769	rBV	288	238	0.01%	0.002%
13	3.571	783	787	793	rVB2	318	292	0.01%	0.002%
14	3.690	820	824	827	rBV2	273	274	0.01%	0.002%
15	3.760	843	846	849	rBV	332	305	0.01%	0.002%
16	3.812	857	862	865	rBV	312	268	0.01%	0.002%
17	3.879	872	883	916	rBV2	166410	550665	26.70%	3.675%
18	4.207	982	985	987	rBV3	475	291	0.01%	0.002%
19	4.342	1010	1027	1049	rBV	332360	821921	39.85%	5.486%
20	4.539	1086	1088	1090	rVB2	777	267	0.01%	0.002%
21	4.596	1104	1106	1109	rVB2	532	238	0.01%	0.002%
22	4.850	1183	1185	1189	rVB2	408	255	0.01%	0.002%
23	4.905	1197	1202	1206	rBV3	326	258	0.01%	0.002%
24	4.976	1220	1224	1227	rBV3	295	274	0.01%	0.002%
25	5.040	1227	1244	1290	rBV2	782121	2062342	100.00%	13.764%
26	5.307	1325	1327	1328	rBV	646	225	0.01%	0.002%
27	5.342	1335	1338	1344	rBV5	382	320	0.02%	0.002%
28	5.461	1372	1375	1378	rBV2	380	259	0.01%	0.002%
29	5.487	1379	1383	1385	rBV3	314	247	0.01%	0.002%
30	5.526	1392	1395	1401	rVB3	355	353	0.02%	0.002%
31	5.571	1405	1409	1410	rBV	510	358	0.02%	0.002%
32	5.612	1410	1422	1438	rBV	545583	1108827	53.77%	7.401%
33	5.905	1502	1513	1529	rBV3	14888	31853	1.54%	0.213%
34	6.066	1550	1563	1595	rBV	445657	939011	45.53%	6.267%
35	6.323	1641	1643	1648	rVB2	538	360	0.02%	0.002%
36	6.416	1670	1672	1677	rVB2	363	243	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027202.D
 Acq On : 03 Aug 2022 19:30
 Operator : SY/MD
 Sample : VIBLK270
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.477	1684	1691	1695	rBV2	445	517	0.03%	0.003%
38	6.538	1708	1710	1716	rVB	586	360	0.02%	0.002%
39	6.574	1716	1721	1725	rBV3	540	416	0.02%	0.003%
40	6.593	1725	1727	1735	rVB3	367	369	0.02%	0.002%
41	6.638	1735	1741	1746	rBV4	464	569	0.03%	0.004%
42	6.683	1751	1755	1757	rBV2	363	268	0.01%	0.002%
43	6.741	1768	1773	1776	rBV	252	221	0.01%	0.001%
44	6.985	1837	1849	1883	rBV	202653	391875	19.00%	2.615%
45	7.172	1904	1907	1909	rBV	366	281	0.01%	0.002%
46	7.201	1914	1916	1921	rVV3	432	378	0.02%	0.003%
47	7.313	1939	1951	1983	rBV	830551	1509061	73.17%	10.072%
48	7.571	2030	2031	2036	rVB3	450	273	0.01%	0.002%
49	7.619	2036	2046	2071	rBV	145407	266125	12.90%	1.776%
50	7.834	2111	2113	2118	rVB3	900	673	0.03%	0.004%
51	7.866	2120	2123	2125	rVV	563	280	0.01%	0.002%
52	7.947	2146	2148	2152	rVB2	532	243	0.01%	0.002%
53	8.088	2182	2192	2232	rBV	484184	971082	47.09%	6.481%
54	8.362	2273	2277	2278	rBV2	656	462	0.02%	0.003%
55	8.419	2285	2295	2314	rVB6	4319	8990	0.44%	0.060%
56	8.609	2352	2354	2360	rBV3	313	289	0.01%	0.002%
57	8.731	2388	2392	2397	rBV4	442	443	0.02%	0.003%
58	8.763	2400	2402	2405	rVB3	484	273	0.01%	0.002%
59	8.789	2405	2410	2413	rBV2	291	309	0.01%	0.002%
60	8.850	2418	2429	2458	rBV	867604	1438074	69.73%	9.598%
61	9.172	2523	2529	2531	rBV	533	403	0.02%	0.003%
62	9.345	2581	2583	2589	rVB	326	257	0.01%	0.002%
63	9.410	2599	2603	2605	rBV2	390	289	0.01%	0.002%
64	9.423	2605	2607	2611	rVV2	310	238	0.01%	0.002%
65	9.683	2685	2688	2695	rVB2	528	494	0.02%	0.003%
66	9.757	2707	2711	2714	rBV2	356	316	0.02%	0.002%
67	9.863	2742	2744	2750	rVB	261	228	0.01%	0.002%
68	10.098	2815	2817	2823	rVB3	293	230	0.01%	0.002%
69	10.214	2841	2853	2878	rBV	657916	1051092	50.97%	7.015%
70	10.365	2898	2900	2904	rBV3	425	251	0.01%	0.002%
71	10.406	2909	2913	2917	rBV3	307	382	0.02%	0.003%
72	10.853	3046	3052	3056	rBV4	637	647	0.03%	0.004%
73	10.972	3085	3089	3091	rBV3	264	233	0.01%	0.002%
74	10.985	3091	3093	3096	rVB	541	275	0.01%	0.002%
75	11.005	3096	3099	3102	rBV3	383	293	0.01%	0.002%
76	11.249	3164	3175	3200	rBV	752339	1149872	55.76%	7.674%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
 Data File : VV027202.D
 Acq On : 03 Aug 2022 19:30
 Operator : SY/MD
 Sample : VIBLK270
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.480	3243	3247	3250	rBV3	417	338	0.02%	0.002%
78	11.622	3279	3291	3312	rBV	788212	1252749	60.74%	8.361%
79	11.889	3371	3374	3378	rBV2	447	281	0.01%	0.002%
80	11.985	3402	3404	3408	rVB3	508	315	0.02%	0.002%
81	12.017	3411	3414	3419	rBV2	375	339	0.02%	0.002%
82	12.133	3447	3450	3455	rBV2	296	290	0.01%	0.002%
83	12.525	3569	3572	3576	rBV3	251	222	0.01%	0.001%
84	12.924	3694	3696	3700	rVB2	402	226	0.01%	0.002%
85	13.030	3725	3729	3731	rBV2	299	229	0.01%	0.002%
86	13.111	3751	3754	3758	rBV2	248	221	0.01%	0.001%
87	13.181	3774	3776	3780	rBV2	484	399	0.02%	0.003%
88	13.287	3805	3809	3811	rBV2	458	329	0.02%	0.002%
89	13.509	3870	3878	3883	rBV4	1639	2134	0.10%	0.014%
90	13.638	3916	3918	3922	rVB2	655	400	0.02%	0.003%
91	13.840	3978	3981	3983	rBV2	546	368	0.02%	0.002%
92	13.892	3994	3997	4001	rBV2	511	345	0.02%	0.002%
93	14.345	4136	4138	4142	rBV4	521	391	0.02%	0.003%
94	14.590	4212	4214	4218	rVB3	598	401	0.02%	0.003%
95	14.612	4218	4221	4223	rBV2	388	241	0.01%	0.002%
96	14.628	4224	4226	4230	rVV2	537	319	0.02%	0.002%
97	14.683	4240	4243	4245	rBV2	461	289	0.01%	0.002%
98	15.104	4370	4374	4375	rBV2	799	486	0.02%	0.003%
99	15.593	4523	4526	4528	rBV4	911	510	0.02%	0.003%
100	16.017	4656	4658	4661	rBV3	954	754	0.04%	0.005%




Sum of corrected areas: 14983088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027202.D
Acq On : 03 Aug 2022 19:30
Operator : SY/MD
Sample : VIBLK270
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

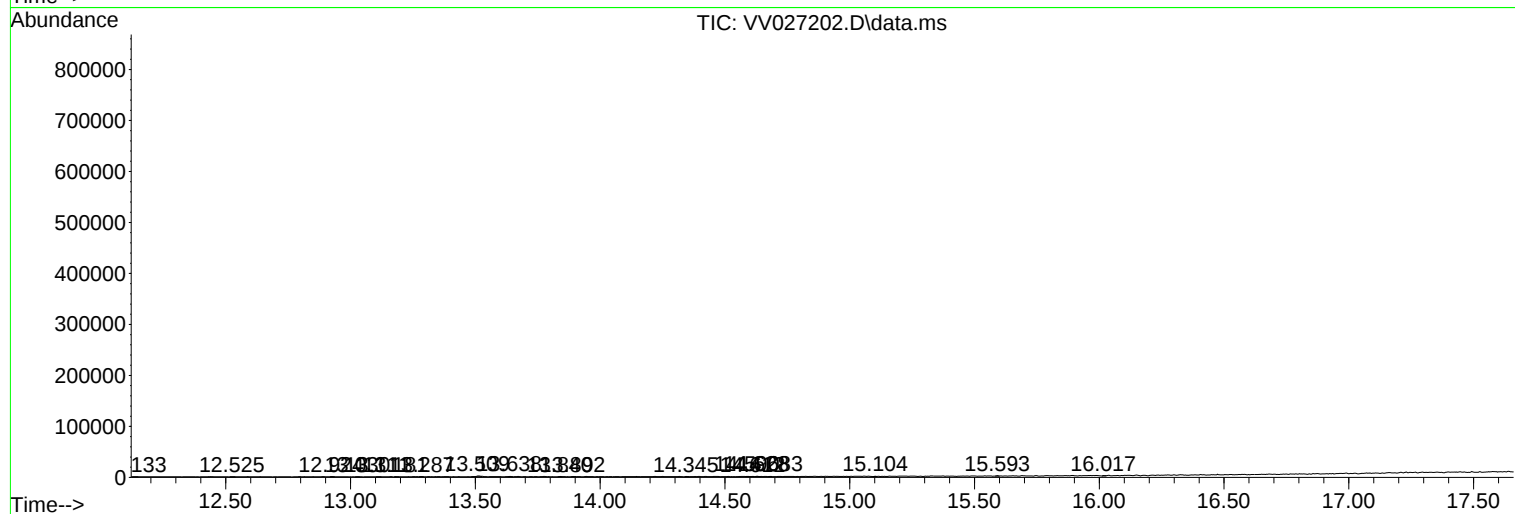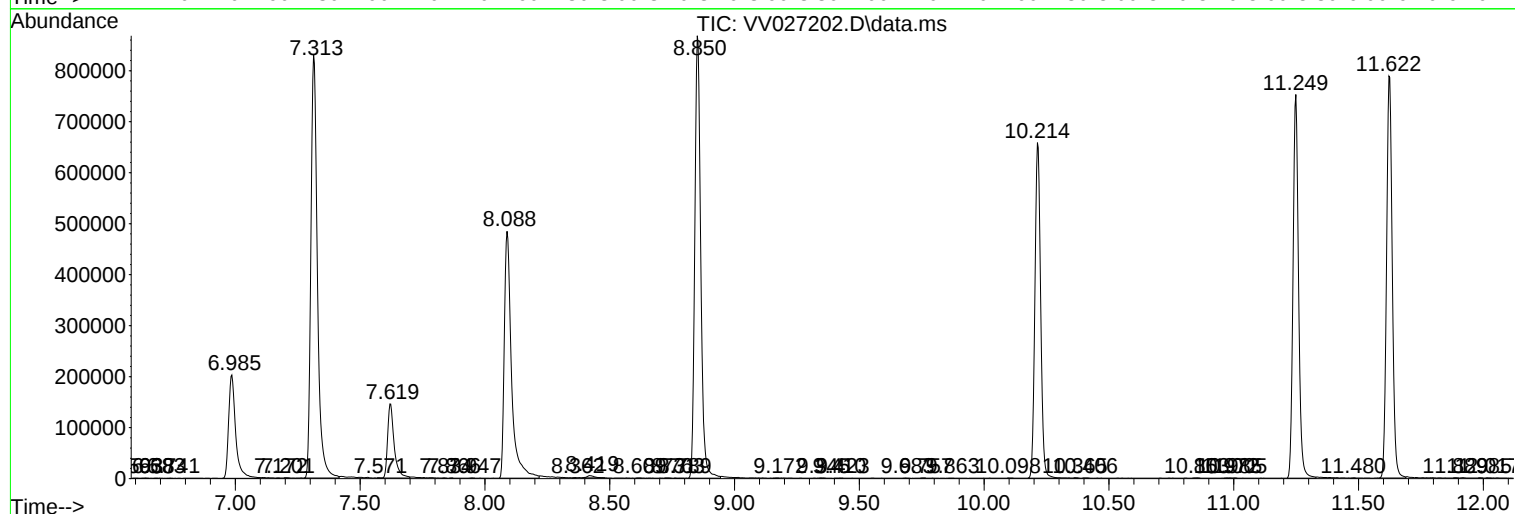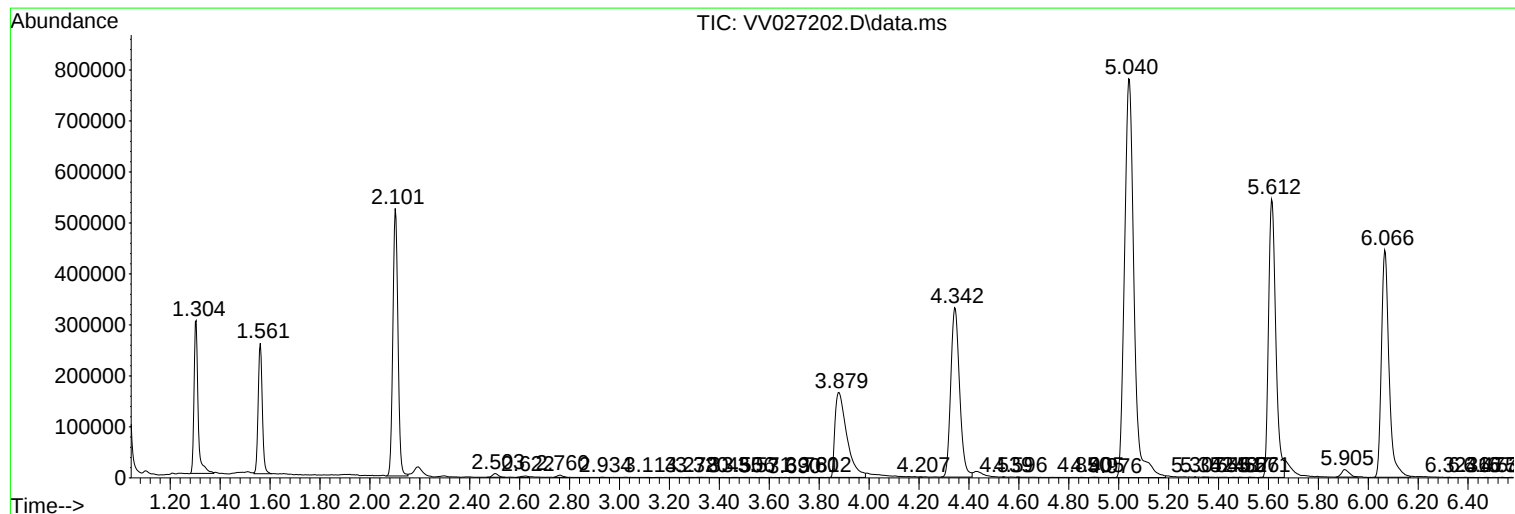

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027202.D
Acq On : 03 Aug 2022 19:30
Operator : SY/MD
Sample : VIBLK270
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080322\
Data File : VV027202.D
Acq On : 03 Aug 2022 19:30
Operator : SY/MD
Sample : VIBLK270
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------