
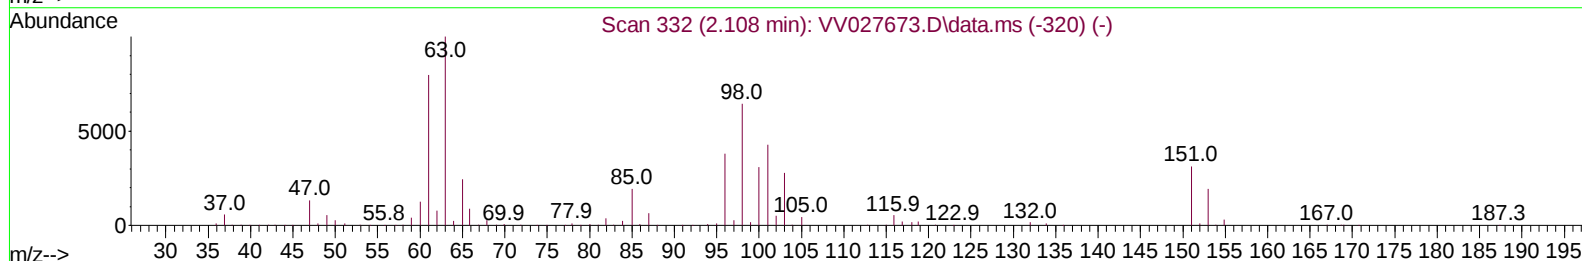
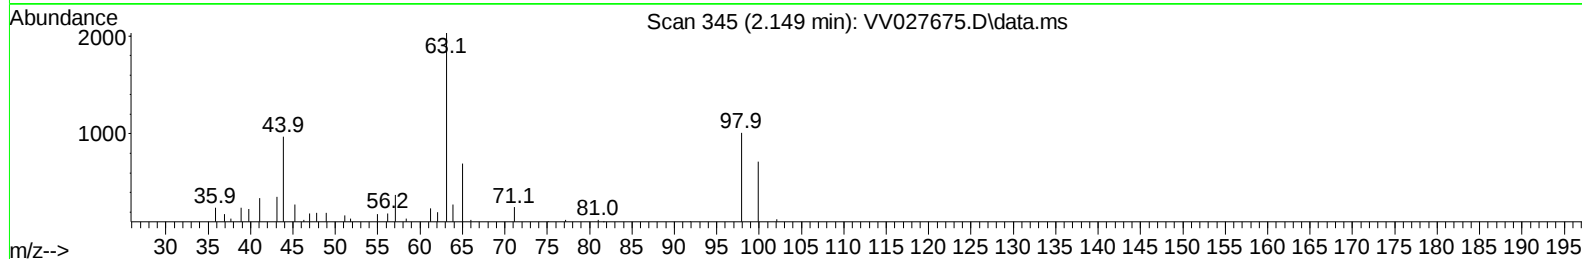


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027675.D
Acq On : 01 Sep 2022 18:34
Operator : SY/MD
Sample : N4366-07DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Sep 02 00:18:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

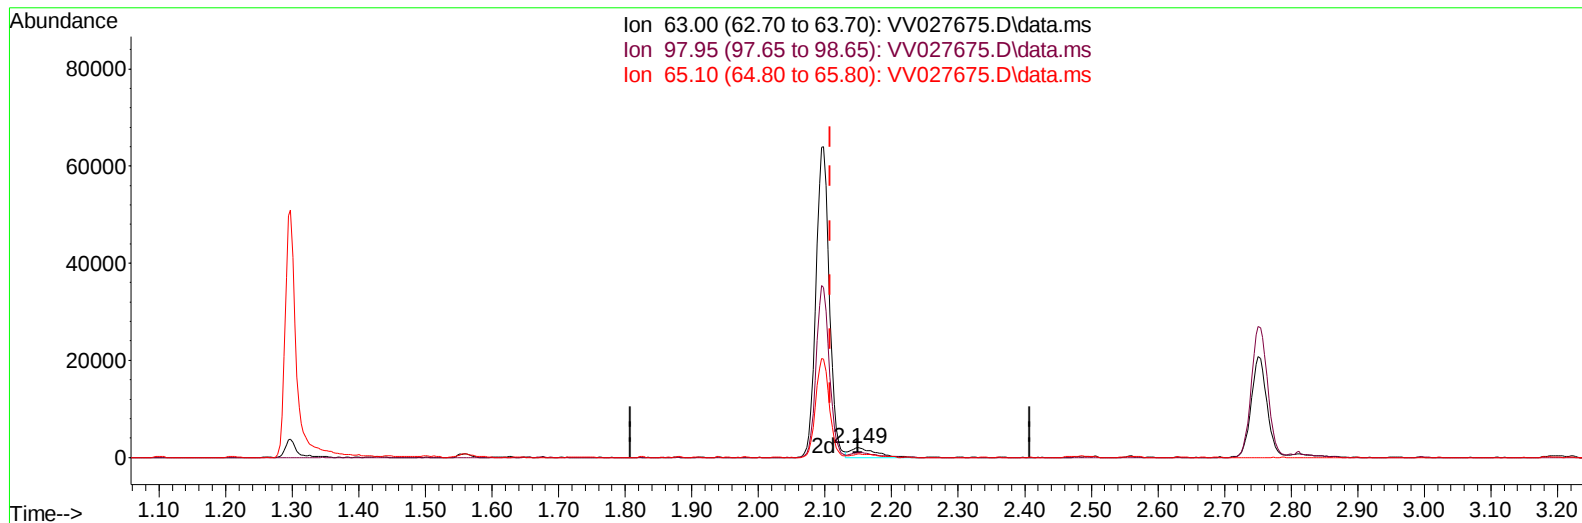

TIC: VV027675.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)




2.149min (+ 0.042) 0.17 ug/L

response 5413

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	65.90	48.09
65.10	24.10	22.87
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027675.D
Acq On : 01 Sep 2022 18:34
Operator : SY/MD
Sample : N4366-07DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Sep 02 00:18:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

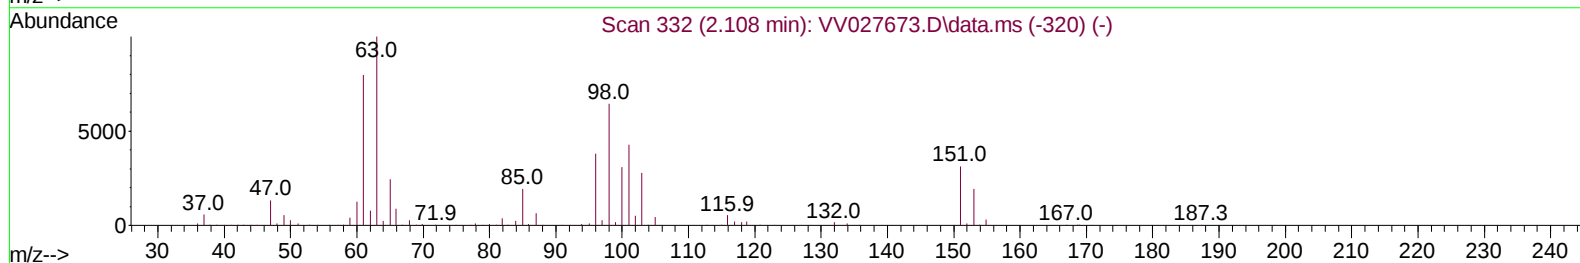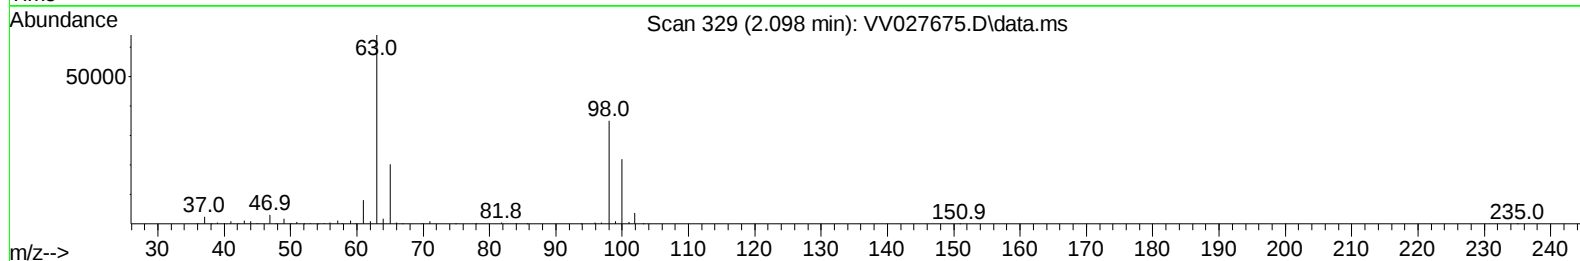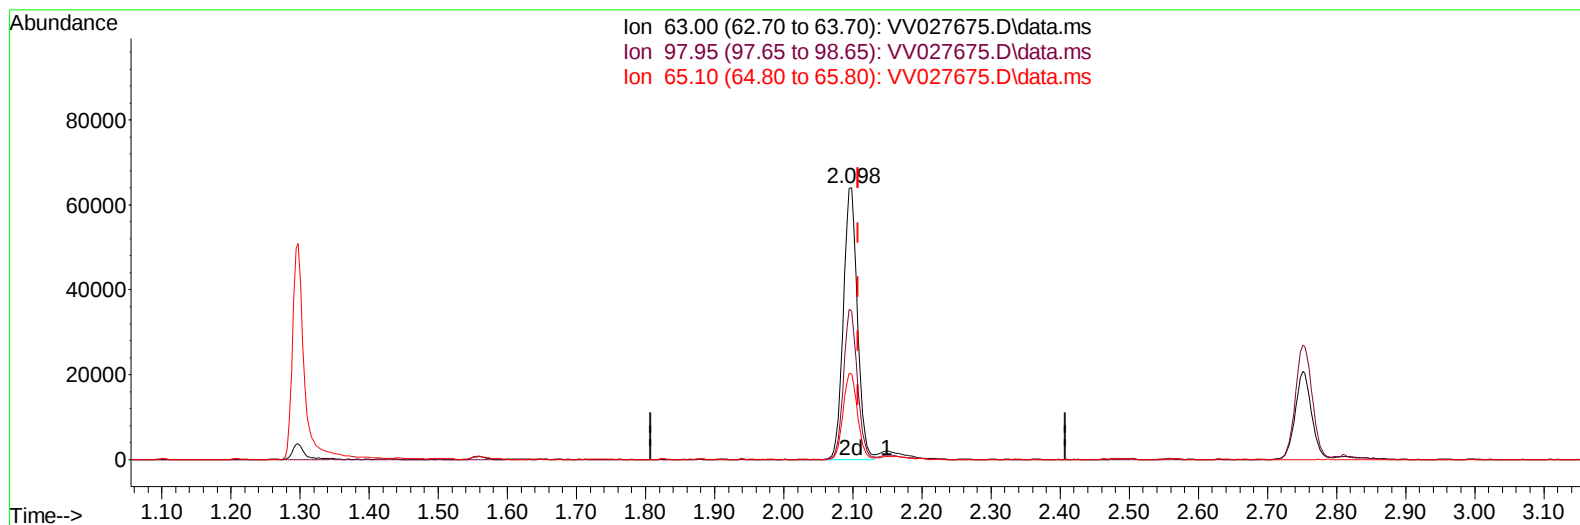

TIC: VV027675.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.098min (-0.010) 2.77 ug/L m

response 89576

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	65.90	2.91#
65.10	24.10	1.38#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027675.D
 Acq On : 01 Sep 2022 18:34
 Operator : SY/MD
 Sample : N4366-07DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Sep 02 00:18:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.596	114	151826	5.000	ug/L	-0.01
28) Chlorobenzene-d5	8.860	117	125457	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52608	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.297	65	61214	3.711	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	74.200%	
7) Chloroethane-d5	1.558	69	50926	3.690	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	73.800%	
11) 1,1-Dichloroethene-d2	2.098	63	89576m	2.775	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.400%#	
20) 2-Butanone-d5	3.956	46	137496	49.305	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.620%	
24) Chloroform-d	4.346	84	121980	3.684	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	73.600%	
26) 1,2-Dichloroethane-d4	5.021	65	66519	4.485	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.600%	
32) Benzene-d6	5.027	84	229379	4.464	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.200%	
36) 1,2-Dichloropropane-d6	6.063	67	73263	4.609	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.200%	
41) Toluene-d8	7.333	98	186471	4.190	ug/L	0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	7.641	79	22164	4.526	ug/L	0.01
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.114	63	76091	41.321	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.640%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	42919	4.196	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	56585	4.804	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.000%	
Target Compounds						
					Qvalue	
17) Methyl tert-butyl Ether	2.780	73	15658	0.578	ug/L #	73
18) trans-1,2-Dichloroethene	2.751	96	72580	5.053	ug/L	95
22) cis-1,2-Dichloroethene	3.908	96	52581	3.668	ug/L #	96
34) Trichloroethene	5.895	95	19311	1.605	ug/L	97
47) Tetrachloroethene	7.988	164	1022	0.105	ug/L	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027675.D
Acq On : 01 Sep 2022 18:34
Operator : SY/MD
Sample : N4366-07DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Sep 02 00:18:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

