




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027679.D
Acq On : 01 Sep 2022 20:12
Operator : SY/MD
Sample : N4366-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E75

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

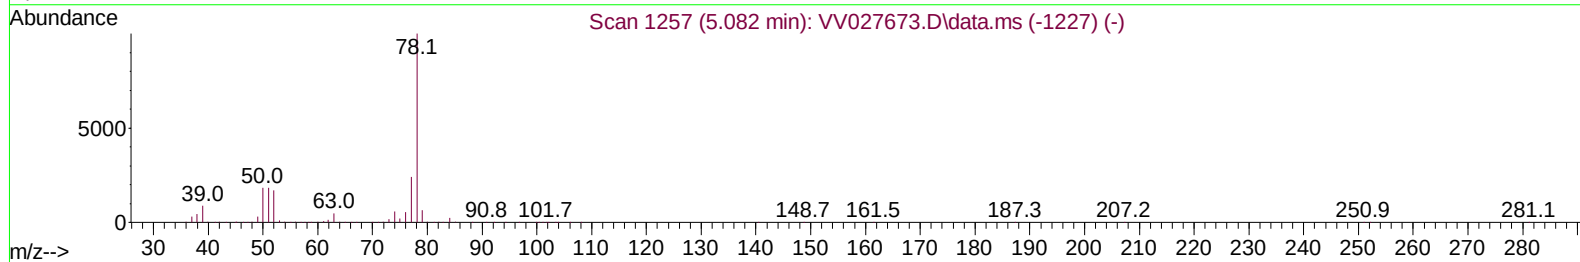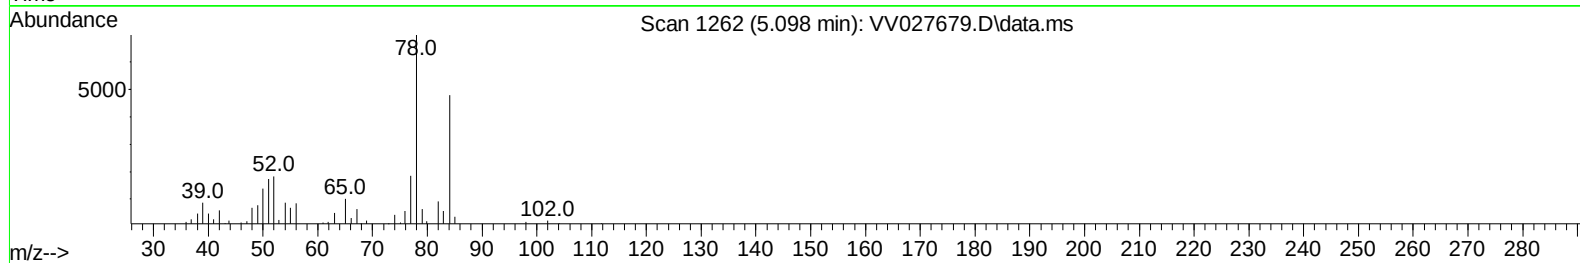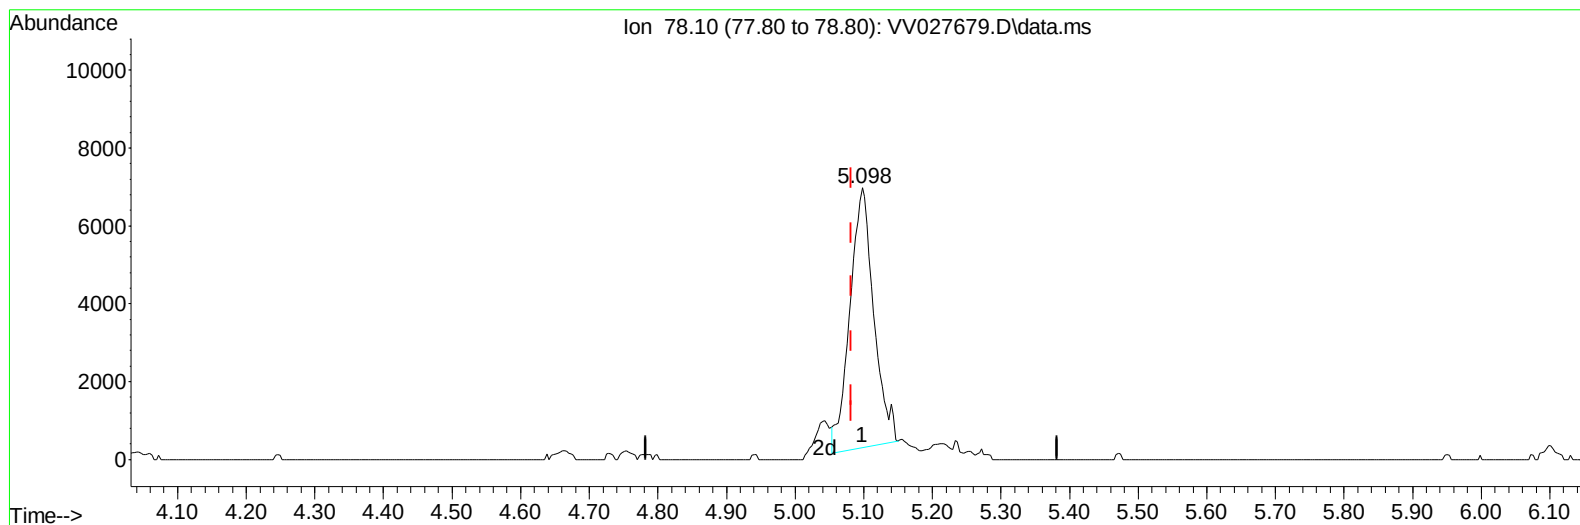

TIC: VV027679.D\data.ms

(33) Benzene (T)

5.098min (+ 0.016) 0.31 ug/L

response 16143

Ion	Exp%	Act%
78.10	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027679.D
 Acq On : 01 Sep 2022 20:12
 Operator : SY/MD
 Sample : N4366-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E75

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

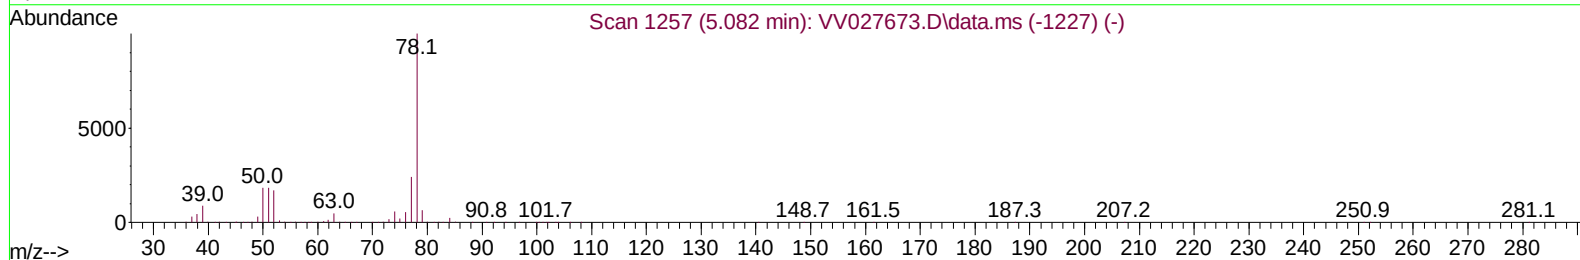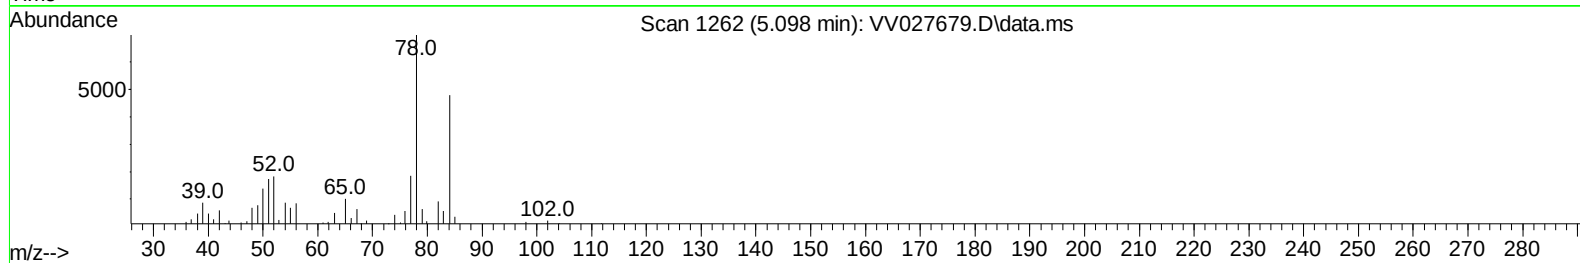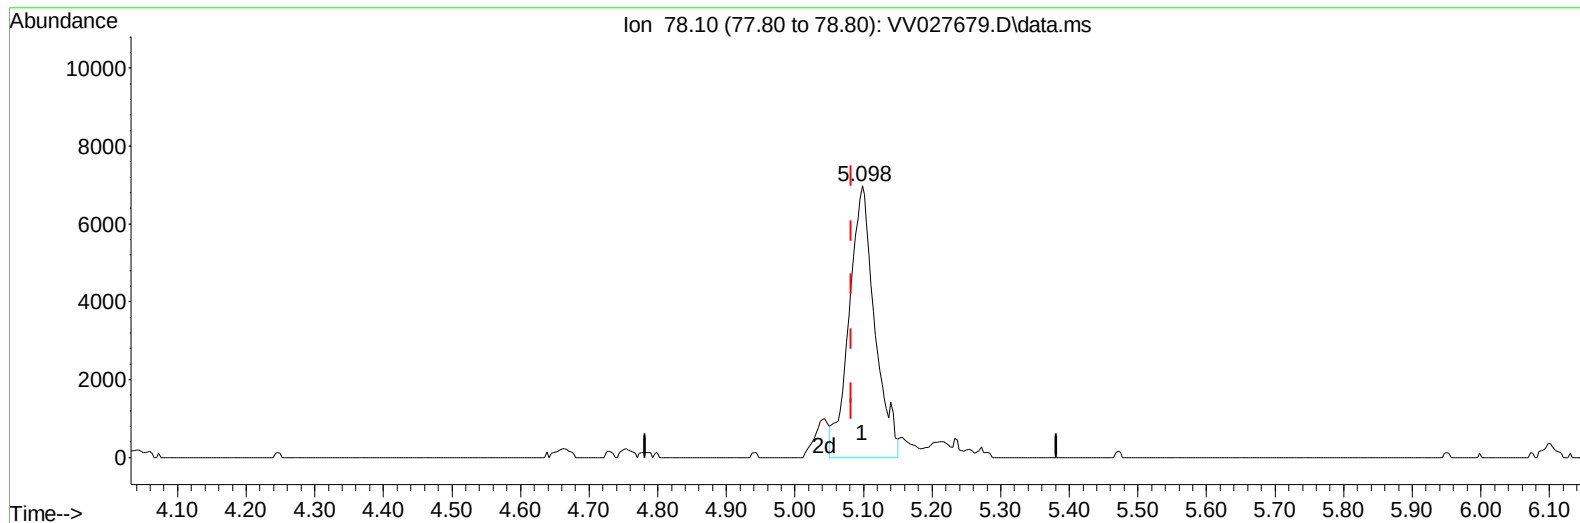

TIC: VV027679.D\data.ms

(33) Benzene (T)

5.098min (+ 0.016) 0.35 ug/L m

response 18100

Ion	Exp%	Act%
78.10	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027679.D
 Acq On : 01 Sep 2022 20:12
 Operator : SY/MD
 Sample : N4366-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E75

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

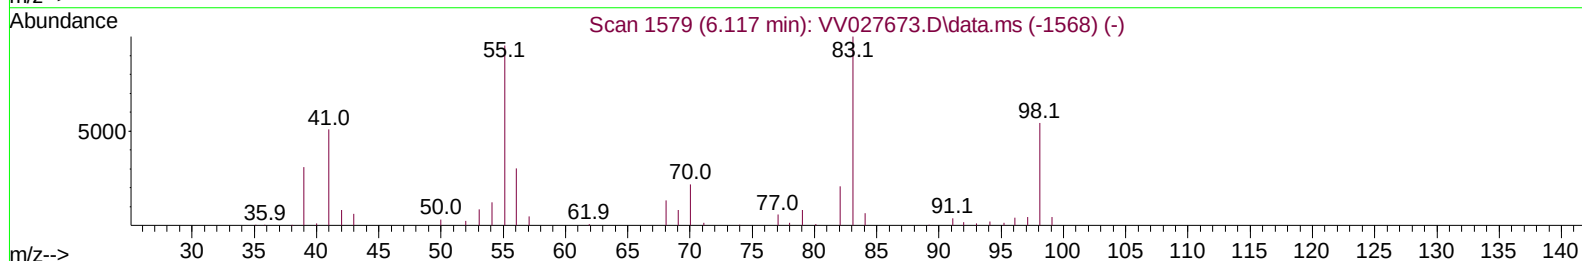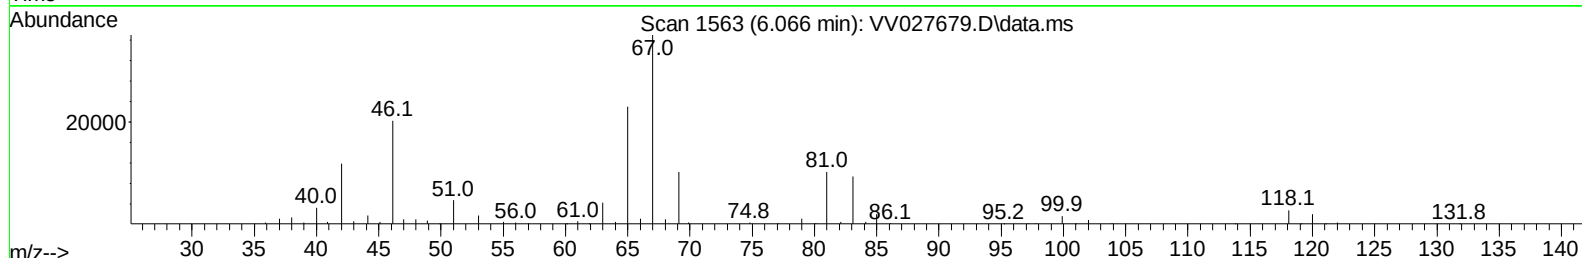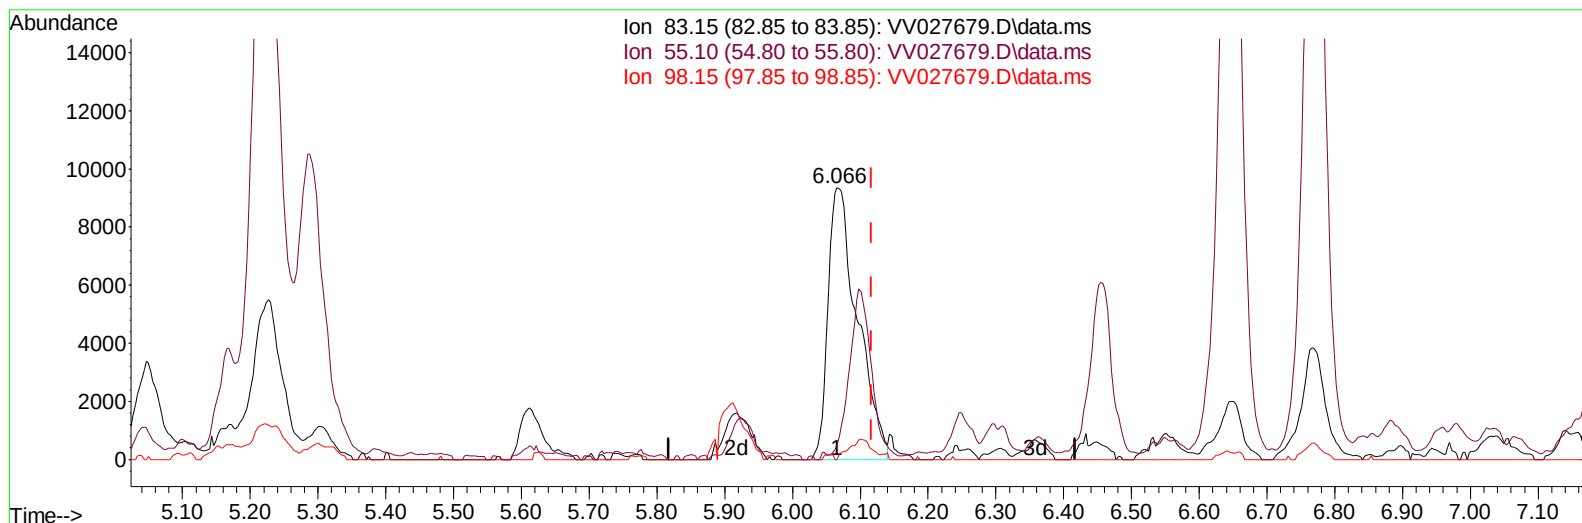

TIC: VV027679.D\data.ms

(35) Methylcyclohexane (T)

6.066min (-0.052) 1.43 ug/L

response 28160

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	82.50	0.00#
98.15	46.10	0.55#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027679.D
 Acq On : 01 Sep 2022 20:12
 Operator : SY/MD
 Sample : N4366-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E75

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

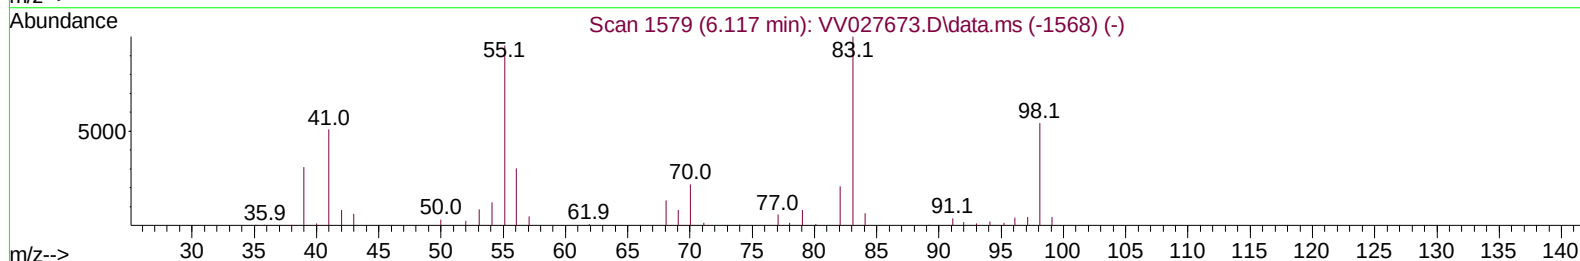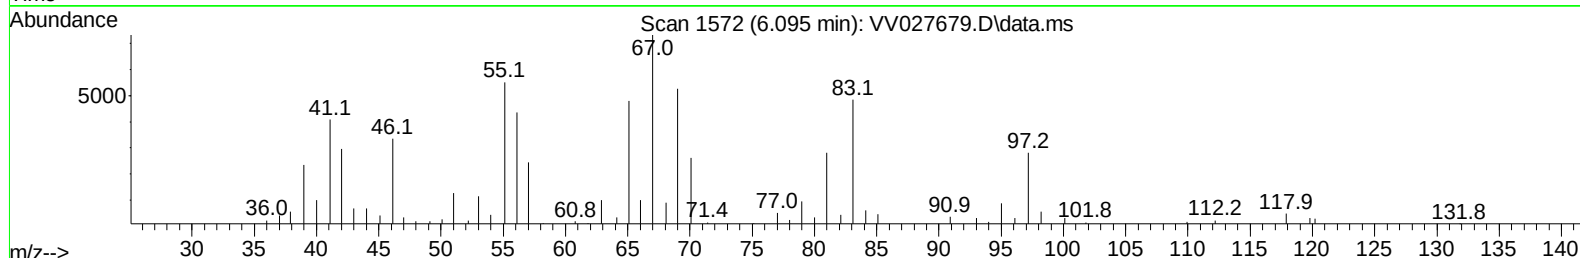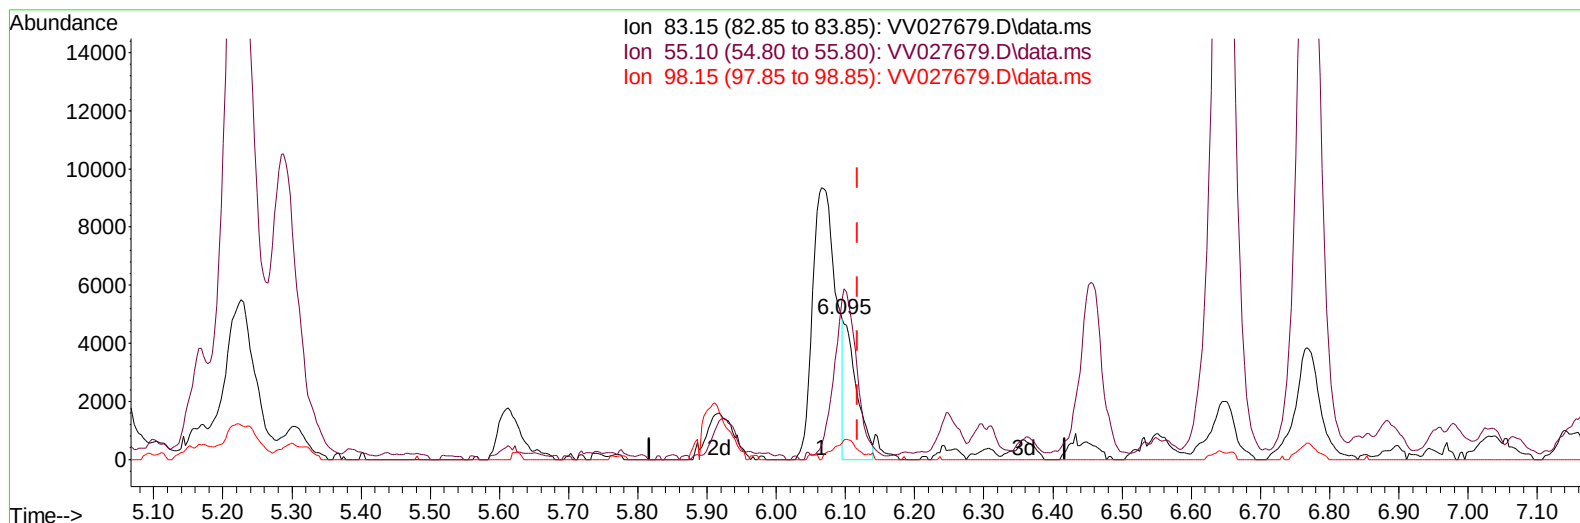

TIC: VV027679.D\data.ms

(35) Methylcyclohexane (T)

6.095min (-0.023) 0.33 ug/L m

response 6439

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	82.50	0.00#
98.15	46.10	2.41#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027679.D
 Acq On : 01 Sep 2022 20:12
 Operator : SY/MD
 Sample : N4366-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E75

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	143604	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	132698	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	57172	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	62853	4.029	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	80.600%	
7) Chloroethane-d5	1.558	69	55422	4.246	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	85.000%	
11) 1,1-Dichloroethene-d2	2.095	63	96615	3.164	ug/L	-0.01
Spiked Amount 5.000	Range 60	- 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.947	46	137062	51.964	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	103.920%	
24) Chloroform-d	4.342	84	138778	4.431	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	88.600%	
26) 1,2-Dichloroethane-d4	5.031	65	67595	4.818	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.400%	
32) Benzene-d6	5.040	84	272863	5.020	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.400%	
36) 1,2-Dichloropropane-d6	6.066	67	80197	4.770	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.400%	
41) Toluene-d8	7.313	98	218851	4.649	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	93.000%	
43) trans-1,3-Dichloroprop...	7.622	79	24513	4.733	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.095	63	93028	47.762	ug/L	-0.01
Spiked Amount 50.000	Range 45	- 130	Recovery	=	95.520%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47746	4.413	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	88.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	65509	5.118	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	102.400%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.301	62	9967	0.559	ug/L #	82
12) 1,1-Dichloroethene	2.101	96	2565	0.214	ug/L #	1
17) Methyl tert-butyl Ether	2.770	73	80530	3.145	ug/L #	1
18) trans-1,2-Dichloroethene	2.748	96	441513	32.497	ug/L	98
22) cis-1,2-Dichloroethene	3.902	96	323214	23.835	ug/L	94
30) Cyclohexane	4.664	56	9216	0.476	ug/L #	92
33) Benzene	5.098	78	18100m	0.350	ug/L	
34) Trichloroethene	5.908	95	102271	8.038	ug/L	99
35) Methylcyclohexane	6.095	83	6439m	0.326	ug/L	
47) Tetrachloroethene	7.976	164	4726	0.458	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027679.D
Acq On : 01 Sep 2022 20:12
Operator : SY/MD
Sample : N4366-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E75

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

