




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027680.D
 Acq On : 01 Sep 2022 20:37
 Operator : SY/MD
 Sample : N4366-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

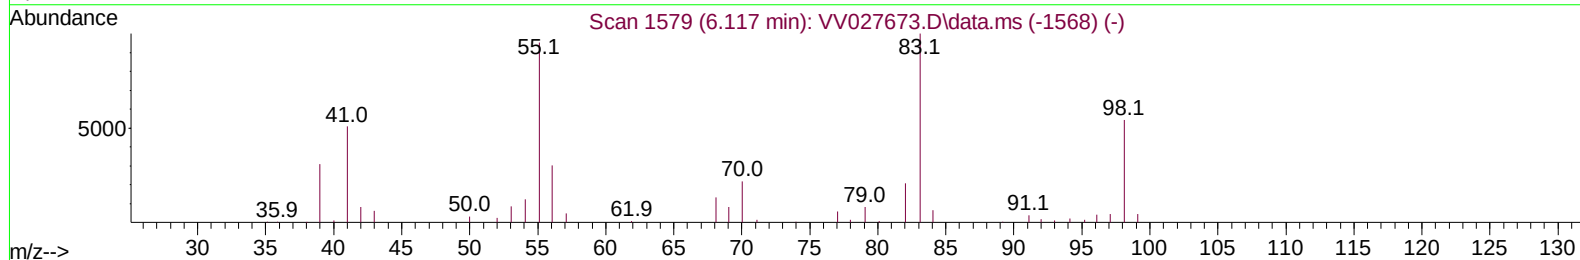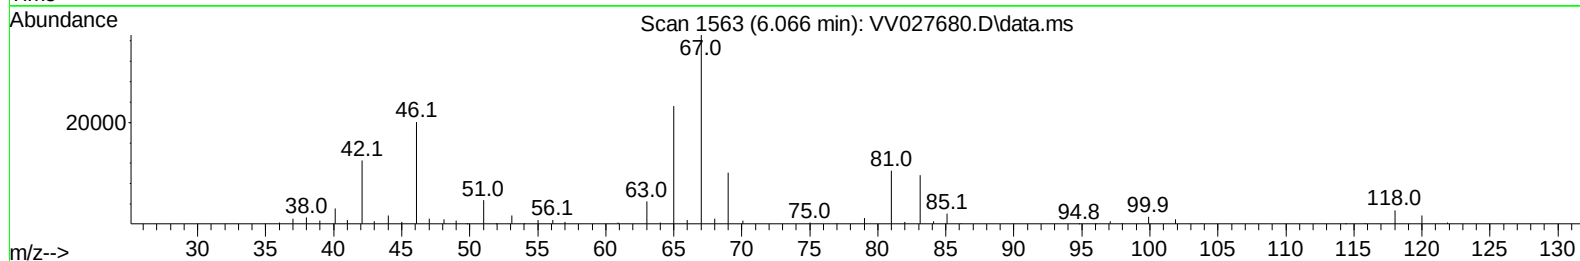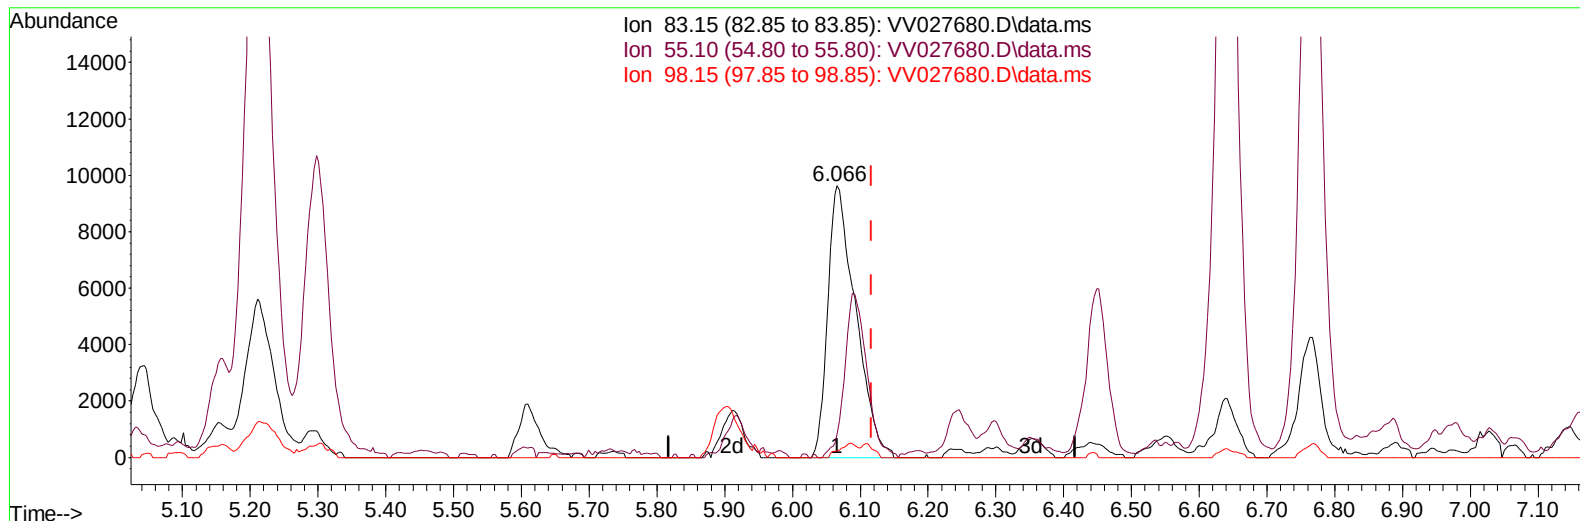

TIC: VV027680.D\data.ms

(35) Methylcyclohexane (T)

6.066min (-0.051) 1.36 ug/L

response 27386

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	82.50	48.28#
98.15	46.10	3.34#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027680.D
 Acq On : 01 Sep 2022 20:37
 Operator : SY/MD
 Sample : N4366-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

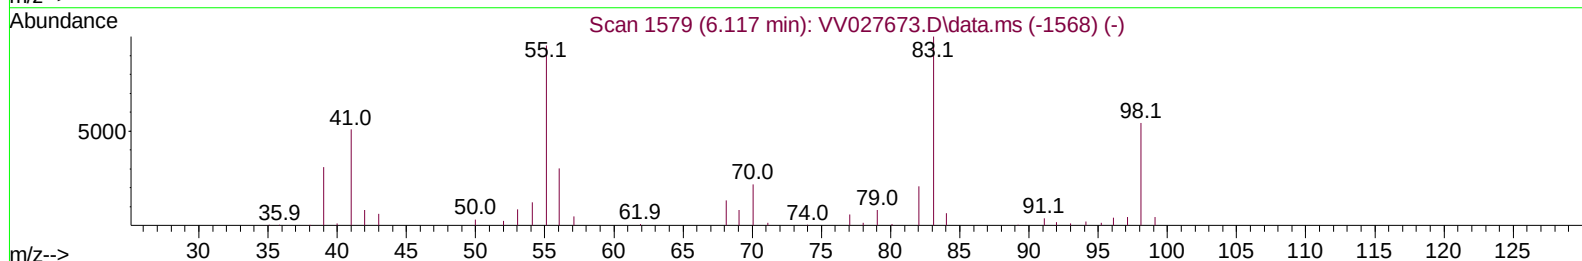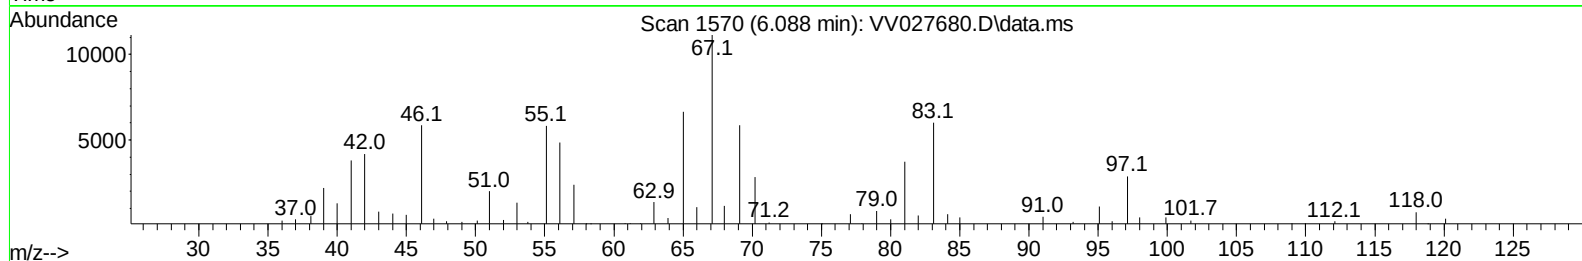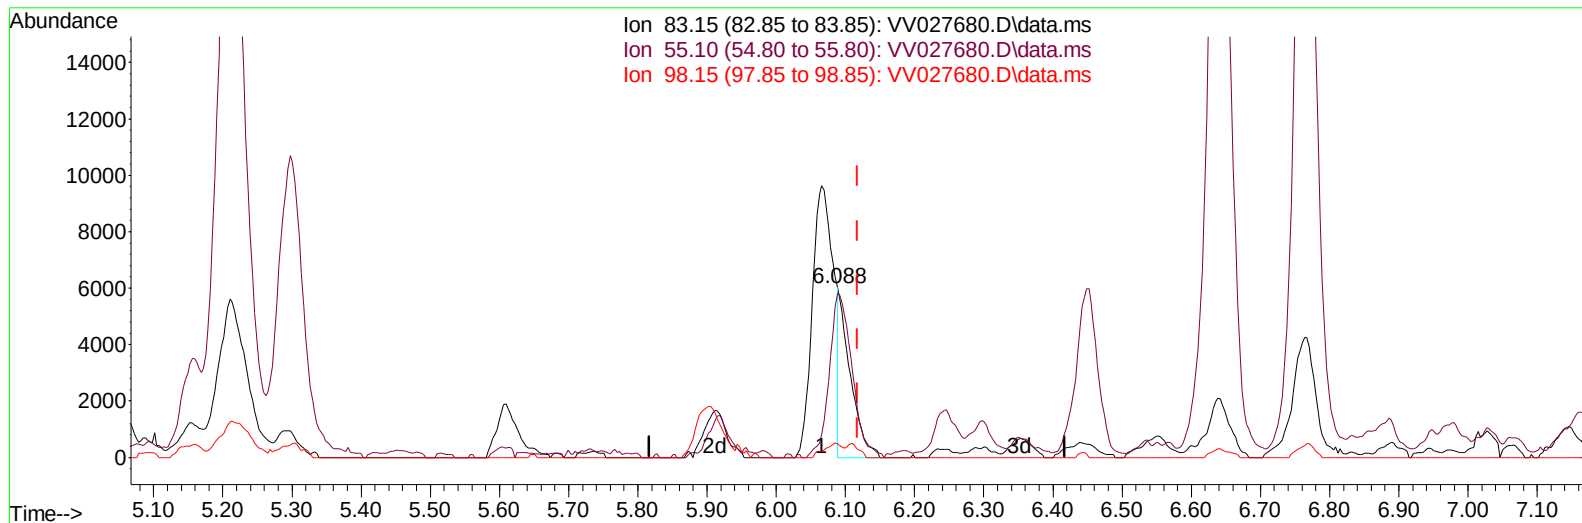

TIC: VV027680.D\data.ms

(35) Methylcyclohexane (T)

6.088min (-0.029) 0.35 ug/L m

response 6968

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	82.50	189.75#
98.15	46.10	13.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027680.D
 Acq On : 01 Sep 2022 20:37
 Operator : SY/MD
 Sample : N4366-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	143594	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	134866	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	58478	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	59879	3.838	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.800%	
7) Chloroethane-d5	1.558	69	52301	4.007	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	80.200%	
11) 1,1-Dichloroethene-d2	2.098	63	92901	3.043	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	60.800%	
20) 2-Butanone-d5	3.953	46	147595	55.961	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	111.920%	
24) Chloroform-d	4.336	84	134600	4.298	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.000%	
26) 1,2-Dichloroethane-d4	5.027	65	65564	4.674	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	93.400%	
32) Benzene-d6	5.037	84	256899	4.650	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.066	67	79540	4.655	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	93.000%	
41) Toluene-d8	7.310	98	206293	4.312	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	7.622	79	21683	4.119	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	82.400%	
46) 2-Hexanone-d5	8.098	63	87523	44.213	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	88.420%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47093	4.283	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	85.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	64623	4.936	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	98.800%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.301	62	9669	0.542	ug/L #	80
12) 1,1-Dichloroethene	2.101	96	1893	0.158	ug/L #	1
17) Methyl tert-butyl Ether	2.773	73	84223	3.289	ug/L #	74
18) trans-1,2-Dichloroethene	2.744	96	396764	29.205	ug/L	98
22) cis-1,2-Dichloroethene	3.896	96	299390	22.080	ug/L #	99
30) Cyclohexane	4.651	56	9007	0.458	ug/L	94
33) Benzene	5.088	78	18949	0.360	ug/L	100
34) Trichloroethene	5.902	95	99577	7.701	ug/L	99
35) Methylcyclohexane	6.088	83	6968m	0.347	ug/L	
47) Tetrachloroethene	7.969	164	4636	0.442	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027680.D
Acq On : 01 Sep 2022 20:37
Operator : SY/MD
Sample : N4366-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:19:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

