
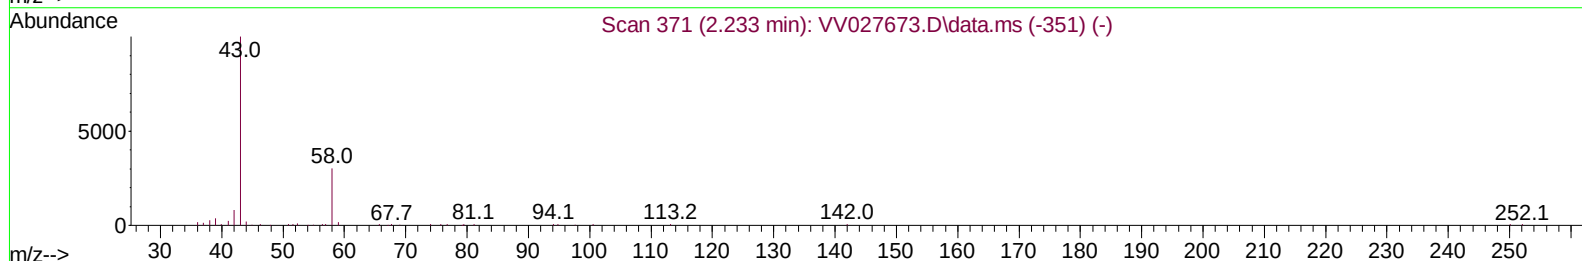
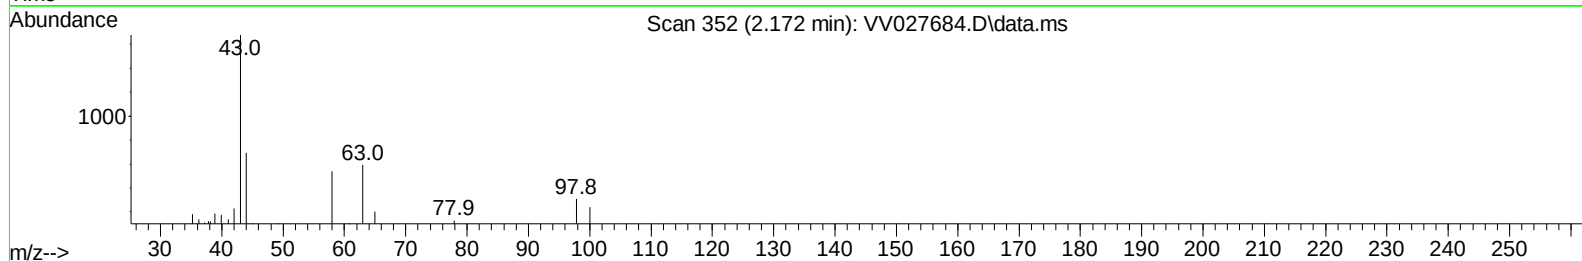


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027684.D
Acq On : 01 Sep 2022 22:15
Operator : SY/MD
Sample : N4369-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 02 00:20:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

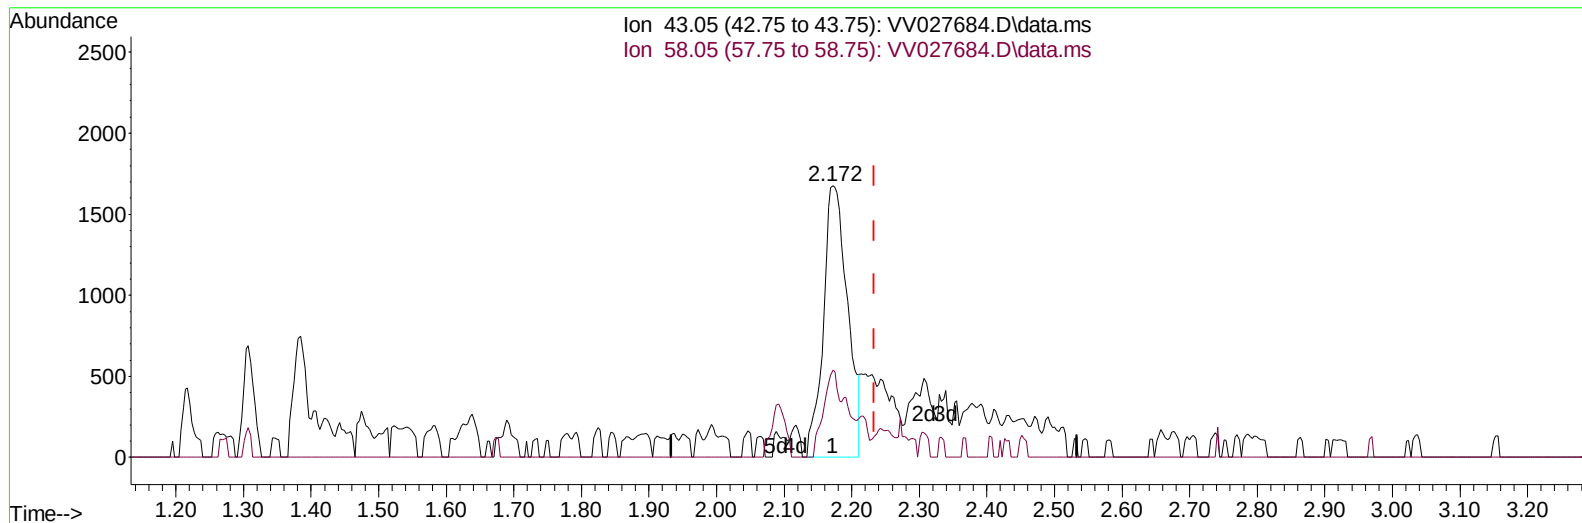

TIC: VV027684.D\data.ms

(13) Acetone (T)




2.172min (-0.061) 2.87 ug/L

response 4192

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	21.23
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027684.D
Acq On : 01 Sep 2022 22:15
Operator : SY/MD
Sample : N4369-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 02 00:20:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

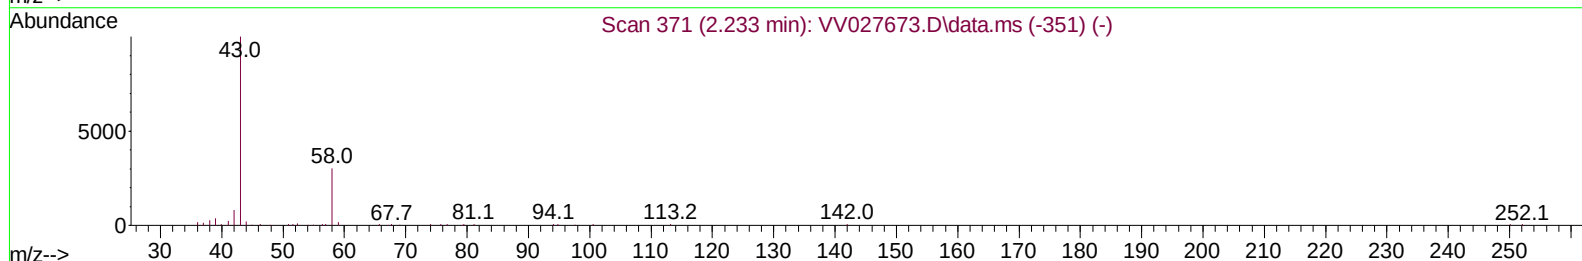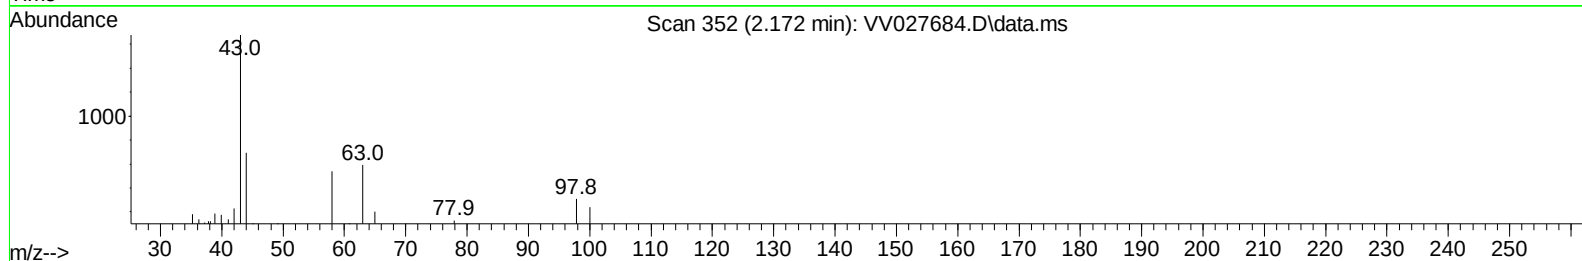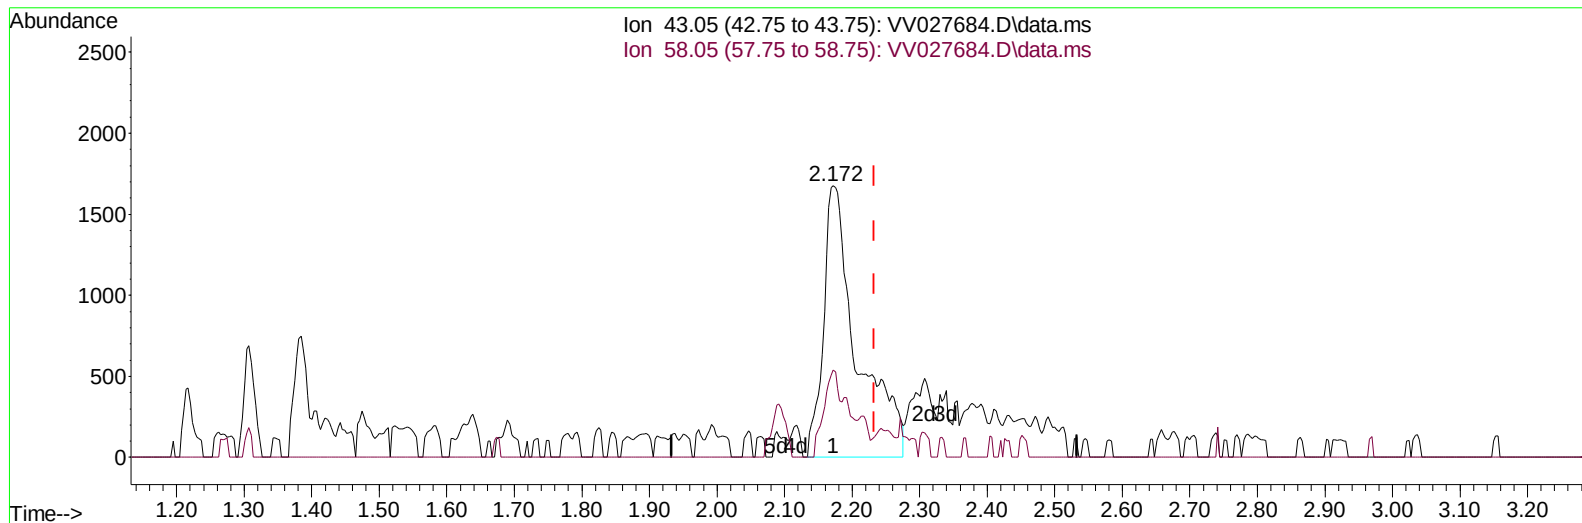

TIC: VV027684.D\data.ms

(13) Acetone (T)

2.172min (-0.061) 3.97 ug/L m

response 5797

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	15.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027684.D
 Acq On : 01 Sep 2022 22:15
 Operator : SY/MD
 Sample : N4369-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 02 00:20:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	117356	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	119888	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50582	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60872	4.775	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	95.400%	
7) Chloroethane-d5	1.568	69	55091	5.165	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	103.200%	
11) 1,1-Dichloroethene-d2	2.108	63	94819	3.800	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	76.000%	
20) 2-Butanone-d5	3.889	46	83344	38.665	ug/L	-0.06
Spiked Amount 50.000	Range 40	- 130	Recovery	=	77.320%	
24) Chloroform-d	4.342	84	129804	5.072	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	5.031	65	60538	5.280	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.600%	
32) Benzene-d6	5.047	84	235135	4.788	ug/L	0.02
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.066	67	71252	4.691	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	93.800%	
41) Toluene-d8	7.313	98	179822	4.228	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	84.600%	
43) trans-1,3-Dichloroprop...	7.622	79	20948	4.477	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	89.600%	
46) 2-Hexanone-d5	8.088	63	76684	43.577	ug/L	-0.02
Spiked Amount 50.000	Range 45	- 130	Recovery	=	87.160%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	44044	4.506	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	90.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60349	5.329	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	106.600%	
Target Compounds						
13) Acetone	2.172	43	5797m	3.975	ug/L	
21) 2-Butanone	3.989	43	11697	5.913	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027684.D
Acq On : 01 Sep 2022 22:15
Operator : SY/MD
Sample : N4369-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 02 00:20:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

