




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027687.D
 Acq On : 01 Sep 2022 23:28
 Operator : SY/MD
 Sample : N4400-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVP1

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:21:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

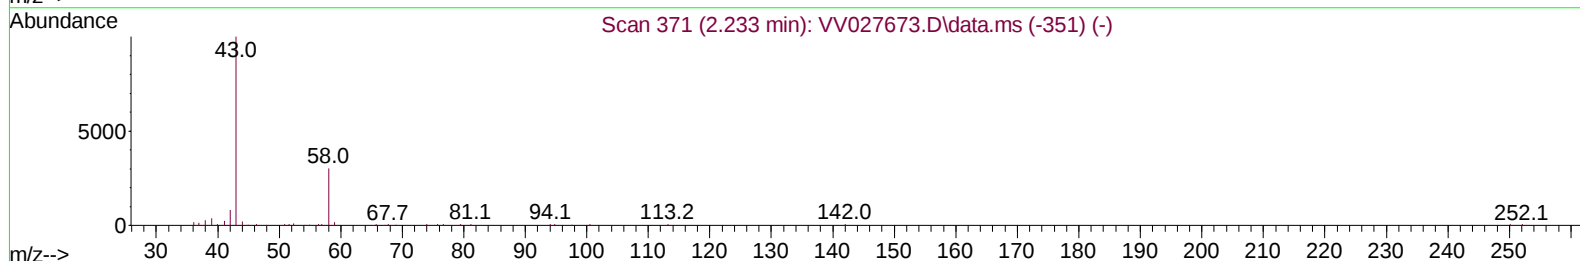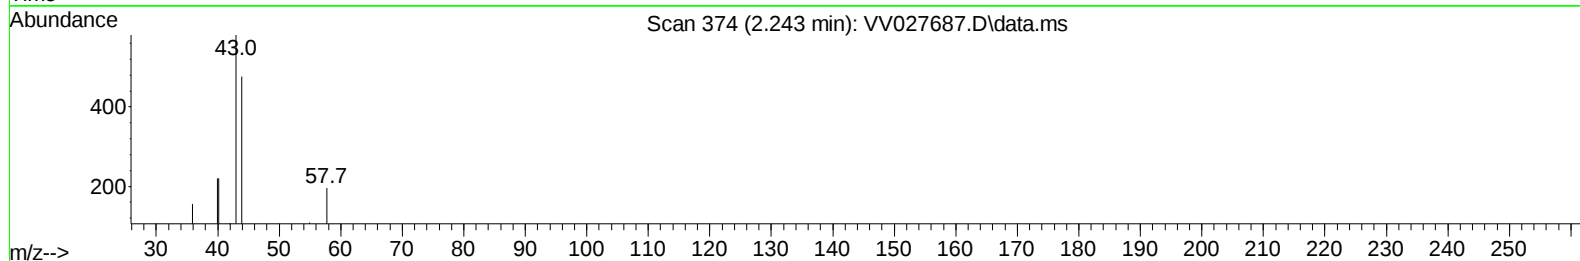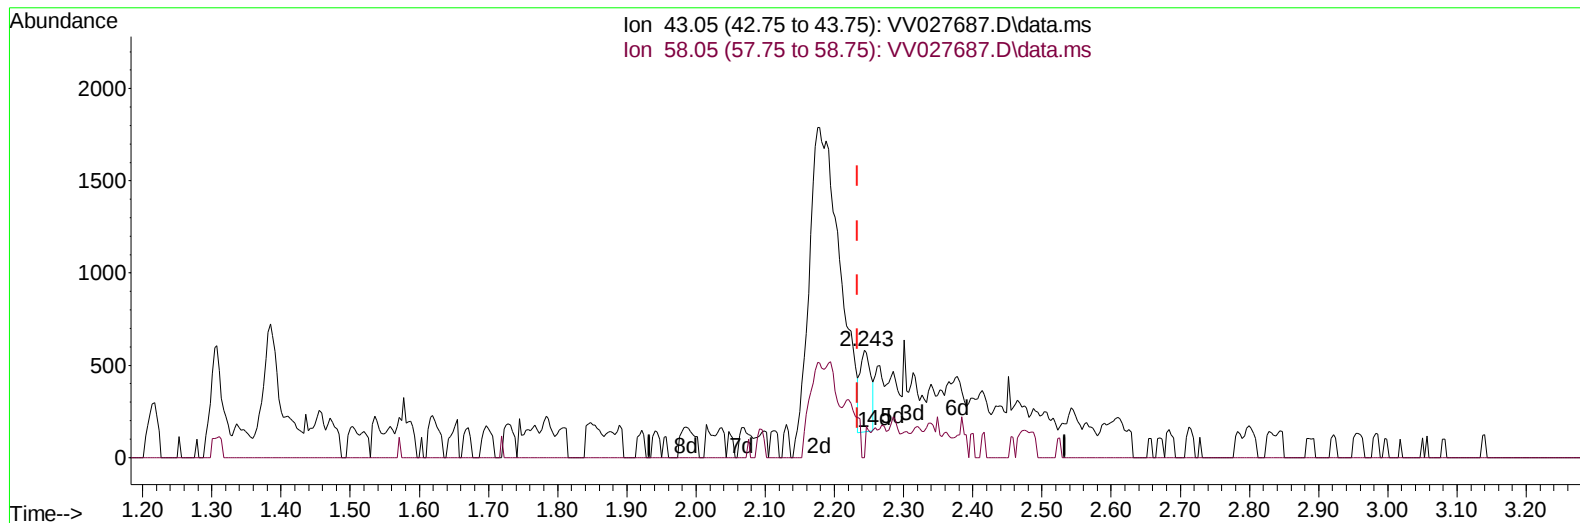

TIC: VV027687.D\data.ms

(13) Acetone (T)

2.243min (+ 0.010) 0.30 ug/L

response 486

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	17.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027687.D
Acq On : 01 Sep 2022 23:28
Operator : SY/MD
Sample : N4400-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVP1

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:21:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

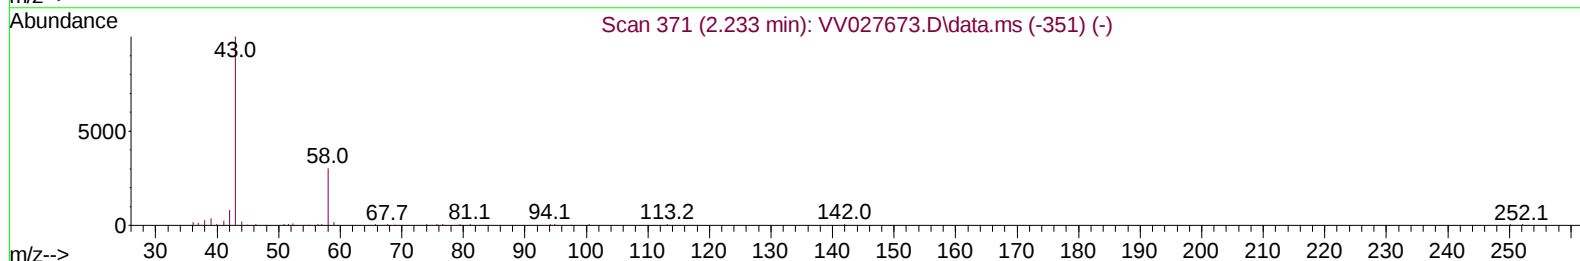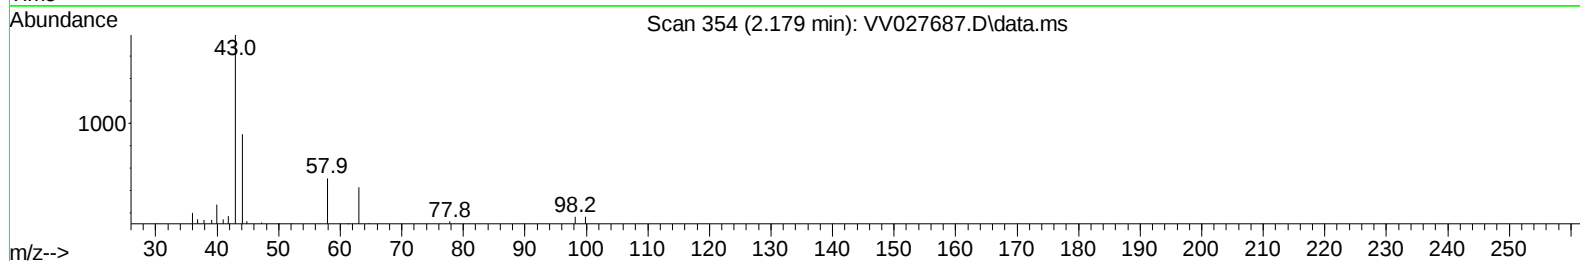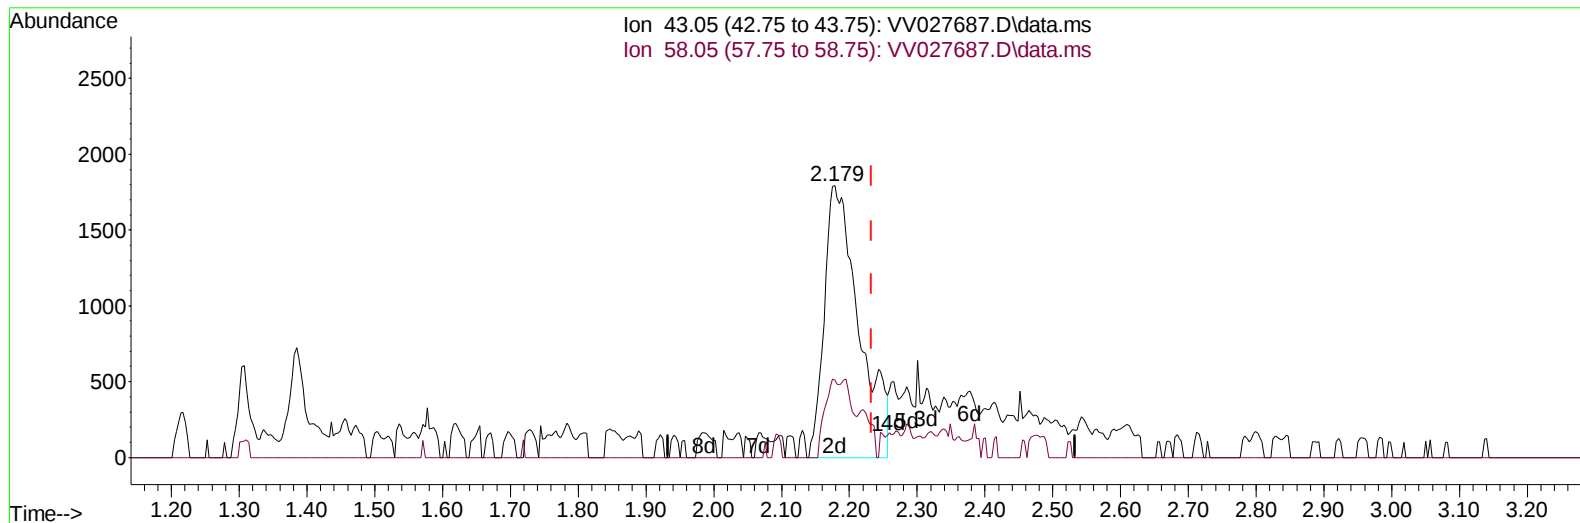

TIC: VV027687.D\data.ms

(13) Acetone (T)

2.179min (-0.055) 3.98 ug/L m

response 6367

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	1.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027687.D
 Acq On : 01 Sep 2022 23:28
 Operator : SY/MD
 Sample : N4400-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVP1

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:21:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	128795	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	127444	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53656	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59750	4.270	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery =	85.400%		
7) Chloroethane-d5	1.568	69	53562	4.575	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery =	91.600%		
11) 1,1-Dichloroethene-d2	2.105	63	94374	3.446	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery =	69.000%		
20) 2-Butanone-d5	3.896	46	67210	28.411	ug/L	-0.05
Spiked Amount 50.000	Range 40	- 130	Recovery =	56.820%		
24) Chloroform-d	4.346	84	127379	4.535	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	90.600%		
26) 1,2-Dichloroethane-d4	5.031	65	59385	4.720	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	94.400%		
32) Benzene-d6	5.047	84	234191	4.486	ug/L	0.02
Spiked Amount 5.000	Range 70	- 125	Recovery =	89.800%		
36) 1,2-Dichloropropane-d6	6.066	67	69088	4.279	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery =	85.600%		
41) Toluene-d8	7.314	98	179714	3.975	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	79.600%		
43) trans-1,3-Dichloroprop...	7.622	79	20781	4.178	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery =	83.600%		
46) 2-Hexanone-d5	8.088	63	77189	41.264	ug/L	-0.02
Spiked Amount 50.000	Range 45	- 130	Recovery =	82.520%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	43158	4.153	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery =	83.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	61473	5.117	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery =	102.400%		
Target Compounds						
					Qvalue	
13) Acetone	2.179	43	6367m	3.978	ug/L	
14) Carbon disulfide	2.291	76	3916	0.115	ug/L #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027687.D
Acq On : 01 Sep 2022 23:28
Operator : SY/MD
Sample : N4400-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBVP1

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:21:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

