

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027688.D
 Acq On : 01 Sep 2022 23:53
 Operator : SY/MD
 Sample : N4400-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG7

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Quant Time: Sep 02 00:21:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	127138	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	122456	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50969	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60844	4.405	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.200%	
7) Chloroethane-d5	1.568	69	54224	4.692	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.800%	
11) 1,1-Dichloroethene-d2	2.108	63	93831	3.471	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.400%	
20) 2-Butanone-d5	3.892	46	70754	30.299	ug/L	-0.06
Spiked Amount	50.000	Range 40 - 130	Recovery	=	60.600%	
24) Chloroform-d	4.346	84	126828	4.574	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.400%	
26) 1,2-Dichloroethane-d4	5.031	65	57890	4.661	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.200%	
32) Benzene-d6	5.047	84	230646	4.598	ug/L	0.02
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
36) 1,2-Dichloropropane-d6	6.066	67	69708	4.493	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.800%	
41) Toluene-d8	7.313	98	181544	4.179	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.600%	
43) trans-1,3-Dichloroprop...	7.625	79	21074	4.409	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.200%	
46) 2-Hexanone-d5	8.088	63	76389	42.499	ug/L	-0.02
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.000%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	42654	4.272	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	85.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	58558	5.132	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.600%	
Target Compounds					Qvalue	
13) Acetone	2.172	43	10416m	6.592	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027688.D
Acq On : 01 Sep 2022 23:53
Operator : SY/MD
Sample : N4400-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBVG7

Quant Time: Sep 02 00:21:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

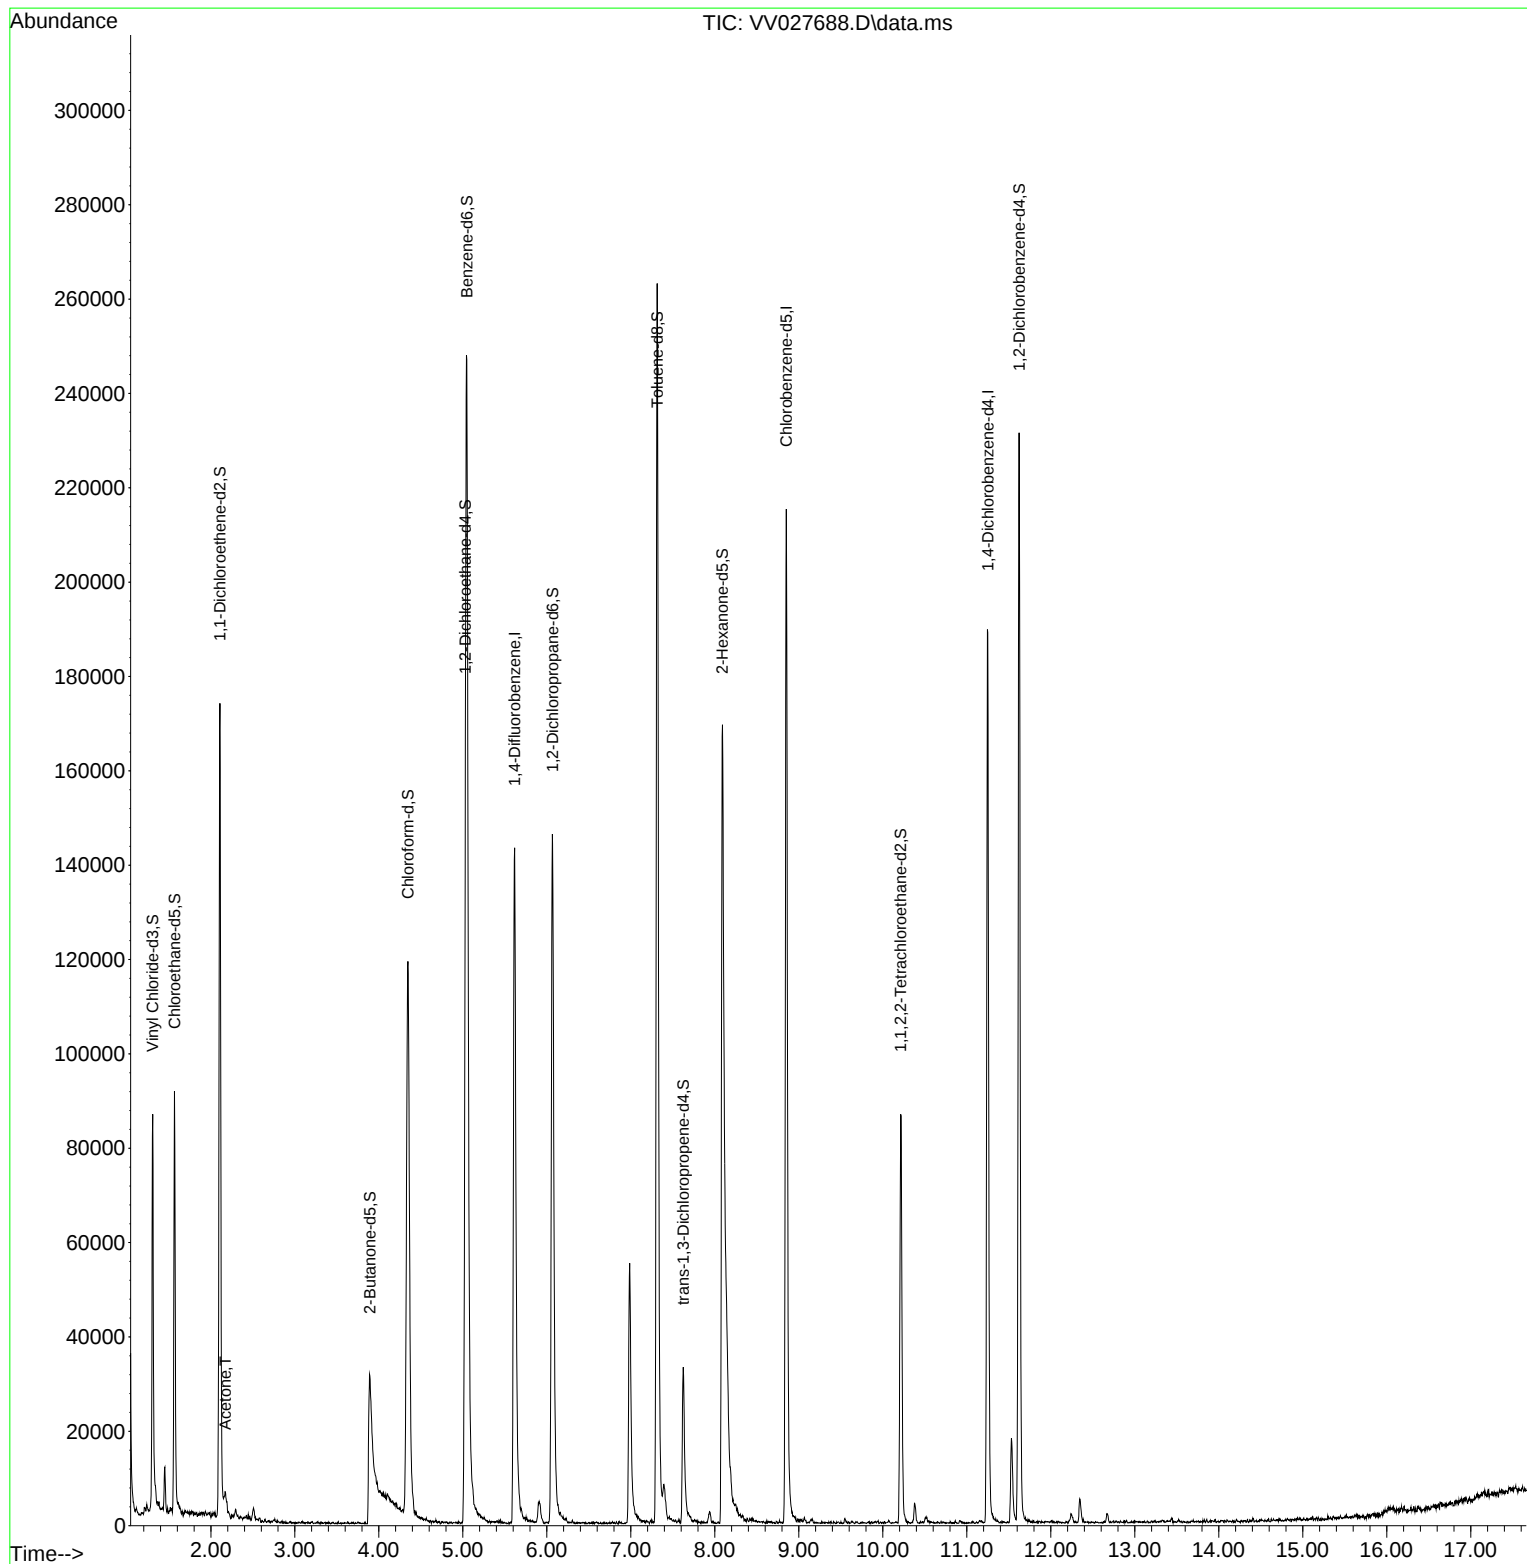

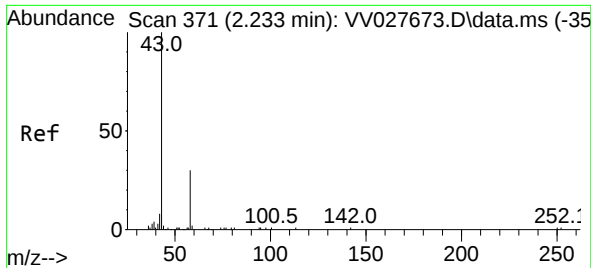

#13
 Acetone
 Concen: 6.592 ug/L m
 RT: 2.172 min Scan# 352
 Delta R.T. -0.061 min
 Lab File: VV027688.D
 Acq: 01 Sep 2022 23:53

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG7

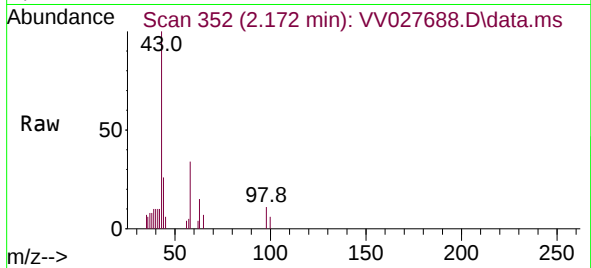

Tgt Ion: 43 Resp: 10416
 Ion Ratio Lower Upper
 43 100
 58 0.8 0.0 38.4

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

