

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027691.D
 Acq On : 02 Sep 2022 01:06
 Operator : SY/MD
 Sample : N4396-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB9

Quant Time: Sep 02 01:39:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 00:17:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	118359	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	112850	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	46515	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59386	4.619	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.400%
7) Chloroethane-d5	1.568	69	53285	4.953	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.000%
11) 1,1-Dichloroethene-d2	2.108	63	91313	3.628	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	3.892	46	78400	36.063	ug/L	-0.06
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.120%
24) Chloroform-d	4.346	84	125372	4.857	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.030	65	59908	5.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	5.047	84	231464	5.007	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
36) 1,2-Dichloropropane-d6	6.066	67	71001	4.966	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.400%
41) Toluene-d8	7.313	98	175415	4.382	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	7.622	79	21117	4.794	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.800%
46) 2-Hexanone-d5	8.088	63	80617	48.669	ug/L	-0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.340%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40795	4.434	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	57976	5.567	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.400%
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	7127	0.572	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027691.D
Acq On : 02 Sep 2022 01:06
Operator : SY/MD
Sample : N4396-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB9

Quant Time: Sep 02 01:39:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 00:17:48 2022
Response via : Initial Calibration

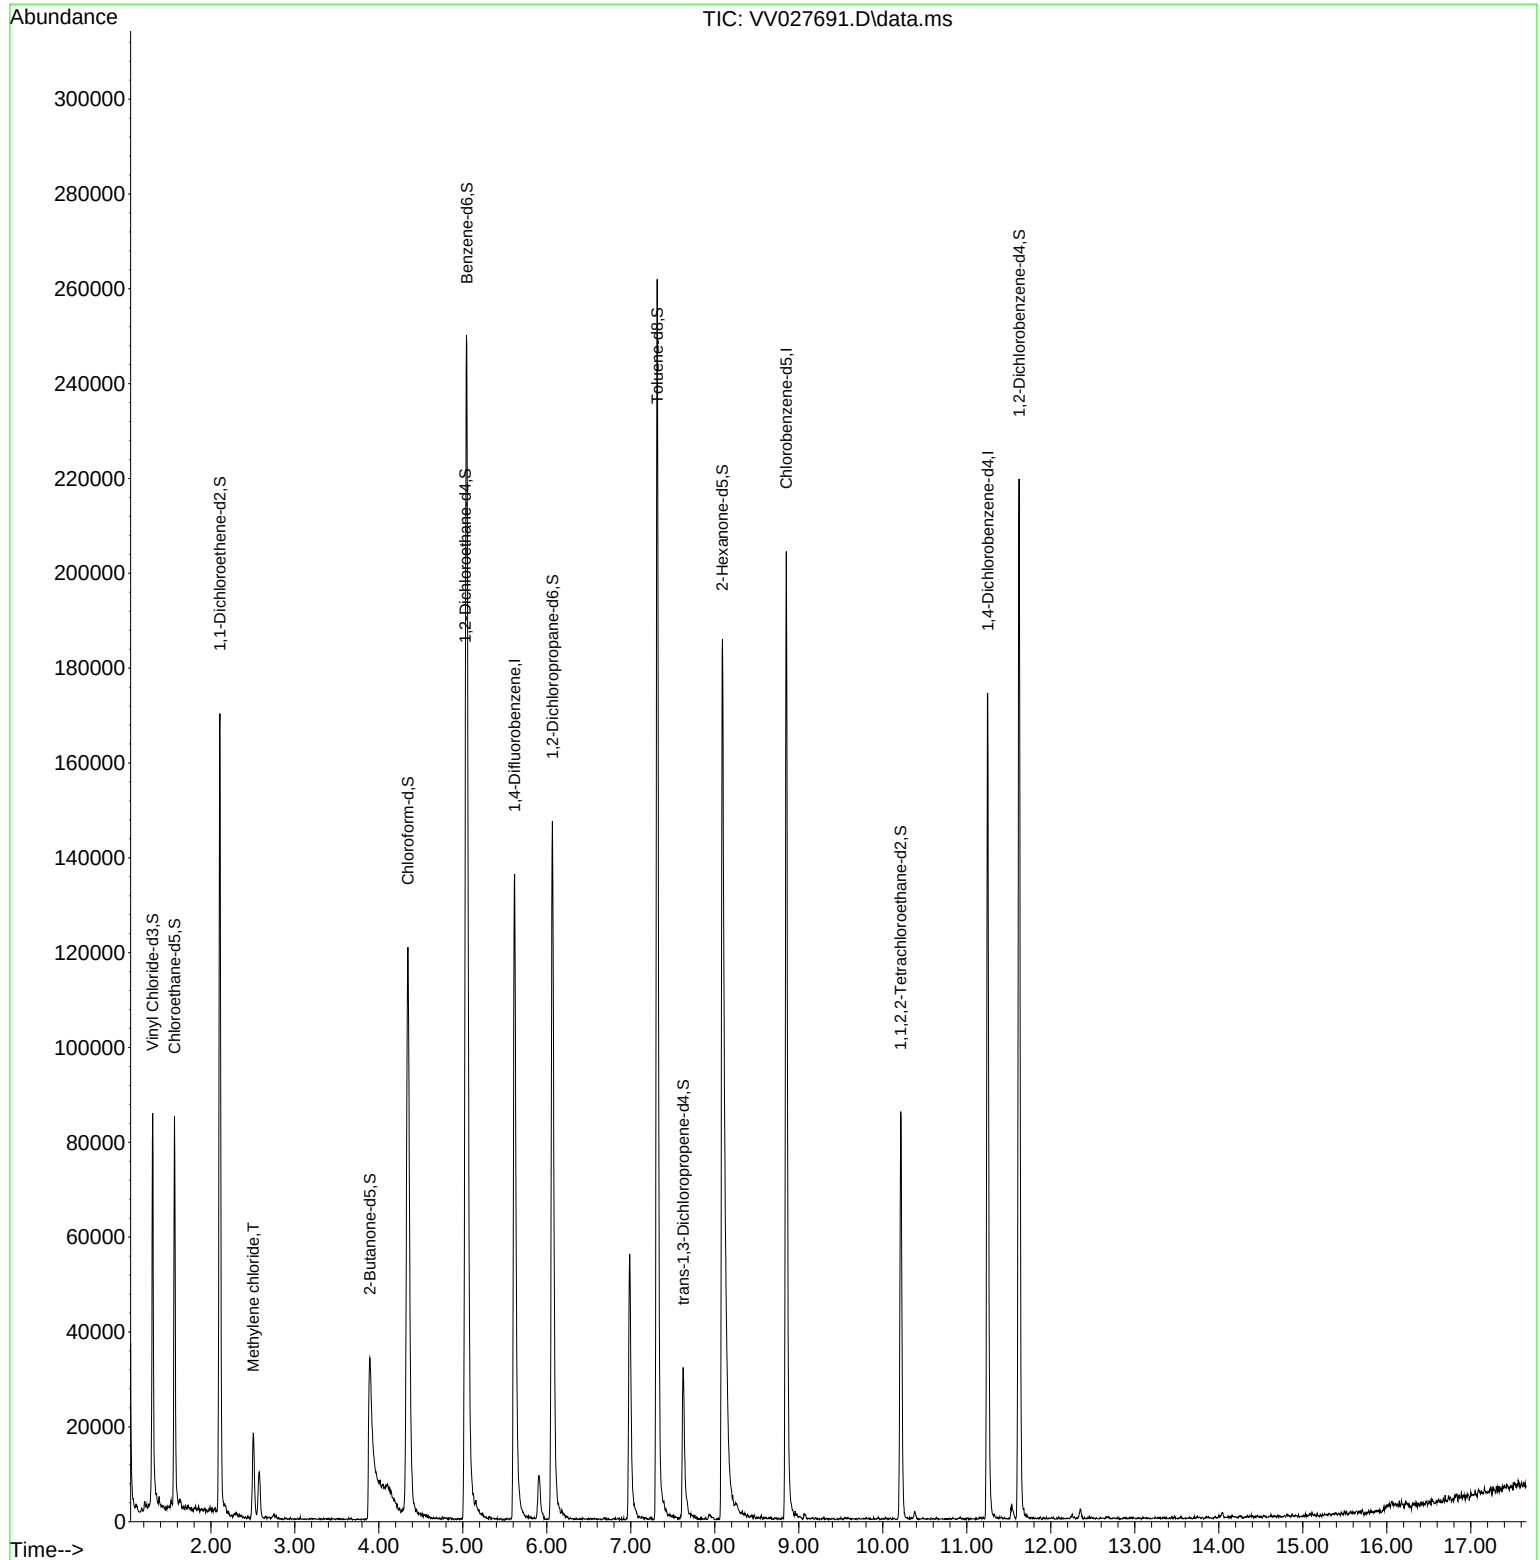

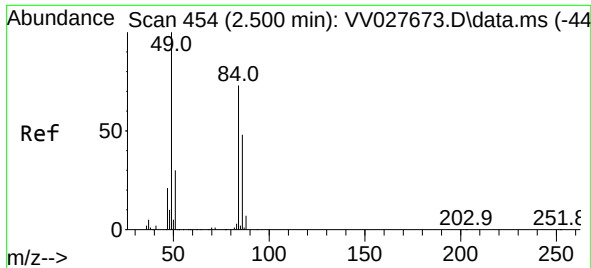

#16
Methylene chloride
Concen: 0.572 ug/L
RT: 2.506 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV027691.D
Acq: 02 Sep 2022 01:06

Instrument :
MSVOA_V
ClientSampleId :
C0AB9

Tgt Ion: 84 Resp: 7127
Ion Ratio Lower Upper
84 100
86 66.8 43.9 81.5
49 131.1 92.5 171.7

