

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027714.D
 Acq On : 02 Sep 2022 11:10
 Operator : SY/MD
 Sample : N4370-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 03 04:16:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 03:03:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	125096	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	122820	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	52456	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	62817	4.622	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.400%
7) Chloroethane-d5	1.568	69	52401	4.609	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.105	63	97186	3.654	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.000%
20) 2-Butanone-d5	3.899	46	79074	34.414	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	68.820%
24) Chloroform-d	4.346	84	116453	4.268	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%
26) 1,2-Dichloroethane-d4	5.030	65	55627	4.552	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	5.047	84	223795	4.448	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.066	67	63689	4.093	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.800%
41) Toluene-d8	7.313	98	179196	4.113	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	7.622	79	19159	3.997	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.088	63	67562	37.477	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37609	3.756	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	57087	4.861	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.200%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	3874	0.294	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027714.D
Acq On : 02 Sep 2022 11:10
Operator : SY/MD
Sample : N4370-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Sep 03 04:16:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 03:03:49 2022
Response via : Initial Calibration

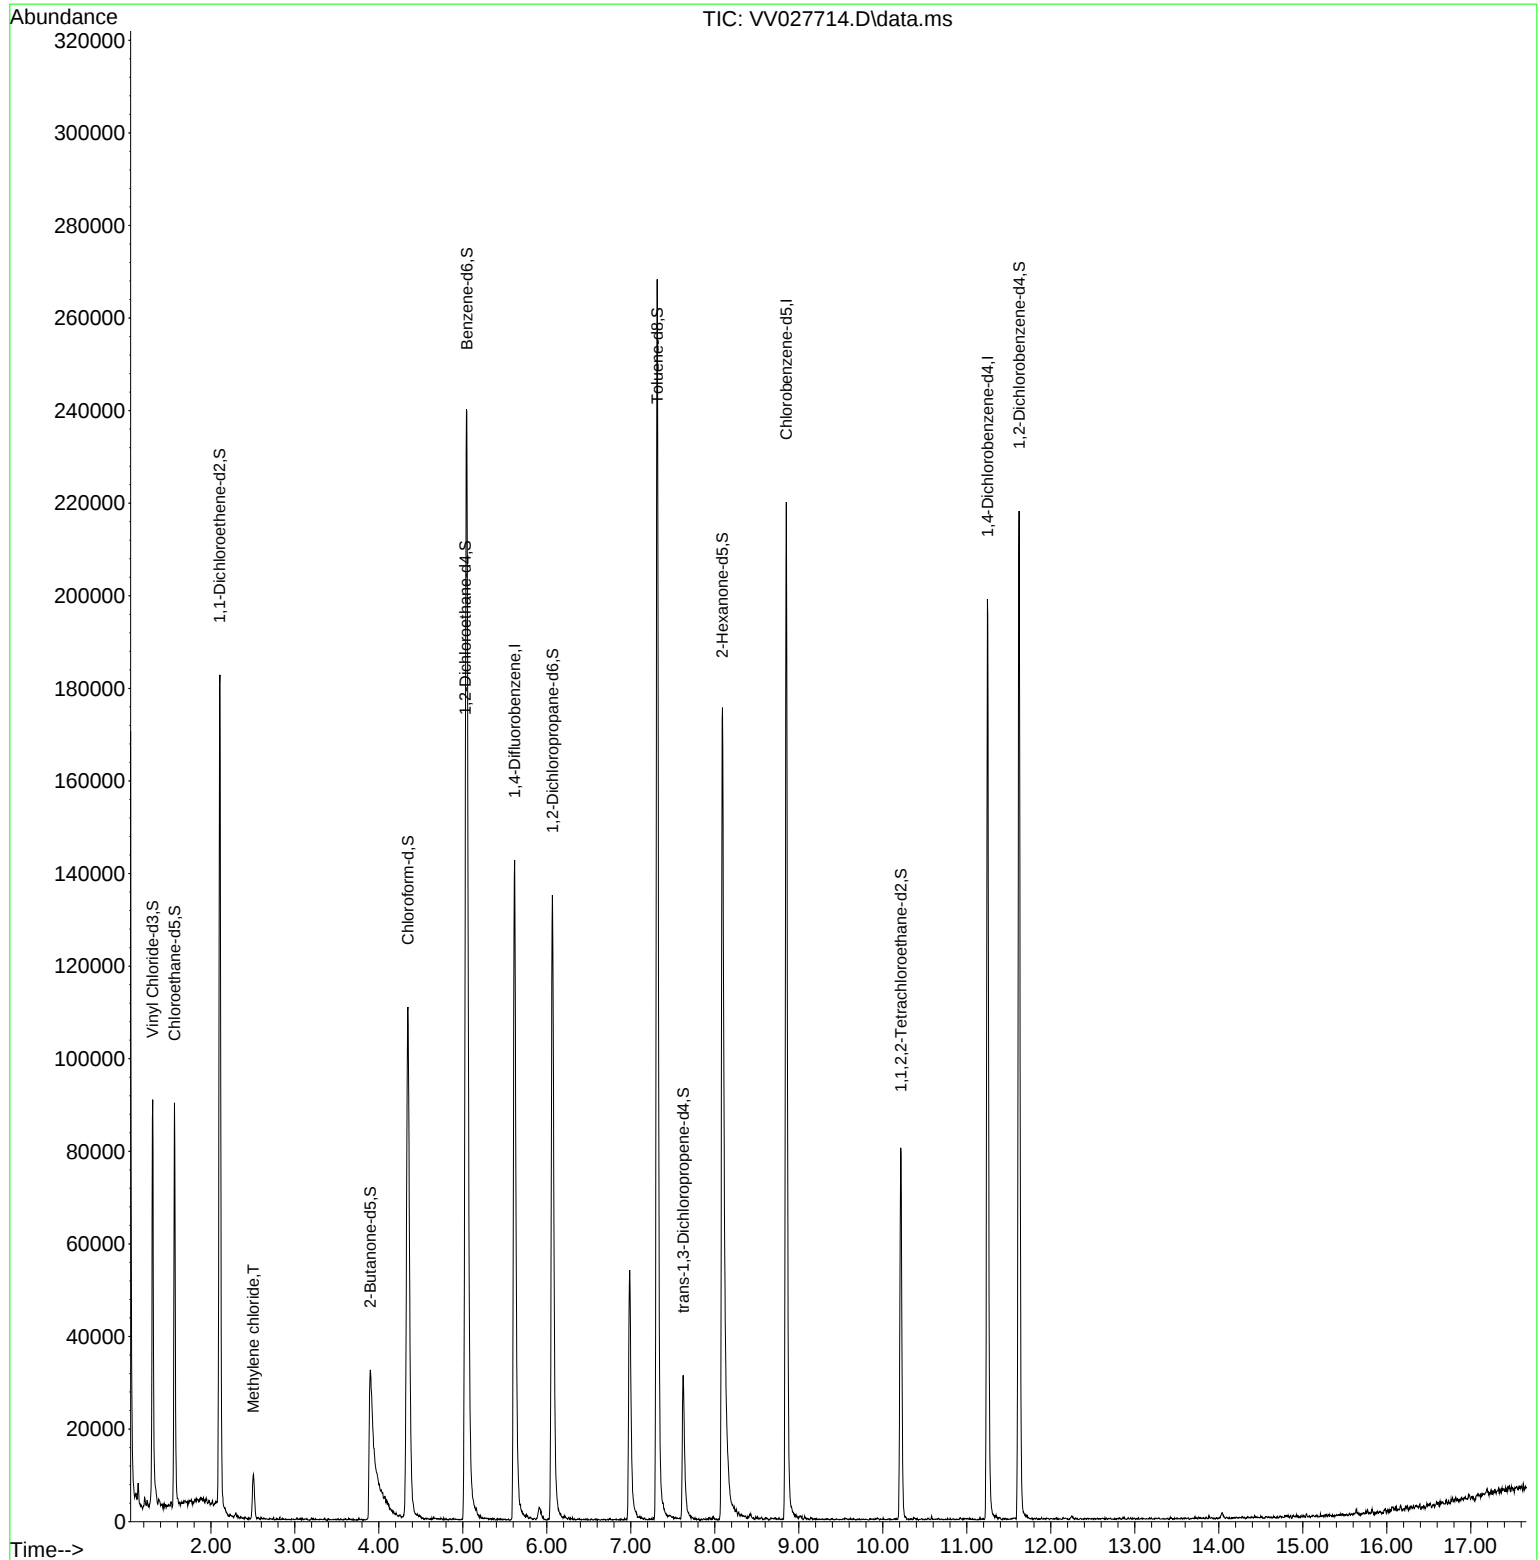

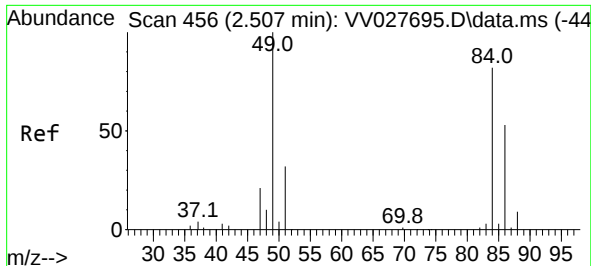

#16
Methylene chloride
Concen: 0.294 ug/L
RT: 2.503 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV027714.D
Acq: 02 Sep 2022 11:10

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

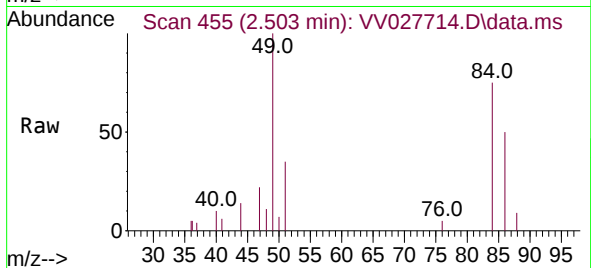

Tgt Ion: 84 Resp: 3874

Ion	Ratio	Lower	Upper
84	100		
86	67.2	43.9	81.5
49	134.1	92.5	171.7

