

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027715.D
 Acq On : 02 Sep 2022 11:33
 Operator : SY/MD
 Sample : N4366-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 03 04:17:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 03:03:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	127997	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	123535	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54979	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61518	4.424	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.400%
7) Chloroethane-d5	1.568	69	51059	4.389	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.108	63	94625	3.477	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.600%
20) 2-Butanone-d5	3.896	46	55961	23.803	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	47.600%
24) Chloroform-d	4.346	84	115377	4.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
26) 1,2-Dichloroethane-d4	5.031	65	54171	4.332	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
32) Benzene-d6	5.050	84	215445	4.258	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.200%
36) 1,2-Dichloropropane-d6	6.069	67	62974	4.023	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.400%
41) Toluene-d8	7.314	98	176008	4.016	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.400%
43) trans-1,3-Dichloroprop...	7.625	79	19481	4.040	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%
46) 2-Hexanone-d5	8.092	63	67933	37.465	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.920%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37780	3.751	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	55414	4.502	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.000%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	3417	0.254	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027715.D
Acq On : 02 Sep 2022 11:33
Operator : SY/MD
Sample : N4366-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 03 04:17:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 03:03:49 2022
Response via : Initial Calibration

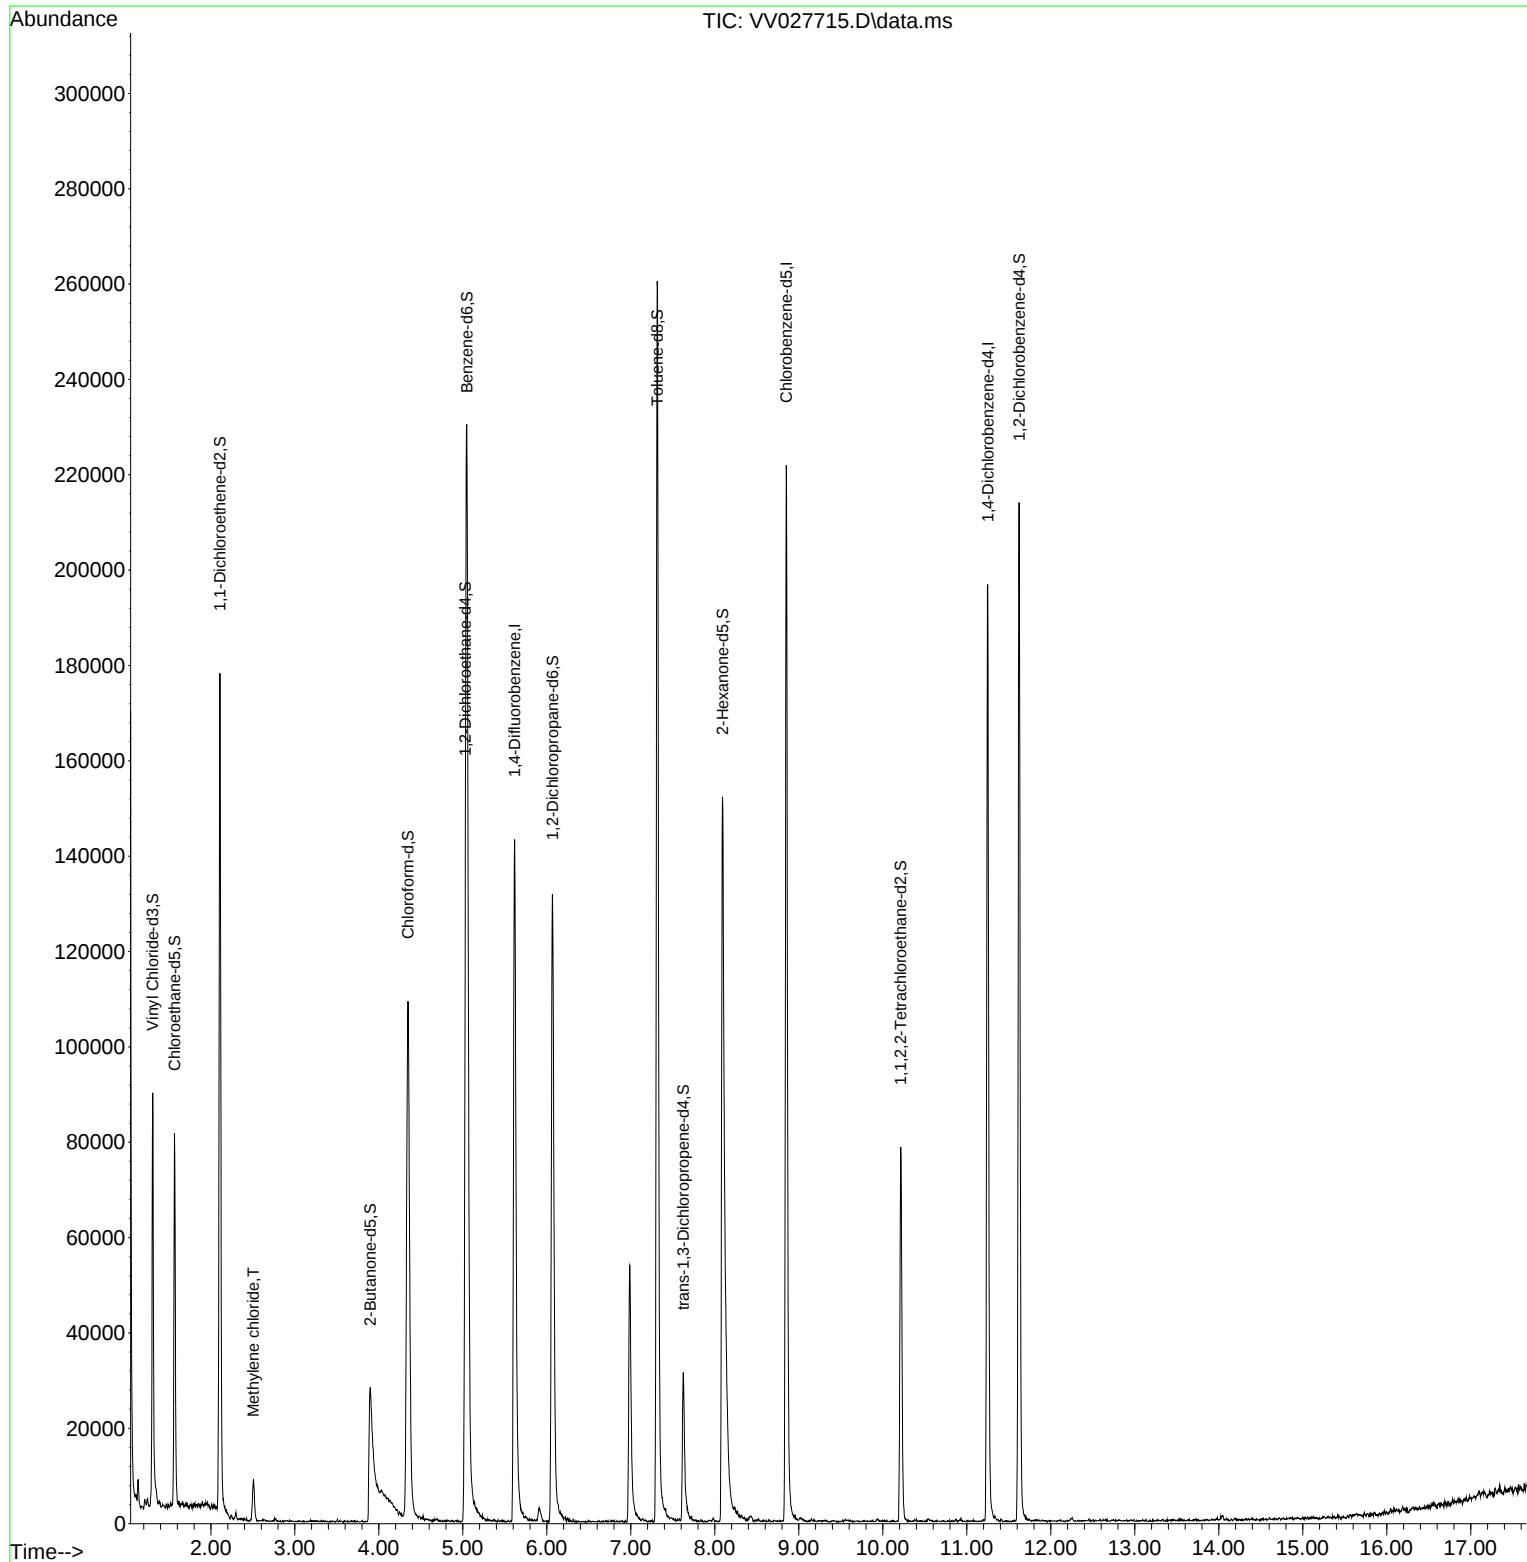

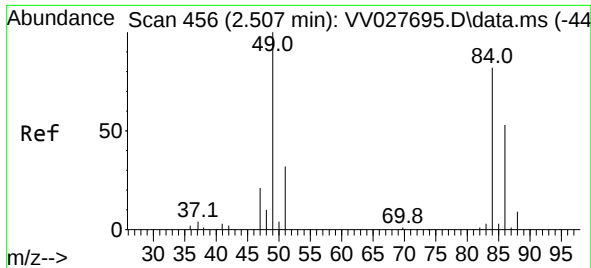

#16

Methylene chloride

Concen: 0.254 ug/L

RT: 2.507 min Scan# 4

Delta R.T. 0.000 min

Lab File: VV027715.D


Acq: 02 Sep 2022 11:33

Instrument :

MSVOA_V

ClientSampleId :

VHBLK001

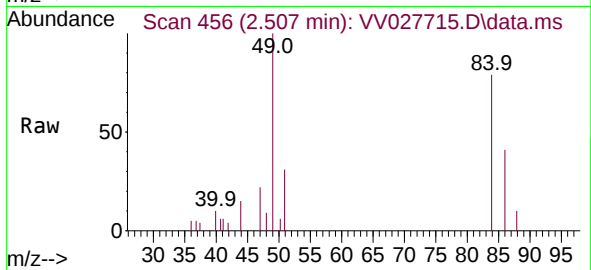

Tgt Ion: 84 Resp: 3417

Ion Ratio Lower Upper

84 100

86 52.0 43.9 81.5

49 126.0 92.5 171.7

