

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027717.D
 Acq On : 02 Sep 2022 12:22
 Operator : SY/MD
 Sample : N4396-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 03 04:17:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 02 03:03:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	117155	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	112052	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49257	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	63713	5.006	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5	1.568	69	52300	4.912	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.200%	
11) 1,1-Dichloroethene-d2	2.105	63	97611	3.919	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.400%	
20) 2-Butanone-d5	3.902	46	58690	27.274	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	54.540%	
24) Chloroform-d	4.346	84	117726	4.608	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
26) 1,2-Dichloroethane-d4	5.031	65	56327	4.921	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.400%	
32) Benzene-d6	5.047	84	225422	4.911	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.200%	
36) 1,2-Dichloropropane-d6	6.066	67	66314	4.671	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.400%	
41) Toluene-d8	7.313	98	184266	4.636	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.625	79	21135	4.832	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.600%	
46) 2-Hexanone-d5	8.088	63	69829	42.457	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.920%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40154	4.395	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	57522	5.216	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	4561	0.370	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027717.D
Acq On : 02 Sep 2022 12:22
Operator : SY/MD
Sample : N4396-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 03 04:17:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 02 03:03:49 2022
Response via : Initial Calibration

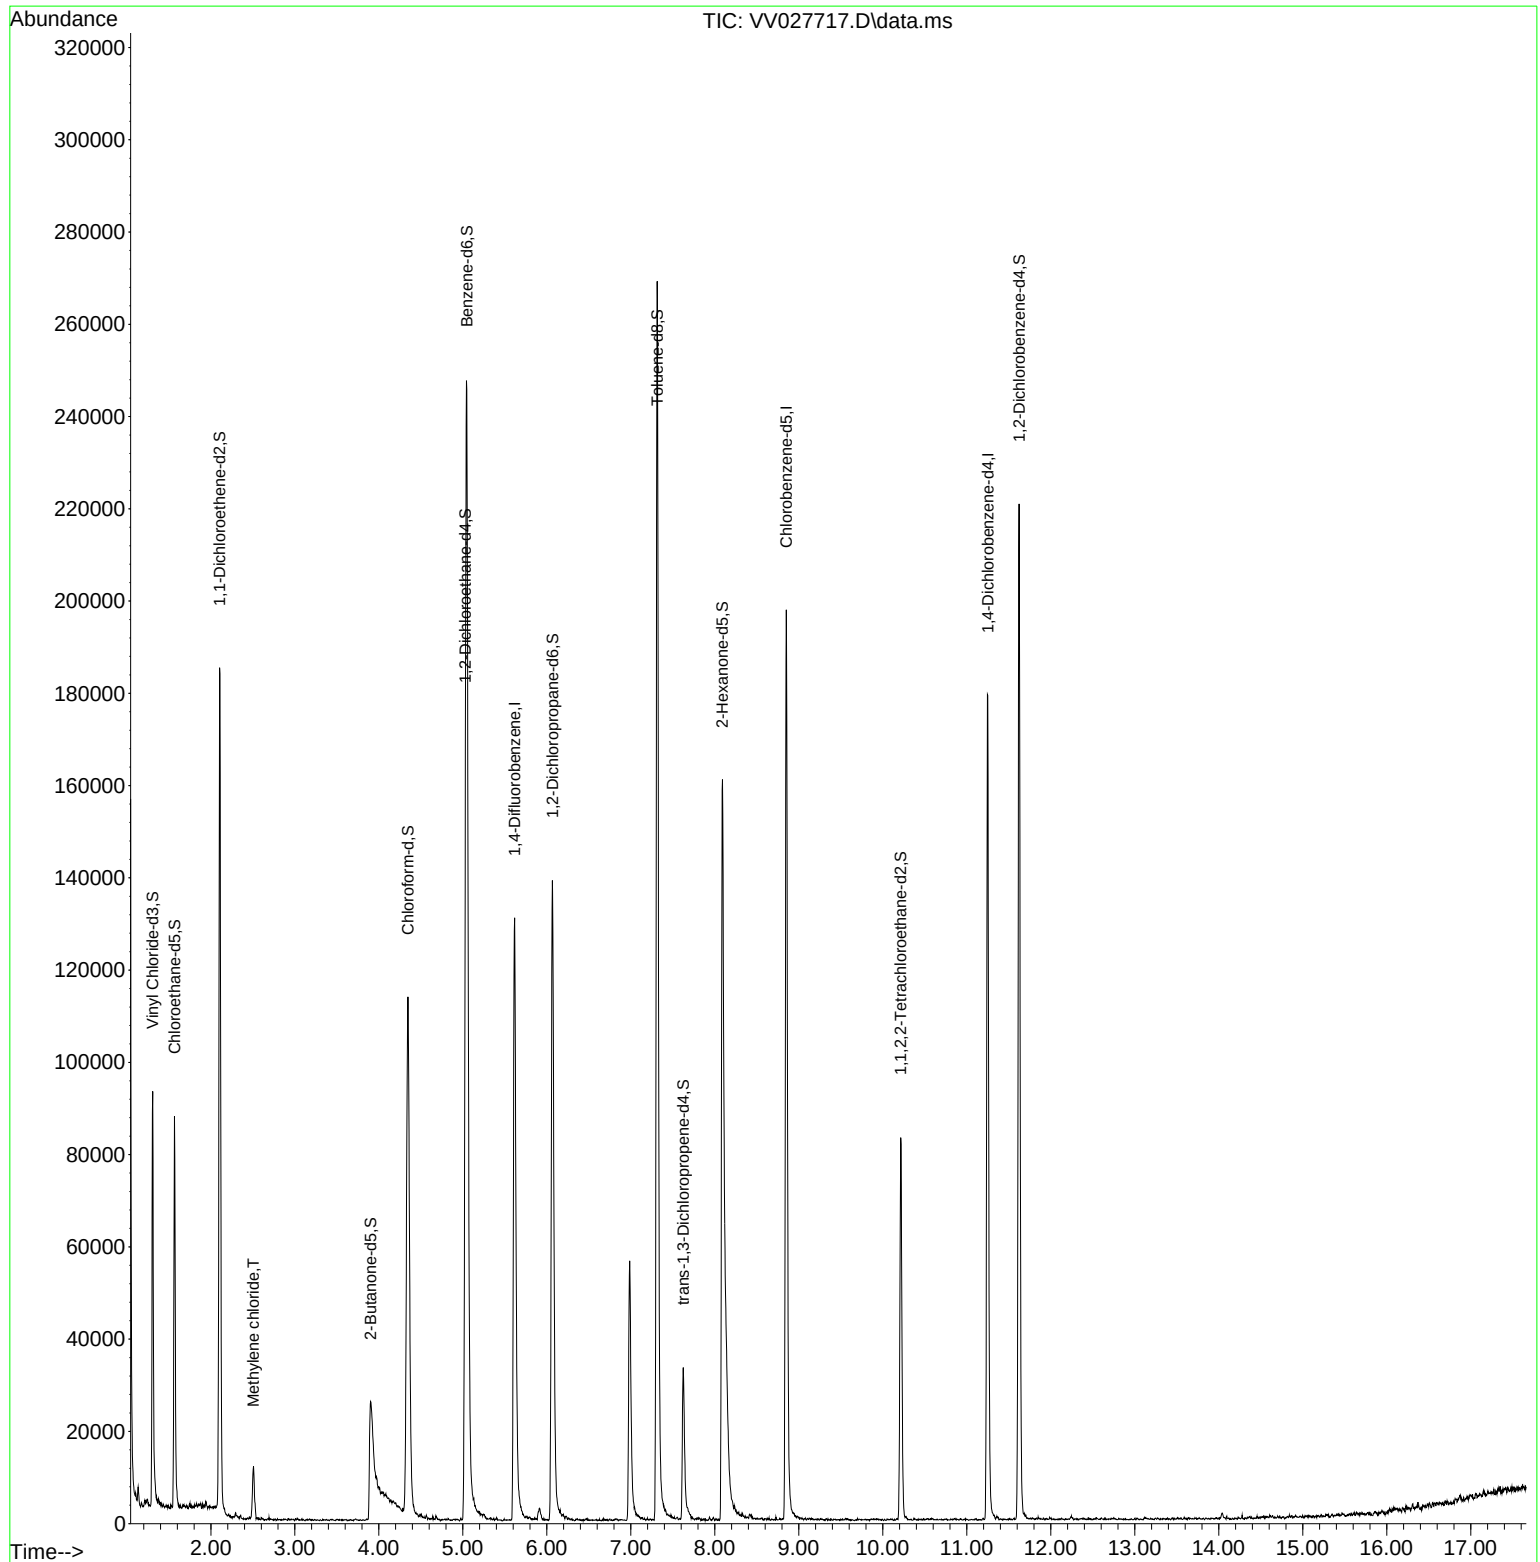

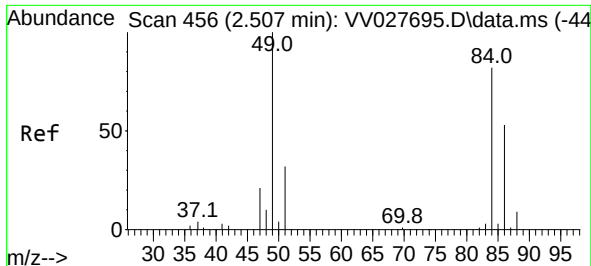

#16
Methylene chloride
Concen: 0.370 ug/L
RT: 2.503 min Scan# 455
Delta R.T. -0.003 min
Lab File: VV027717.D
Acq: 02 Sep 2022 12:22

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4561
Ion Ratio Lower Upper
84 100
86 56.8 43.9 81.5
49 123.9 92.5 171.7

