

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027725.D
 Acq On : 02 Sep 2022 16:11
 Operator : SY/MD
 Sample : N4404-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVF5

Quant Time: Sep 03 05:33:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 03 05:30:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	126525	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	122693	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53981	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59585	4.335	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.600%
7) Chloroethane-d5	1.568	69	56104	4.879	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.600%
11) 1,1-Dichloroethene-d2	2.108	63	95763	3.560	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.200%
20) 2-Butanone-d5	3.896	46	74856	32.211	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	64.420%
24) Chloroform-d	4.346	84	122623	4.444	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	5.031	65	59178	4.787	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
32) Benzene-d6	5.047	84	227509	4.527	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.066	67	68230	4.389	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.800%
41) Toluene-d8	7.313	98	181203	4.163	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.200%
43) trans-1,3-Dichloroprop...	7.625	79	20133	4.204	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.088	63	82117	45.598	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.200%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41872	4.186	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	63579	5.261	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds					Qvalue	
13) Acetone	2.175	43	7070	4.496	ug/L	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027725.D
Acq On : 02 Sep 2022 16:11
Operator : SY/MD
Sample : N4404-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF5

Quant Time: Sep 03 05:33:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 03 05:30:57 2022
Response via : Initial Calibration

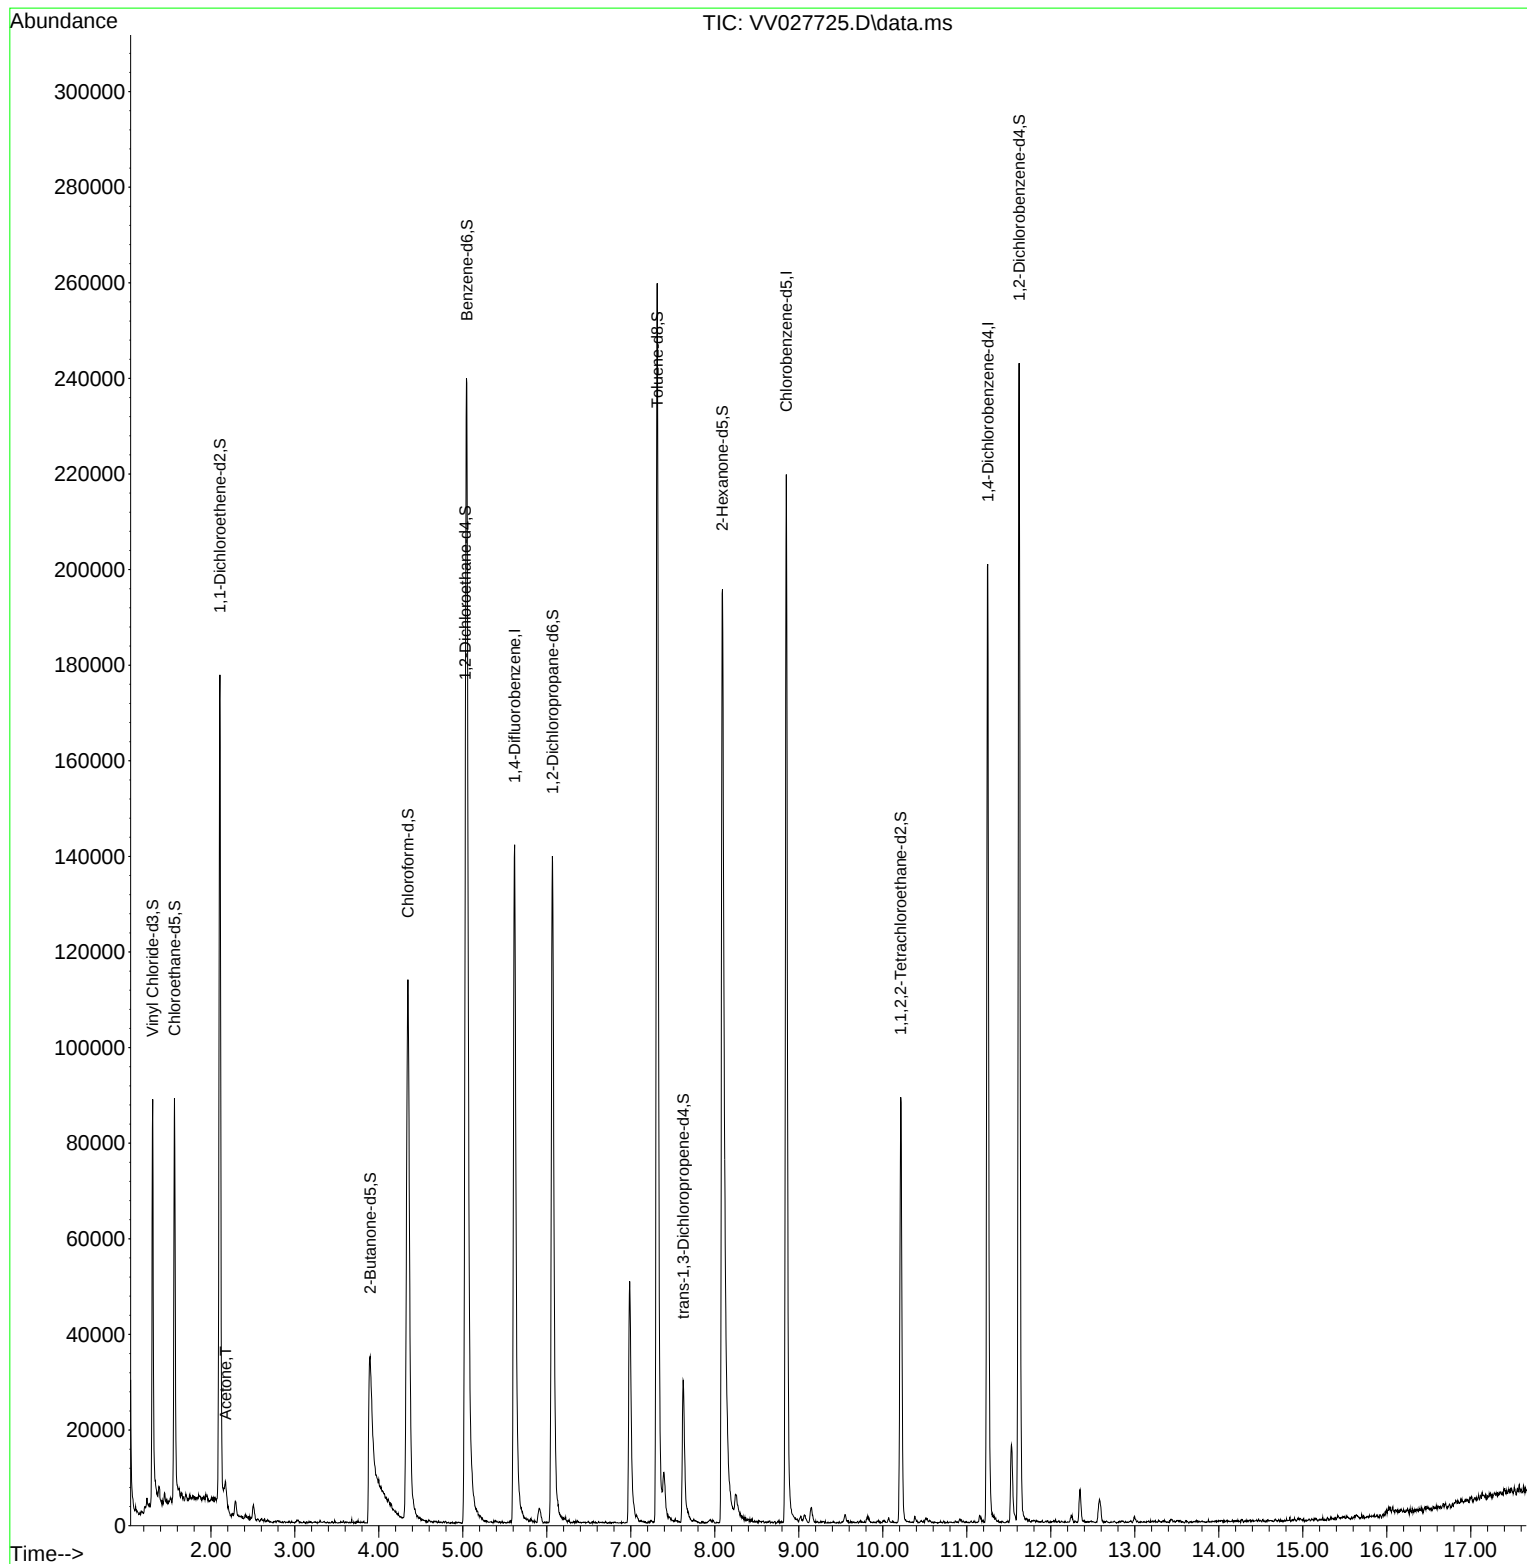

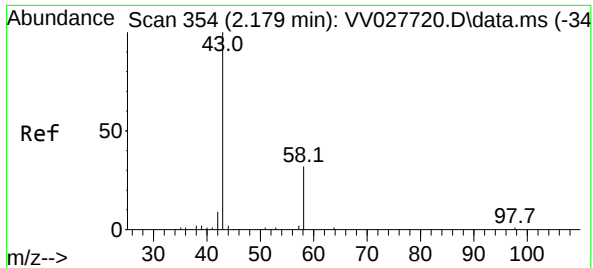

#13
 Acetone
 Concen: 4.496 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV027725.D
 Acq: 02 Sep 2022 16:11

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVF5

Tgt Ion: 43 Resp: 7070
 Ion Ratio Lower Upper
 43 100
 58 38.0 0.0 38.4

