

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027727.D
 Acq On : 02 Sep 2022 17:00
 Operator : SY/MD
 Sample : N4404-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVD6

Quant Time: Sep 03 05:34:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 03 05:30:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	122017	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	118001	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52432	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	0.000	65	0d	0.000	ug/L	
Spiked Amount	5.000	Range	40 - 130	Recovery	=	0.000%#
7) Chloroethane-d5	1.565	69	55176	4.975	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.600%
11) 1,1-Dichloroethene-d2	2.101	63	63551	2.450	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.000%#
20) 2-Butanone-d5	3.896	46	78690	35.111	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	70.220%
24) Chloroform-d	4.343	84	120648	4.534	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
26) 1,2-Dichloroethane-d4	5.027	65	59468	4.989	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	5.043	84	218779	4.526	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.066	67	65445	4.377	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%
41) Toluene-d8	7.313	98	141634	3.384	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.600%#
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount	5.000	Range	55 - 130	Recovery	=	0.000%#
46) 2-Hexanone-d5	8.088	63	81655	47.144	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.280%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	39974	4.155	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	61342	5.226	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.600%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.973	164	16981	1.851	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027727.D
Acq On : 02 Sep 2022 17:00
Operator : SY/MD
Sample : N4404-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVD6

Quant Time: Sep 03 05:34:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 03 05:30:57 2022
Response via : Initial Calibration

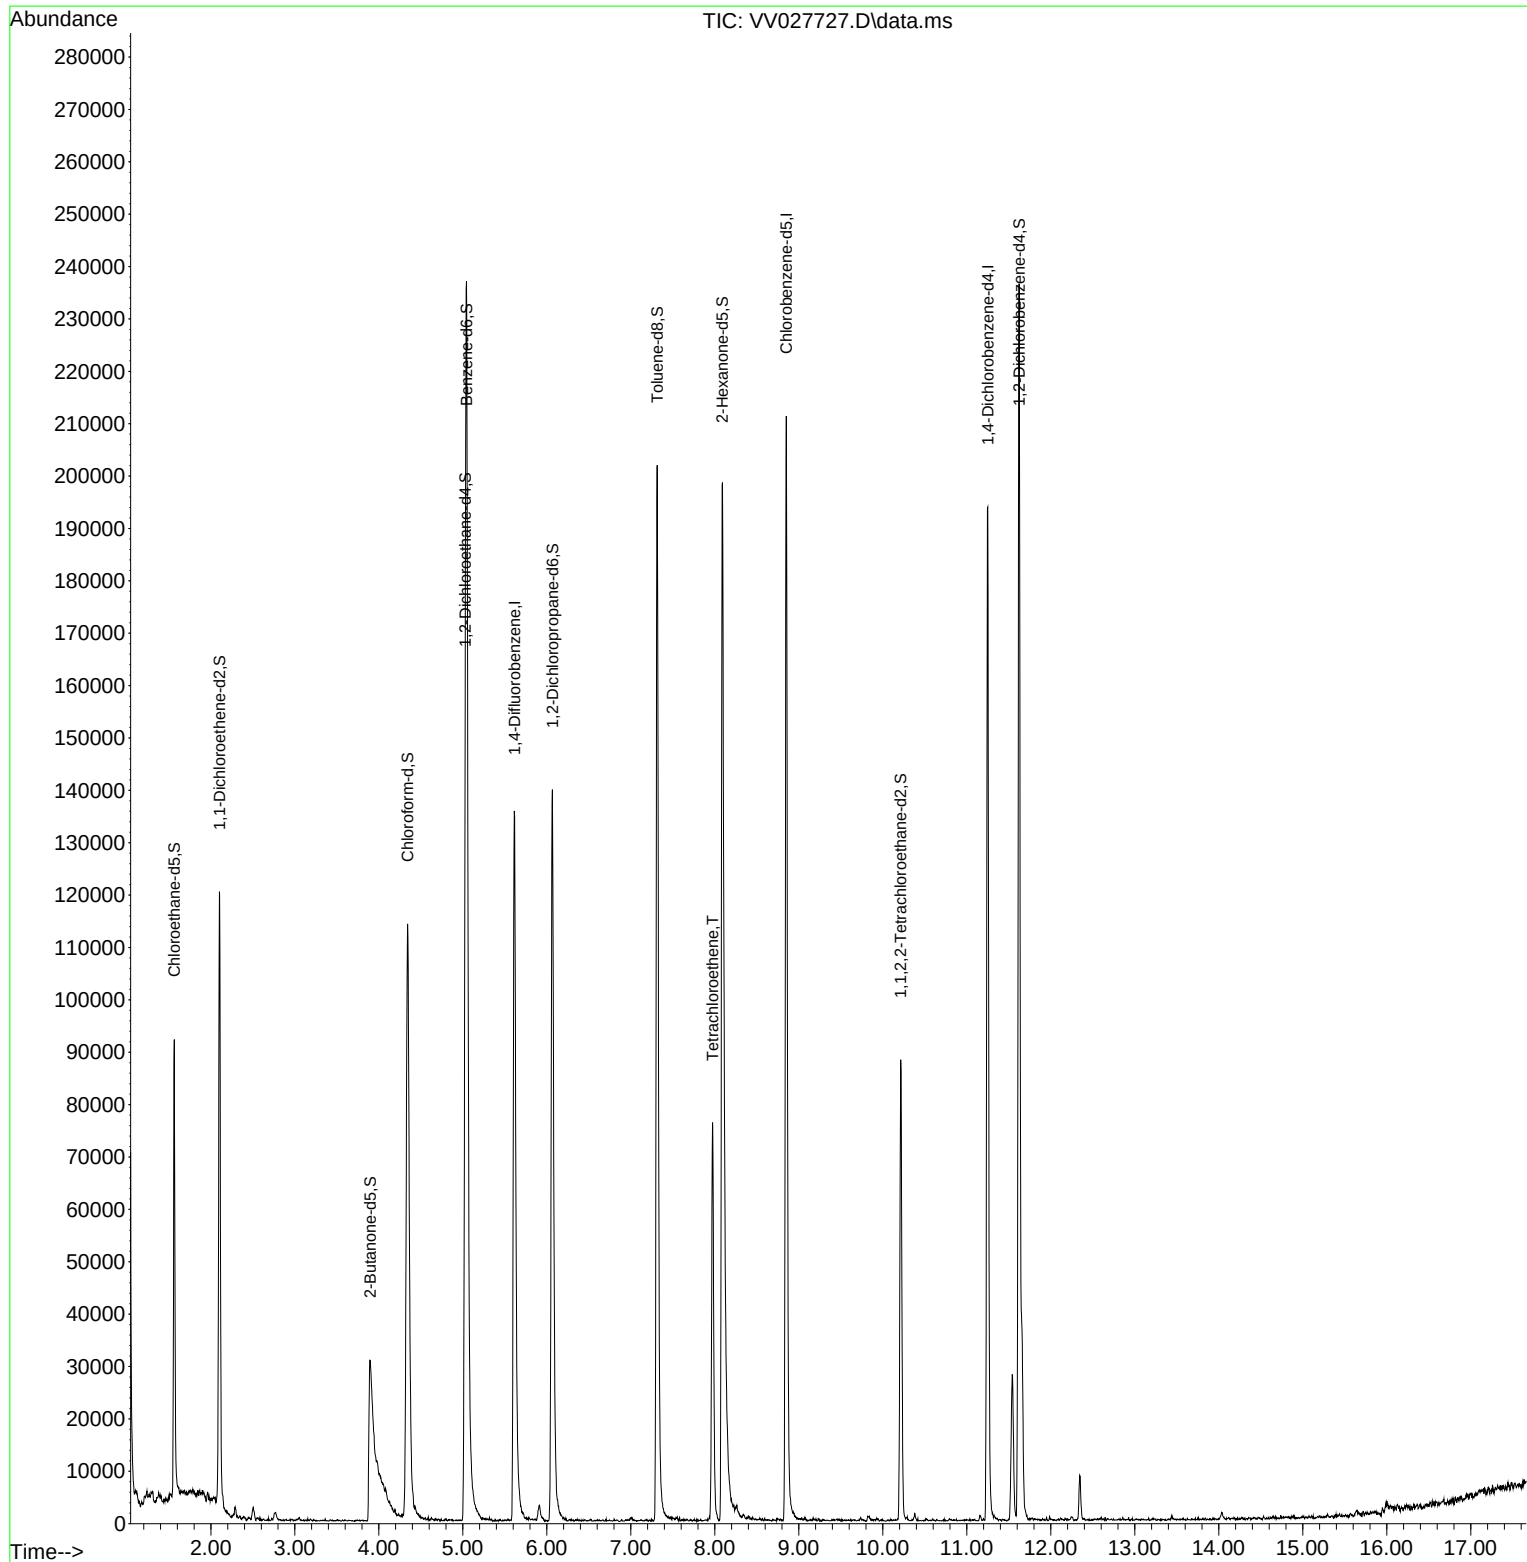

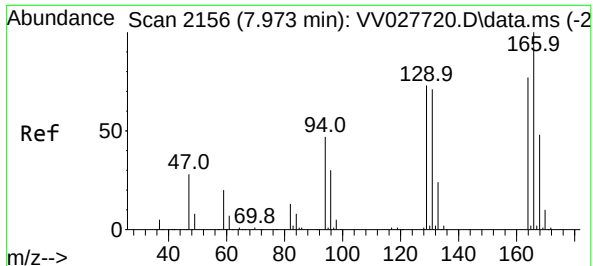

#47
 Tetrachloroethene
 Concen: 1.851 ug/L
 RT: 7.973 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV027727.D
 Acq: 02 Sep 2022 17:00

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVD6

Tgt Ion:	164	Resp:	16981
Ion	Ratio	Lower	Upper
164	100		
129	100.6	65.9	122.3
131	95.7	64.5	119.7
166	131.2	88.8	165.0

