

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027729.D
 Acq On : 02 Sep 2022 17:49
 Operator : SY/MD
 Sample : N4404-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 03 05:34:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 03 05:30:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	116205	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	114095	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49656	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	64709	5.126	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.600%	
7) Chloroethane-d5	1.568	69	53359	5.052	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.000%	
11) 1,1-Dichloroethene-d2	2.108	63	99167	4.014	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.200%	
20) 2-Butanone-d5	3.892	46	62509	29.286	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	58.580%	
24) Chloroform-d	4.346	84	109200	4.309	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.200%	
26) 1,2-Dichloroethane-d4	5.030	65	52966	4.665	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.400%	
32) Benzene-d6	5.047	84	206680	4.422	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.400%	
36) 1,2-Dichloropropane-d6	6.066	67	60644	4.195	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	84.000%	
41) Toluene-d8	7.313	98	170247	4.206	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.200%	
43) trans-1,3-Dichloroprop...	7.622	79	19225	4.317	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.400%	
46) 2-Hexanone-d5	8.088	63	69746	41.647	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.300%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	36592	3.934	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	78.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	54908	4.939	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	7130	0.583	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027729.D
Acq On : 02 Sep 2022 17:49
Operator : SY/MD
Sample : N4404-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Sep 03 05:34:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 03 05:30:57 2022
Response via : Initial Calibration

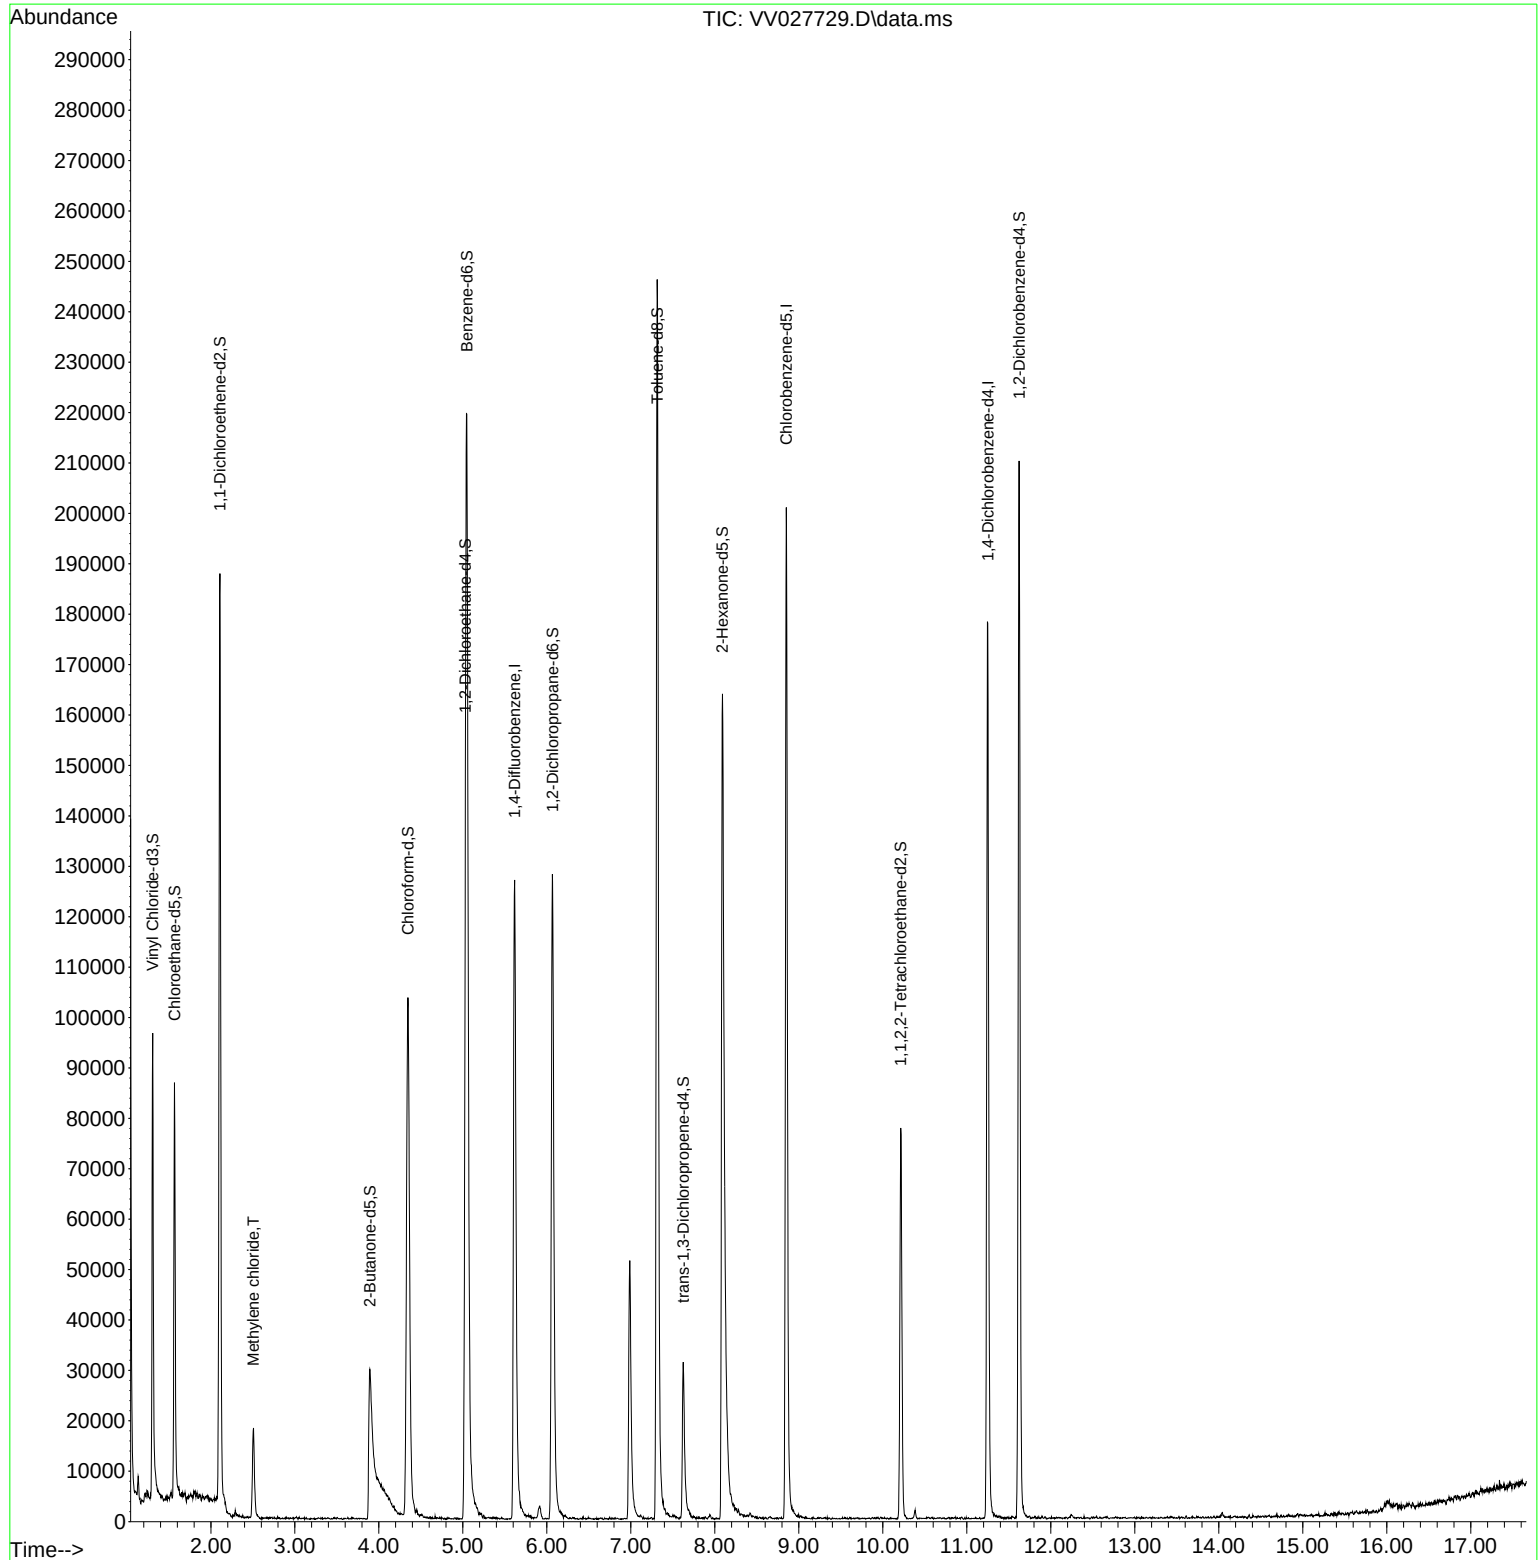

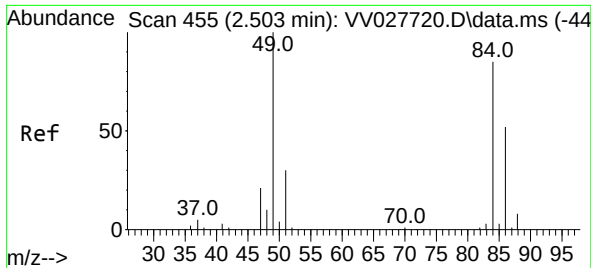

#16
Methylene chloride
Concen: 0.583 ug/L
RT: 2.506 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV027729.D
Acq: 02 Sep 2022 17:49

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

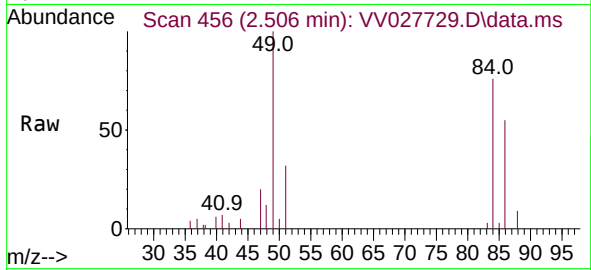

Tgt Ion:	84	Resp:	7130
Ion	Ratio	Lower	Upper
84	100		
86	71.6	43.9	81.5
49	130.8	92.5	171.7

