

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027677.D
 Acq On : 01 Sep 2022 19:23
 Operator : SY/MD
 Sample : N4366-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	99	rBV	85681	95903	15.39%	2.117%
2	1.568	156	164	174	rBV	85840	98303	15.78%	2.170%
3	2.105	321	331	344	rBV	166700	245400	39.38%	5.416%
4	3.889	874	886	910	rBV2	33619	119455	19.17%	2.637%
5	4.346	1010	1028	1052	rBV	118324	325693	52.27%	7.189%
6	5.043	1228	1245	1271	rBV2	235624	623152	100.00%	13.754%
7	5.616	1407	1423	1449	rBV	132453	288373	46.28%	6.365%
8	5.915	1500	1516	1533	rBV	7170	18003	2.89%	0.397%
9	6.066	1549	1563	1592	rBV	145886	314510	50.47%	6.942%
10	6.513	1695	1702	1715	rVB6	4178	7244	1.16%	0.160%
11	6.985	1839	1849	1879	rBV	54659	114446	18.37%	2.526%
12	7.313	1939	1951	1971	rBV	251013	461312	74.03%	10.182%
13	7.622	2037	2047	2067	rBV2	32089	63387	10.17%	1.399%
14	7.976	2147	2157	2171	rVB3	36772	64136	10.29%	1.416%
15	8.091	2180	2193	2221	rBV2	187656	494504	79.36%	10.915%
16	8.850	2417	2429	2457	rBV	216566	370532	59.46%	8.178%
17	10.214	2842	2853	2866	rBV	94142	150349	24.13%	3.319%
18	11.249	3163	3175	3198	rBV	183791	296220	47.54%	6.538%
19	11.622	3279	3291	3311	rBV	218016	350912	56.31%	7.745%
20	15.924	4605	4629	4630	rBV	12776	28774	4.62%	0.635%




Sum of corrected areas: 4530608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027677.D
Acq On : 01 Sep 2022 19:23
Operator : SY/MD
Sample : N4366-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

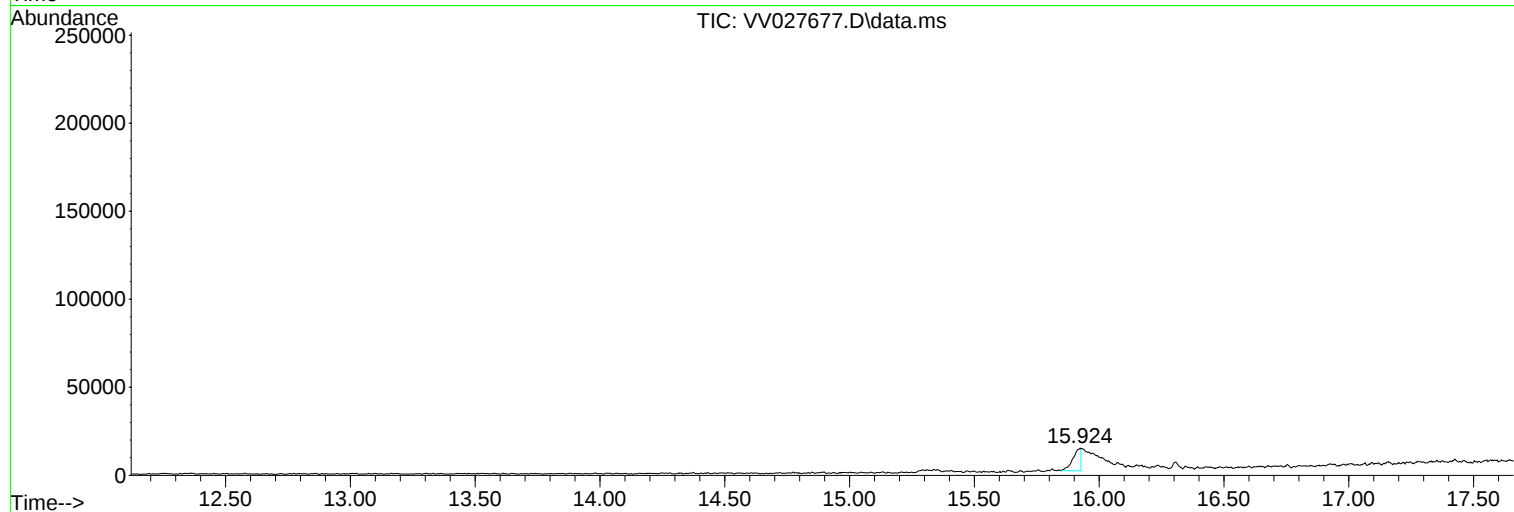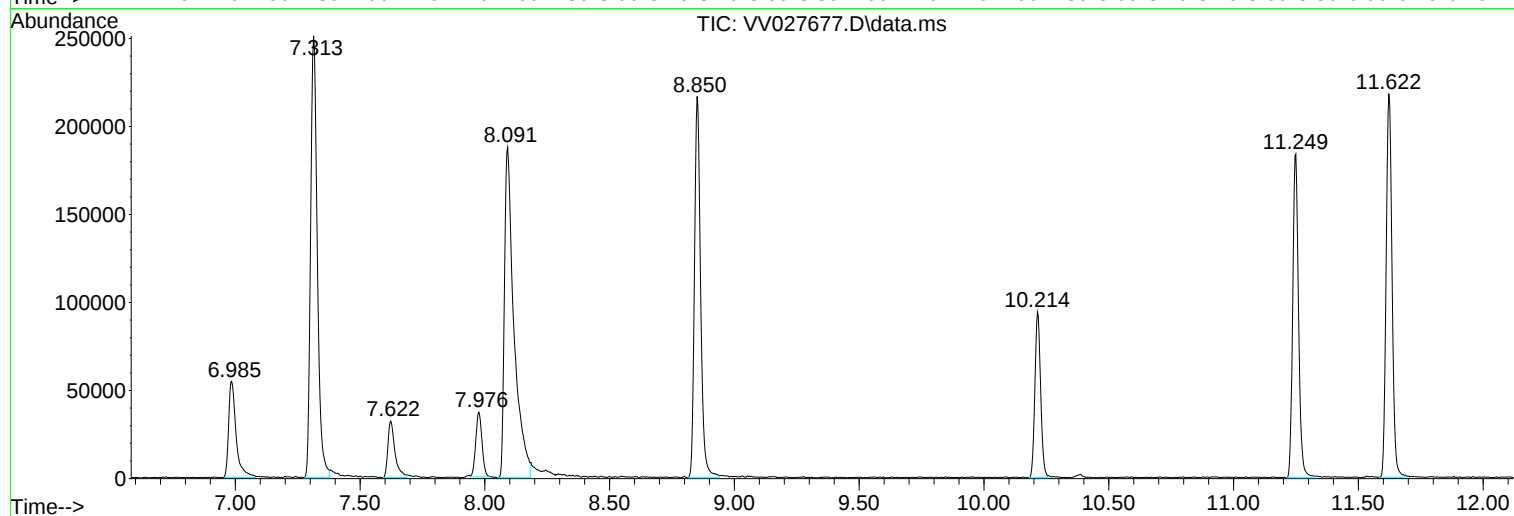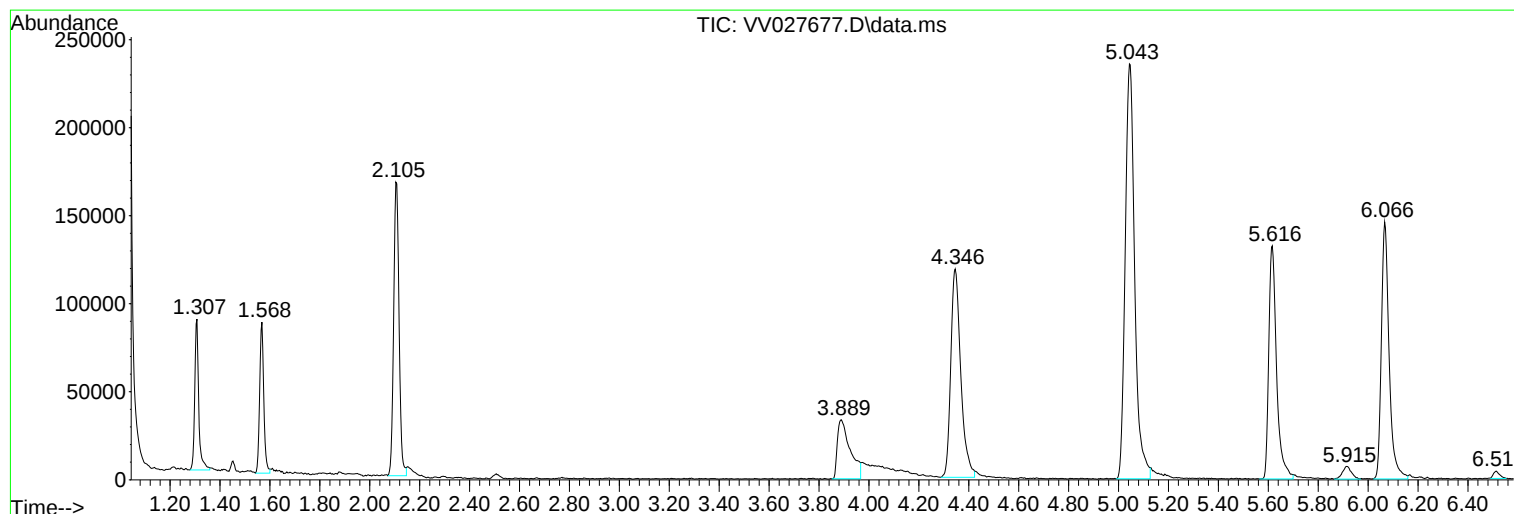

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027677.D
Acq On : 01 Sep 2022 19:23
Operator : SY/MD
Sample : N4366-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027677.D
Acq On : 01 Sep 2022 19:23
Operator : SY/MD
Sample : N4366-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc