

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027678.D
 Acq On : 01 Sep 2022 19:48
 Operator : SY/MD
 Sample : N4366-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rBV	81644	95614	14.72%	2.009%
2	1.568	155	164	175	rBV	81144	99291	15.29%	2.086%
3	2.105	317	331	341	rBV	173272	247957	38.18%	5.209%
4	3.896	877	888	910	rBV	35367	127807	19.68%	2.685%
5	4.346	1011	1028	1063	rBV2	117176	308879	47.56%	6.489%
6	5.043	1228	1245	1277	rBV2	247811	649429	100.00%	13.642%
7	5.616	1411	1423	1446	rBV	140774	304907	46.95%	6.405%
8	5.915	1503	1516	1532	rBV5	21464	50261	7.74%	1.056%
9	6.066	1550	1563	1590	rBV	148851	322117	49.60%	6.767%
10	6.986	1838	1849	1872	rBV2	55964	113340	17.45%	2.381%
11	7.313	1939	1951	1974	rBV	261317	477576	73.54%	10.032%
12	7.622	2036	2047	2070	rBV	34607	67995	10.47%	1.428%
13	7.976	2145	2157	2172	rVB2	64980	112602	17.34%	2.365%
14	8.092	2181	2193	2233	rBV2	192441	526493	81.07%	11.060%
15	8.850	2416	2429	2454	rBV	229174	389216	59.93%	8.176%
16	10.214	2842	2853	2874	rBV	96342	155620	23.96%	3.269%
17	11.246	3162	3174	3196	rBV	201719	323696	49.84%	6.800%
18	11.622	3278	3291	3311	rBV	227767	366204	56.39%	7.693%
19	15.914	4612	4626	4628	rBV10	11493	21346	3.29%	0.448%




Sum of corrected areas: 4760350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027678.D
Acq On : 01 Sep 2022 19:48
Operator : SY/MD
Sample : N4366-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

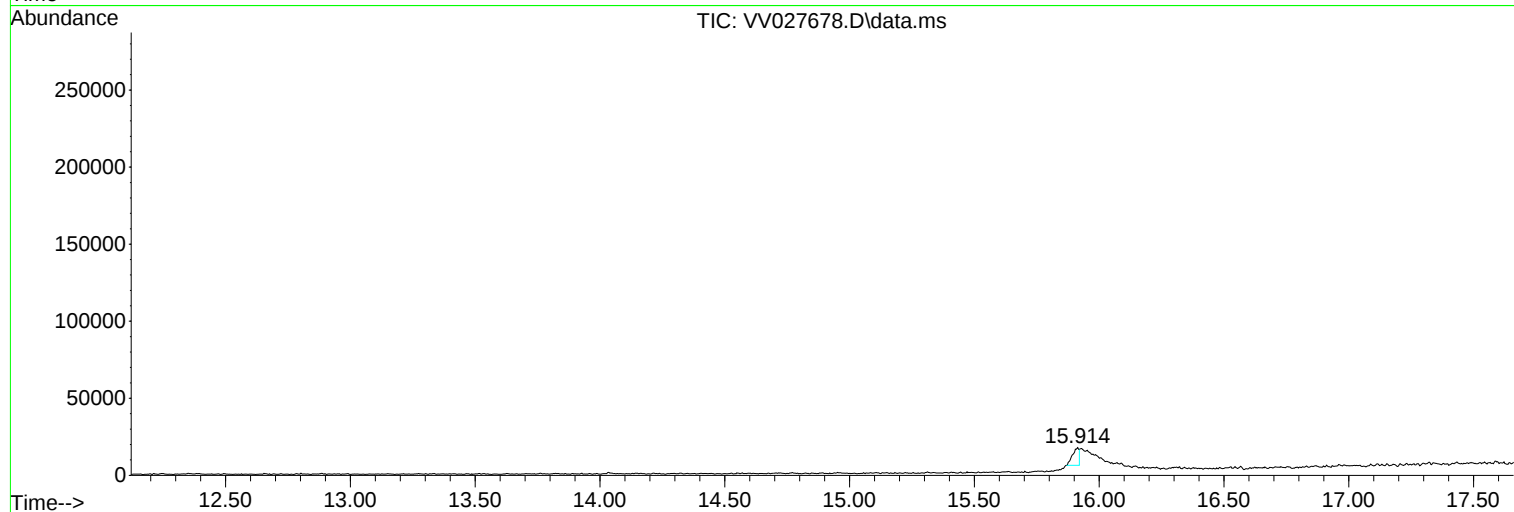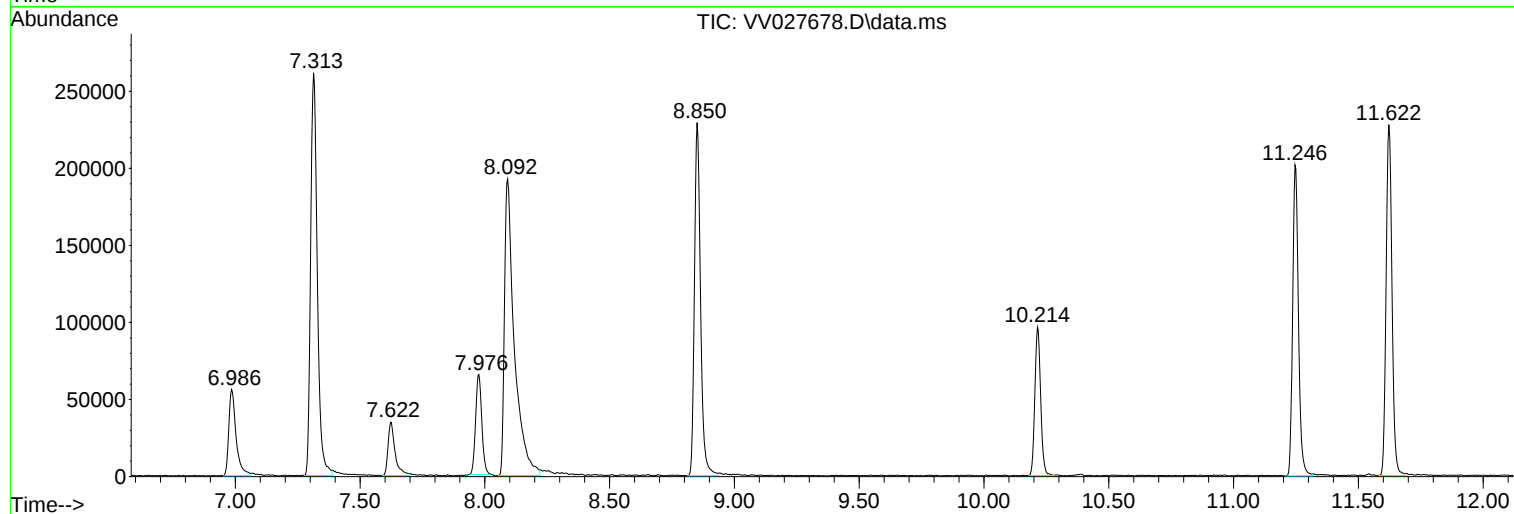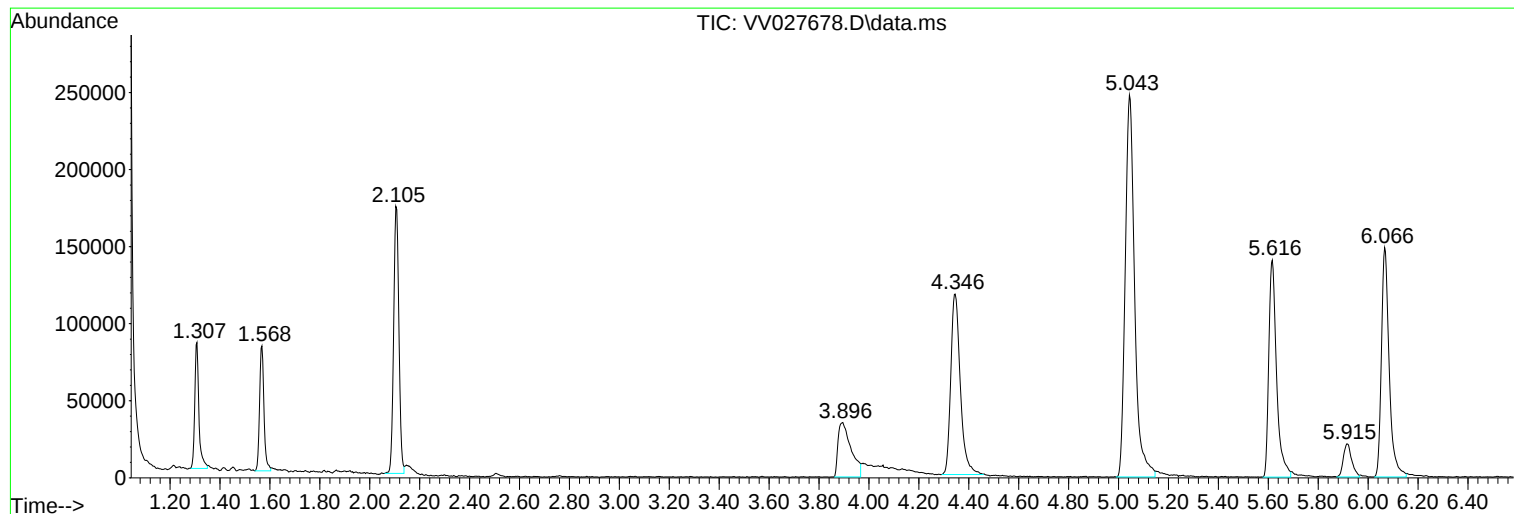

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027678.D
Acq On : 01 Sep 2022 19:48
Operator : SY/MD
Sample : N4366-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027678.D
Acq On : 01 Sep 2022 19:48
Operator : SY/MD
Sample : N4366-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc