

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027682.D
 Acq On : 01 Sep 2022 21:26
 Operator : SY/MD
 Sample : N4369-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F41

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	70	80	94	rBV	79868	92242	15.05%	2.004%
2	1.558	153	161	172	rBV	78262	90359	14.74%	1.964%
3	2.098	318	329	341	rBV	163078	231589	37.79%	5.033%
4	2.777	528	540	559	rVB3	23846	54176	8.84%	1.177%
5	3.966	893	910	934	rBV2	54188	195235	31.86%	4.243%
6	4.355	1013	1031	1049	rBV	116388	287654	46.93%	6.251%
7	5.034	1228	1242	1265	rBV2	281135	612881	100.00%	13.318%
8	5.597	1402	1417	1448	rVB	176270	371792	60.66%	8.079%
9	5.892	1496	1509	1523	rBV6	10457	23846	3.89%	0.518%
10	6.069	1550	1564	1590	rVB	146983	316022	51.56%	6.867%
11	6.641	1733	1742	1745	rBV3	4245	6687	1.09%	0.145%
12	7.011	1847	1857	1873	rBV2	56565	107272	17.50%	2.331%
13	7.336	1946	1958	1979	rBV	252698	448750	73.22%	9.752%
14	7.645	2043	2054	2067	rBV2	32999	60048	9.80%	1.305%
15	7.989	2150	2161	2183	rVB2	49101	87668	14.30%	1.905%
16	8.117	2189	2201	2238	rBV2	219752	464489	75.79%	10.094%
17	8.860	2421	2432	2461	rBV	218309	363821	59.36%	7.906%
18	10.220	2841	2855	2867	rBV	92514	145146	23.68%	3.154%
19	11.249	3165	3175	3195	rBV	187473	293707	47.92%	6.382%
20	11.625	3280	3292	3311	rBV	213079	340454	55.55%	7.398%
21	15.918	4616	4627	4628	rBV8	6003	8002	1.31%	0.174%




Sum of corrected areas: 4601840

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027682.D
Acq On : 01 Sep 2022 21:26
Operator : SY/MD
Sample : N4369-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

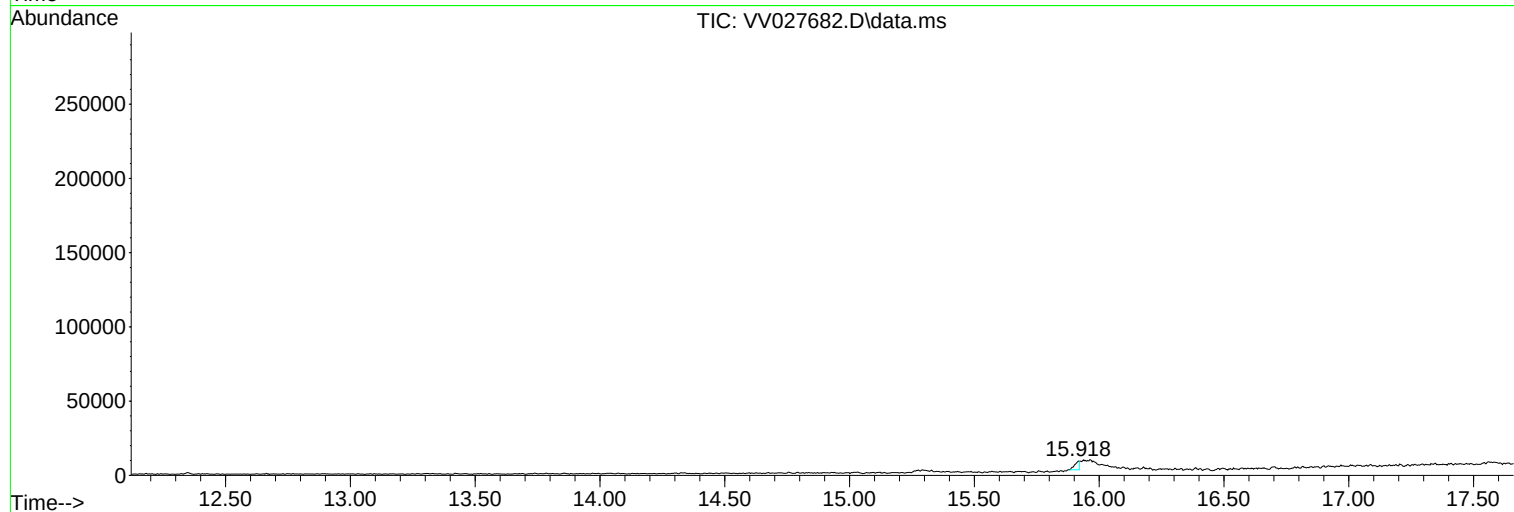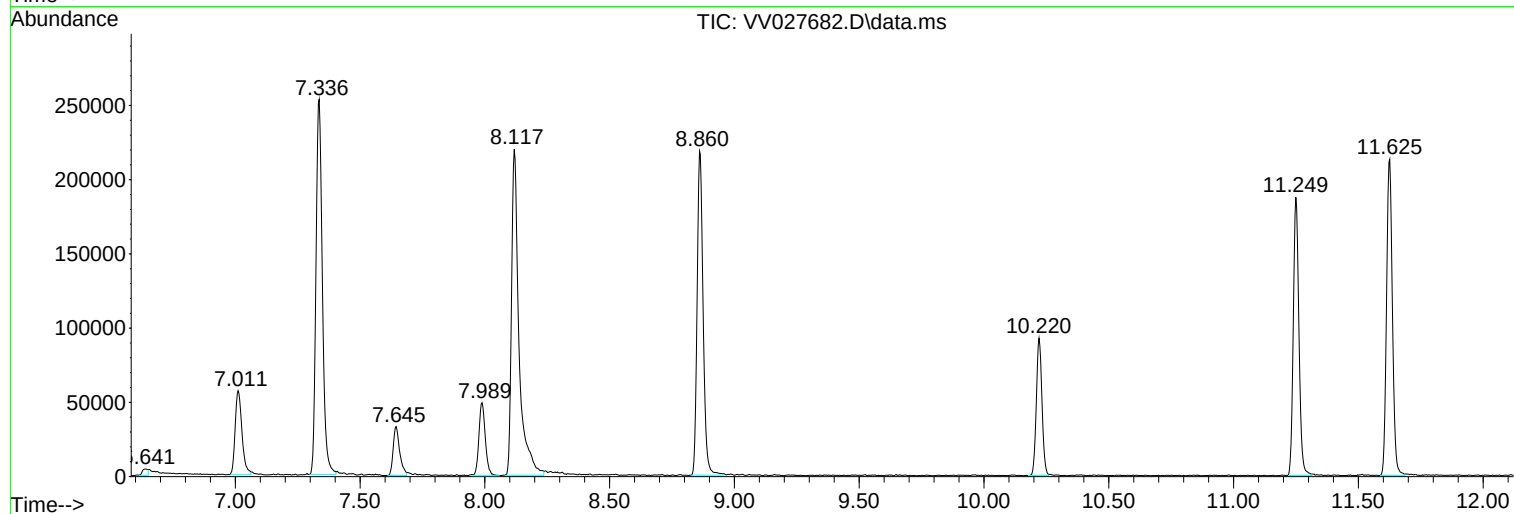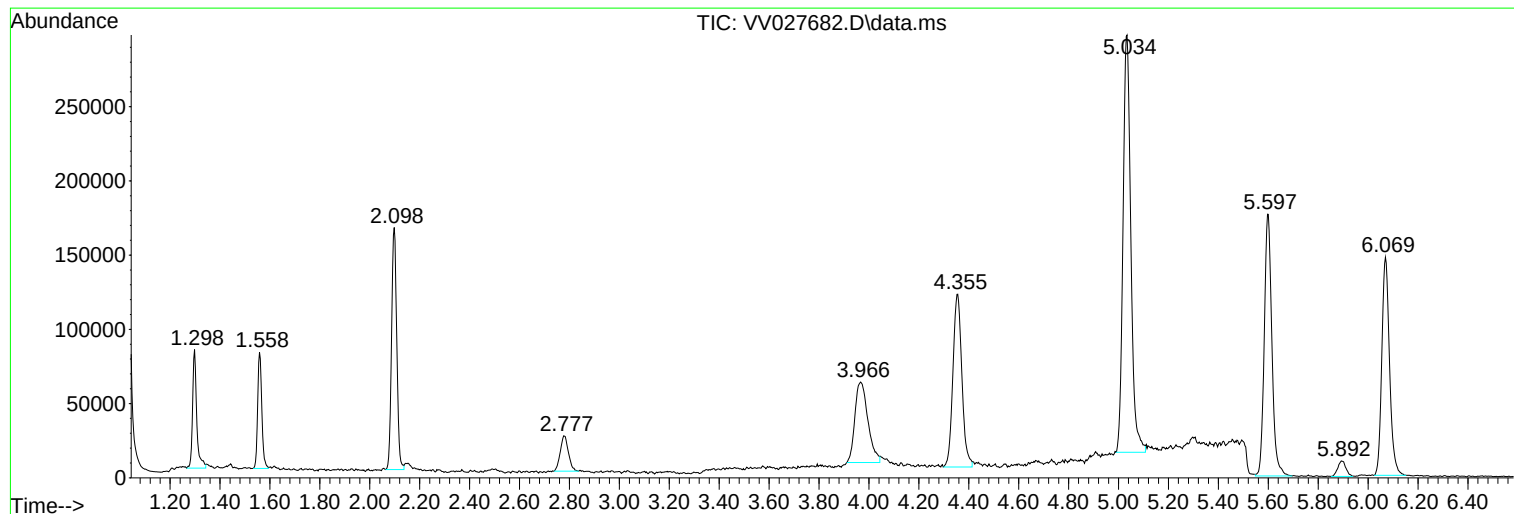

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027682.D
Acq On : 01 Sep 2022 21:26
Operator : SY/MD
Sample : N4369-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027682.D
Acq On : 01 Sep 2022 21:26
Operator : SY/MD
Sample : N4369-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc