

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027686.D
 Acq On : 01 Sep 2022 23:04
 Operator : SY/MD
 Sample : N4400-21DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	99	rBV	84149	99594	14.83%	1.985%
2	1.565	156	163	174	rBV	85263	97583	14.53%	1.945%
3	2.105	320	331	344	rBV	172608	252727	37.64%	5.037%
4	2.503	447	455	465	rBV5	4954	8171	1.22%	0.163%
5	3.892	873	887	917	rBV2	38118	152563	22.72%	3.041%
6	4.346	1012	1028	1052	rBV	122609	310133	46.19%	6.181%
7	5.043	1228	1245	1284	rBV2	253923	671484	100.00%	13.383%
8	5.616	1410	1423	1452	rBV	137302	296570	44.17%	5.911%
9	5.918	1504	1517	1540	rBV7	17178	42043	6.26%	0.838%
10	6.066	1551	1563	1587	rBV	148172	320924	47.79%	6.396%
11	6.986	1839	1849	1871	rBV	56838	113997	16.98%	2.272%
12	7.313	1940	1951	1973	rBV	265988	488108	72.69%	9.729%
13	7.622	2038	2047	2074	rBV2	33621	69377	10.33%	1.383%
14	7.973	2137	2156	2175	rBV2	233564	403046	60.02%	8.033%
15	8.092	2183	2193	2229	rBV	190354	505092	75.22%	10.067%
16	8.850	2419	2429	2447	rBV	215621	360694	53.72%	7.189%
17	10.214	2841	2853	2870	rBV2	92721	153435	22.85%	3.058%
18	11.249	3163	3175	3190	rBV	183163	292589	43.57%	5.832%
19	11.532	3253	3263	3276	rBV6	4980	10118	1.51%	0.202%
20	11.622	3279	3291	3314	rBV	227011	369048	54.96%	7.356%




Sum of corrected areas: 5017296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027686.D
Acq On : 01 Sep 2022 23:04
Operator : SY/MD
Sample : N4400-21DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

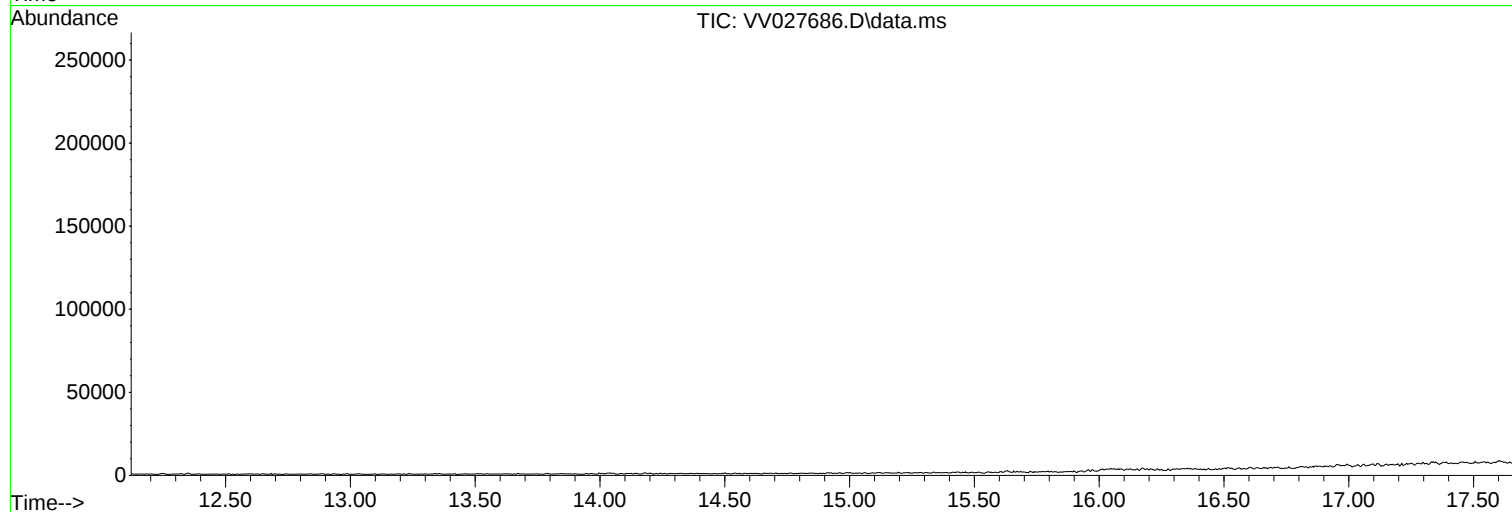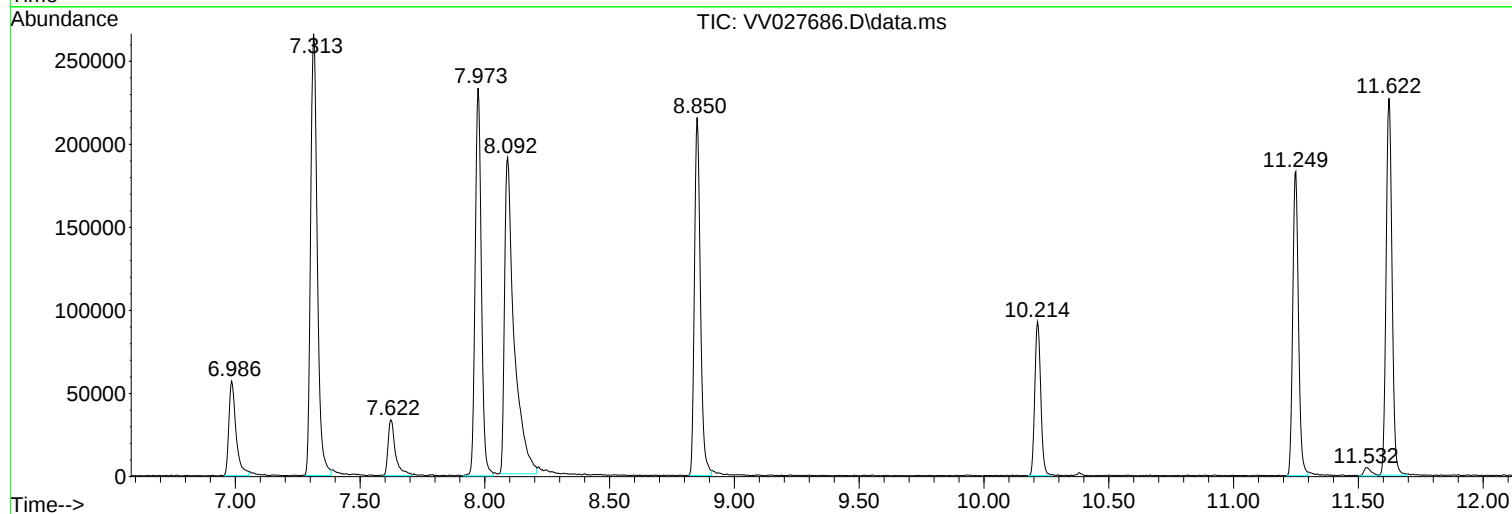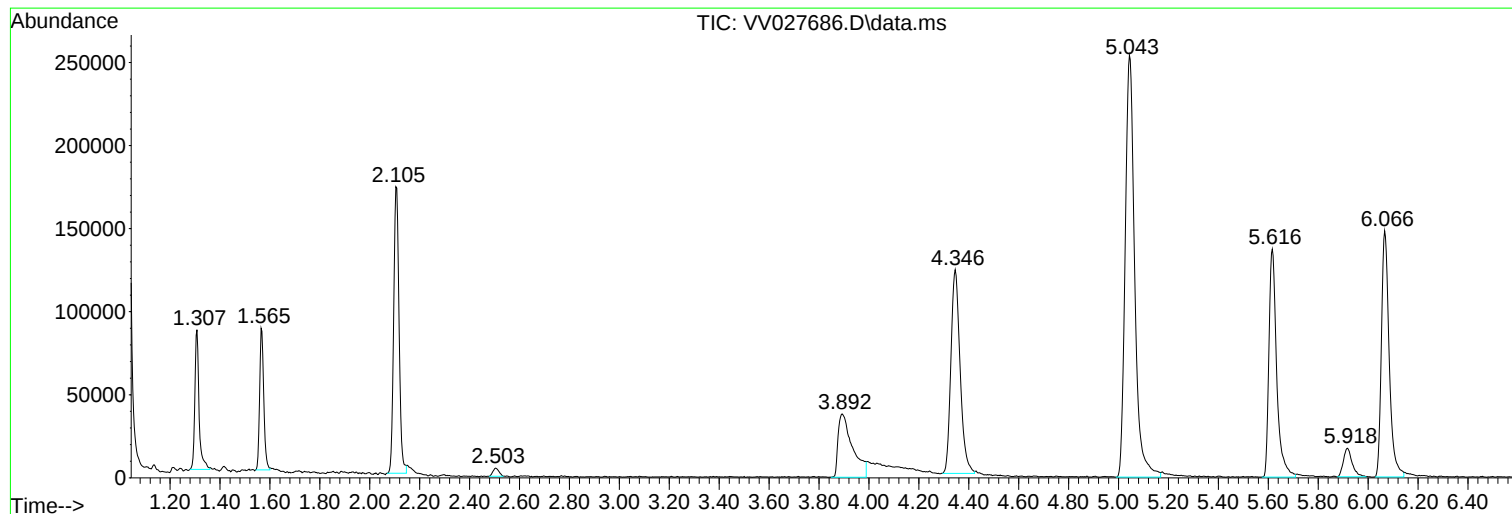

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027686.D
Acq On : 01 Sep 2022 23:04
Operator : SY/MD
Sample : N4400-21DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027686.D
Acq On : 01 Sep 2022 23:04
Operator : SY/MD
Sample : N4400-21DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc