

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027691.D
 Acq On : 02 Sep 2022 01:06
 Operator : SY/MD
 Sample : N4396-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	95	rBV	82263	97058	15.26%	2.204%
2	1.568	156	164	178	rBV	82026	96129	15.12%	2.183%
3	2.108	321	332	347	rBV	168145	242063	38.07%	5.497%
4	2.503	445	455	468	rBV2	17971	30542	4.80%	0.694%
5	2.577	468	478	490	rVB3	9702	17825	2.80%	0.405%
6	3.892	877	887	909	rBV	33903	113050	17.78%	2.567%
7	4.346	1013	1028	1049	rBV	118437	298205	46.90%	6.772%
8	5.043	1229	1245	1269	rBV2	249669	635845	100.00%	14.440%
9	5.616	1411	1423	1453	rBV	135969	288331	45.35%	6.548%
10	5.905	1502	1513	1536	rVB3	9276	21813	3.43%	0.495%
11	6.066	1550	1563	1584	rBV	147159	311573	49.00%	7.076%
12	6.985	1839	1849	1865	rBV2	55901	106712	16.78%	2.423%
13	7.313	1937	1951	1975	rBV	261611	466526	73.37%	10.595%
14	7.622	2036	2047	2069	rBV	31840	63670	10.01%	1.446%
15	8.091	2182	2193	2229	rBV3	185511	497073	78.18%	11.288%
16	8.850	2419	2429	2458	rBV	203948	346066	54.43%	7.859%
17	10.214	2840	2853	2871	rBV2	85976	140863	22.15%	3.199%
18	11.249	3164	3175	3194	rBV	174070	274450	43.16%	6.233%
19	11.622	3279	3291	3308	rBV	219309	355663	55.94%	8.077%




Sum of corrected areas: 4403457

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027691.D
Acq On : 02 Sep 2022 01:06
Operator : SY/MD
Sample : N4396-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

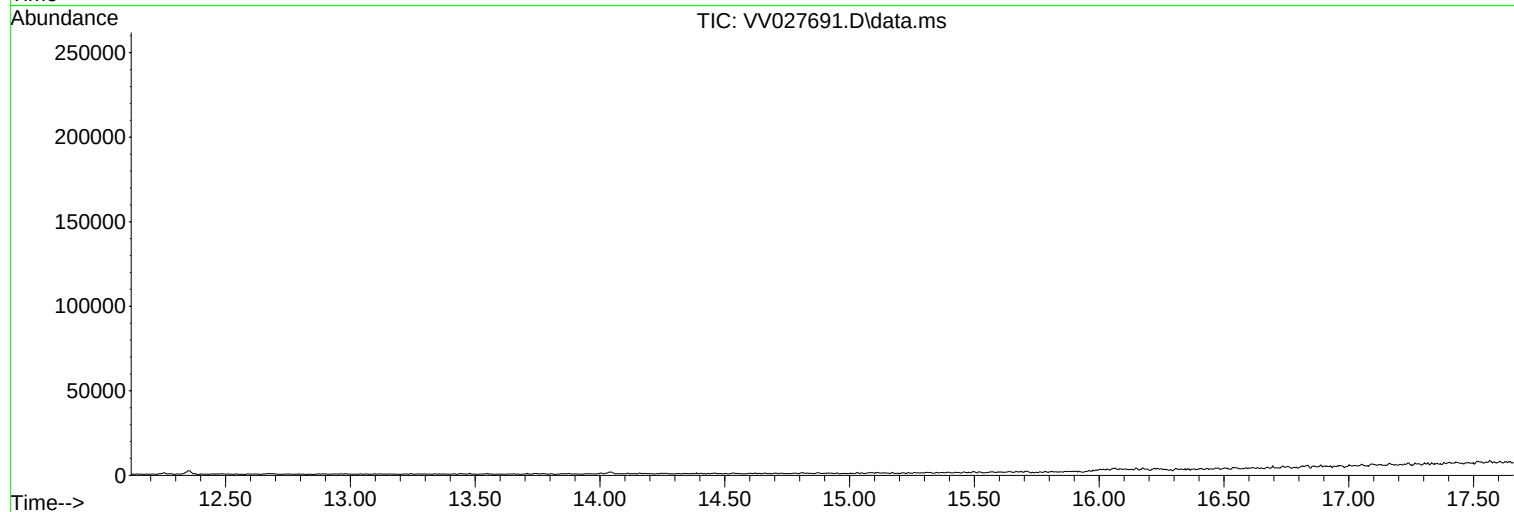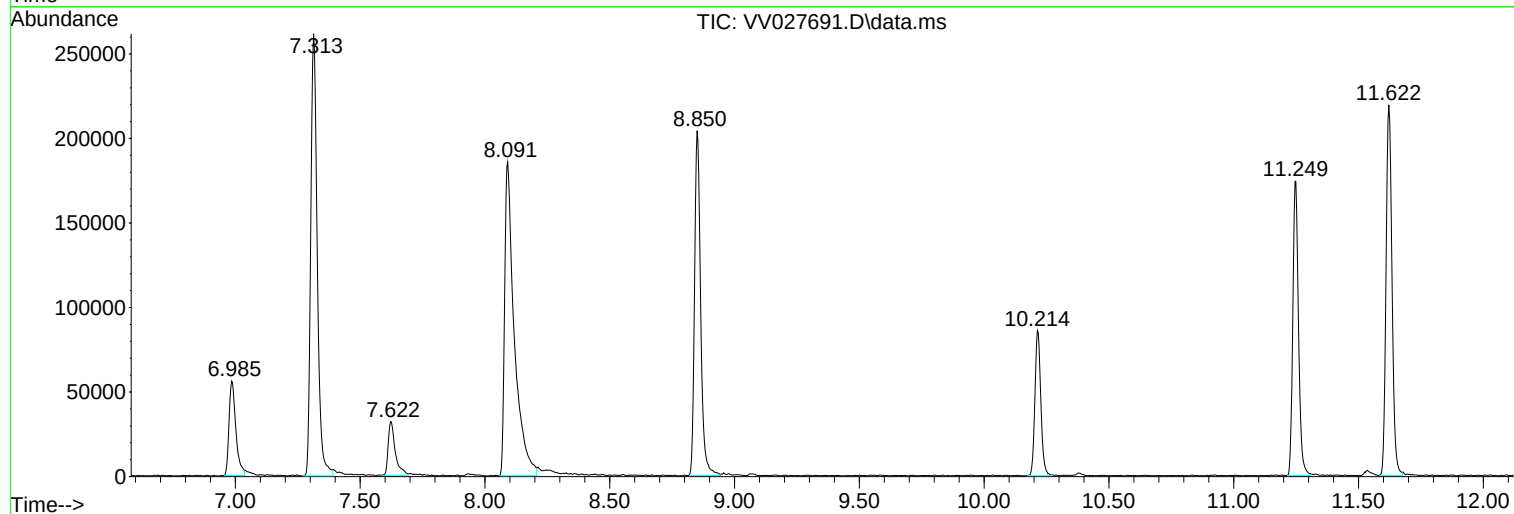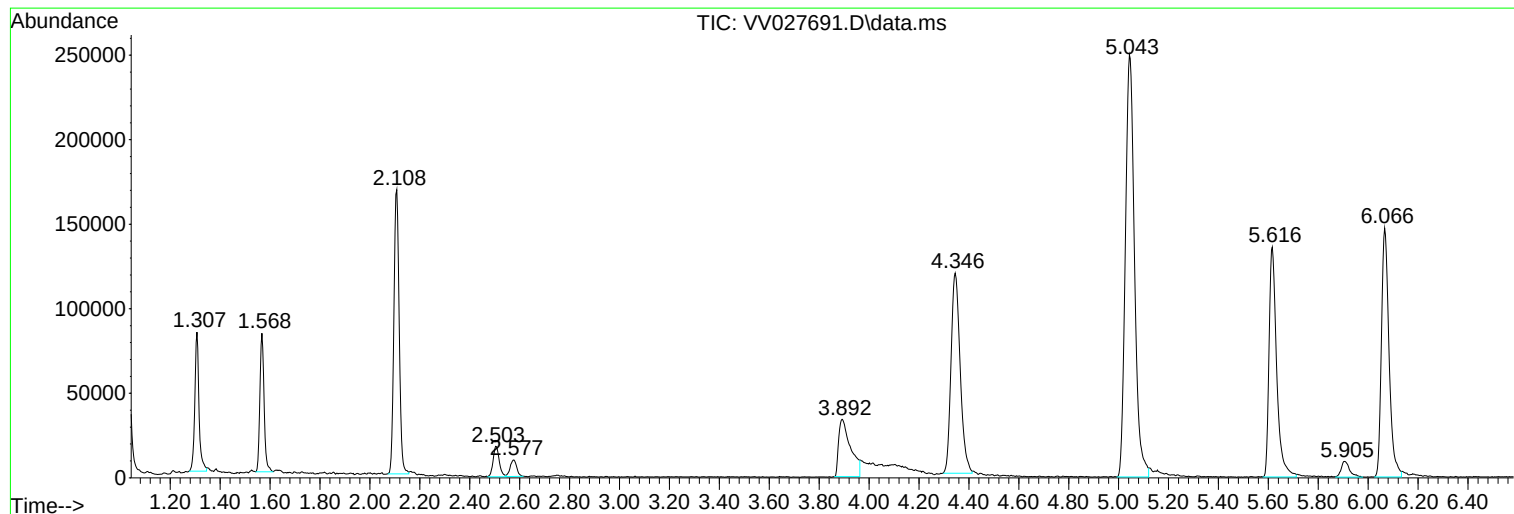

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027691.D
Acq On : 02 Sep 2022 01:06
Operator : SY/MD
Sample : N4396-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027691.D
Acq On : 02 Sep 2022 01:06
Operator : SY/MD
Sample : N4396-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc